

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041786.D
 Acq On : 11 Sep 2023 19:33
 Operator : MA/JU
 Sample : 04247-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJY1

Quant Time: Sep 12 04:27:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.984	152	4251	0.400	ng/u1	0.00
4) Naphthalene-d8	10.796	136	10201	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.624	164	4636	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.375	188	8501	0.400	ng/u1	0.00
17) Chrysene-d12	21.545	240	3327	0.400	ng/u1	0.00
23) Perylene-d12	23.965	264	4079	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	27333	4.207	ng/u1	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	4300	0.327	ng/u1	0.00
18) Fluoranthene-d10	19.394	212	5995	0.372	ng/u1	0.00
Target Compounds						
14) Pentachlorophenol	16.999	266	171	0.050	ng/u1	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041786.D
Acq On : 11 Sep 2023 19:33
Operator : MA/JU
Sample : 04247-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJY1

Quant Time: Sep 12 04:27:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

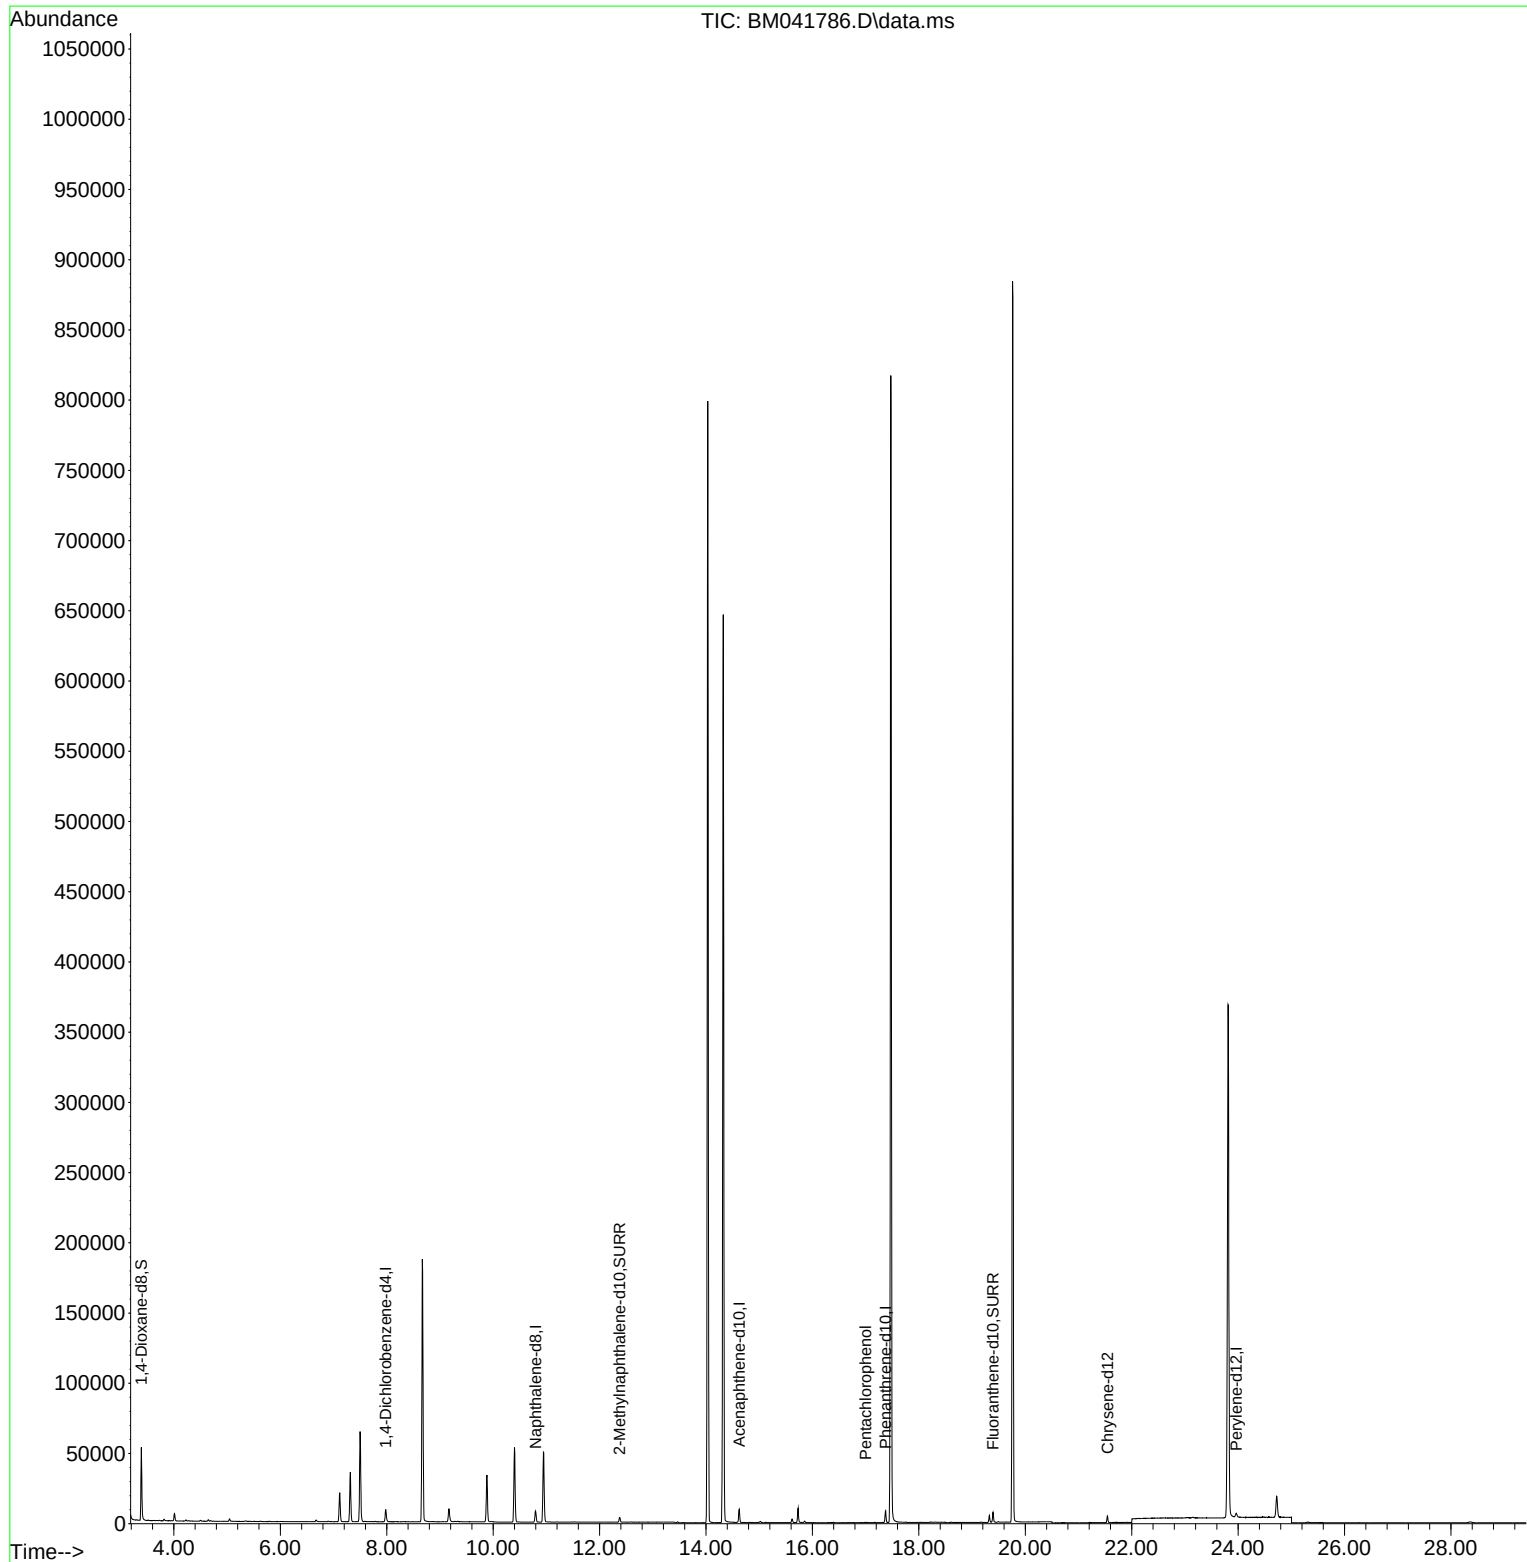

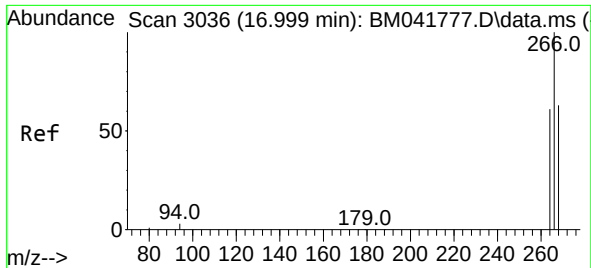

#14
 Pentachlorophenol
 Concen: 0.050 ng/ul
 RT: 16.999 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM041786.D
 Acq: 11 Sep 2023 19:33

Instrument :
 BNA_M
 ClientSampleId :
 BBJY1

Tgt Ion:	266	Resp:	171
Ion	Ratio	Lower	Upper
266	100		
264	56.1	50.0	75.0
268	63.2	50.8	76.2

