

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
 Data File : BM041788.D
 Acq On : 11 Sep 2023 20:47
 Operator : MA/JU
 Sample : 04247-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJ77

Quant Time: Sep 12 04:27:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 09 23:26:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.979	152	3667	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.796	136	8816	0.400	ng/u1	-0.01
9) Acenaphthene-d10	14.620	164	4377	0.400	ng/u1	-0.01
13) Phenanthrene-d10	17.371	188	7478	0.400	ng/u1	-0.01
17) Chrysene-d12	21.542	240	2971	0.400	ng/u1	0.00
23) Perylene-d12	23.962	264	3766	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.389	96	28128	5.019	ng/u1	-0.01
6) 2-Methylnaphthalene-d10	12.379	152	4055	0.357	ng/u1	0.00
18) Fluoranthene-d10	19.394	212	5470	0.380	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.423	88	22019	3.782	ng/u1	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091123\
Data File : BM041788.D
Acq On : 11 Sep 2023 20:47
Operator : MA/JU
Sample : 04247-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJ77


Quant Time: Sep 12 04:27:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM090523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 09 23:26:58 2023
Response via : Initial Calibration

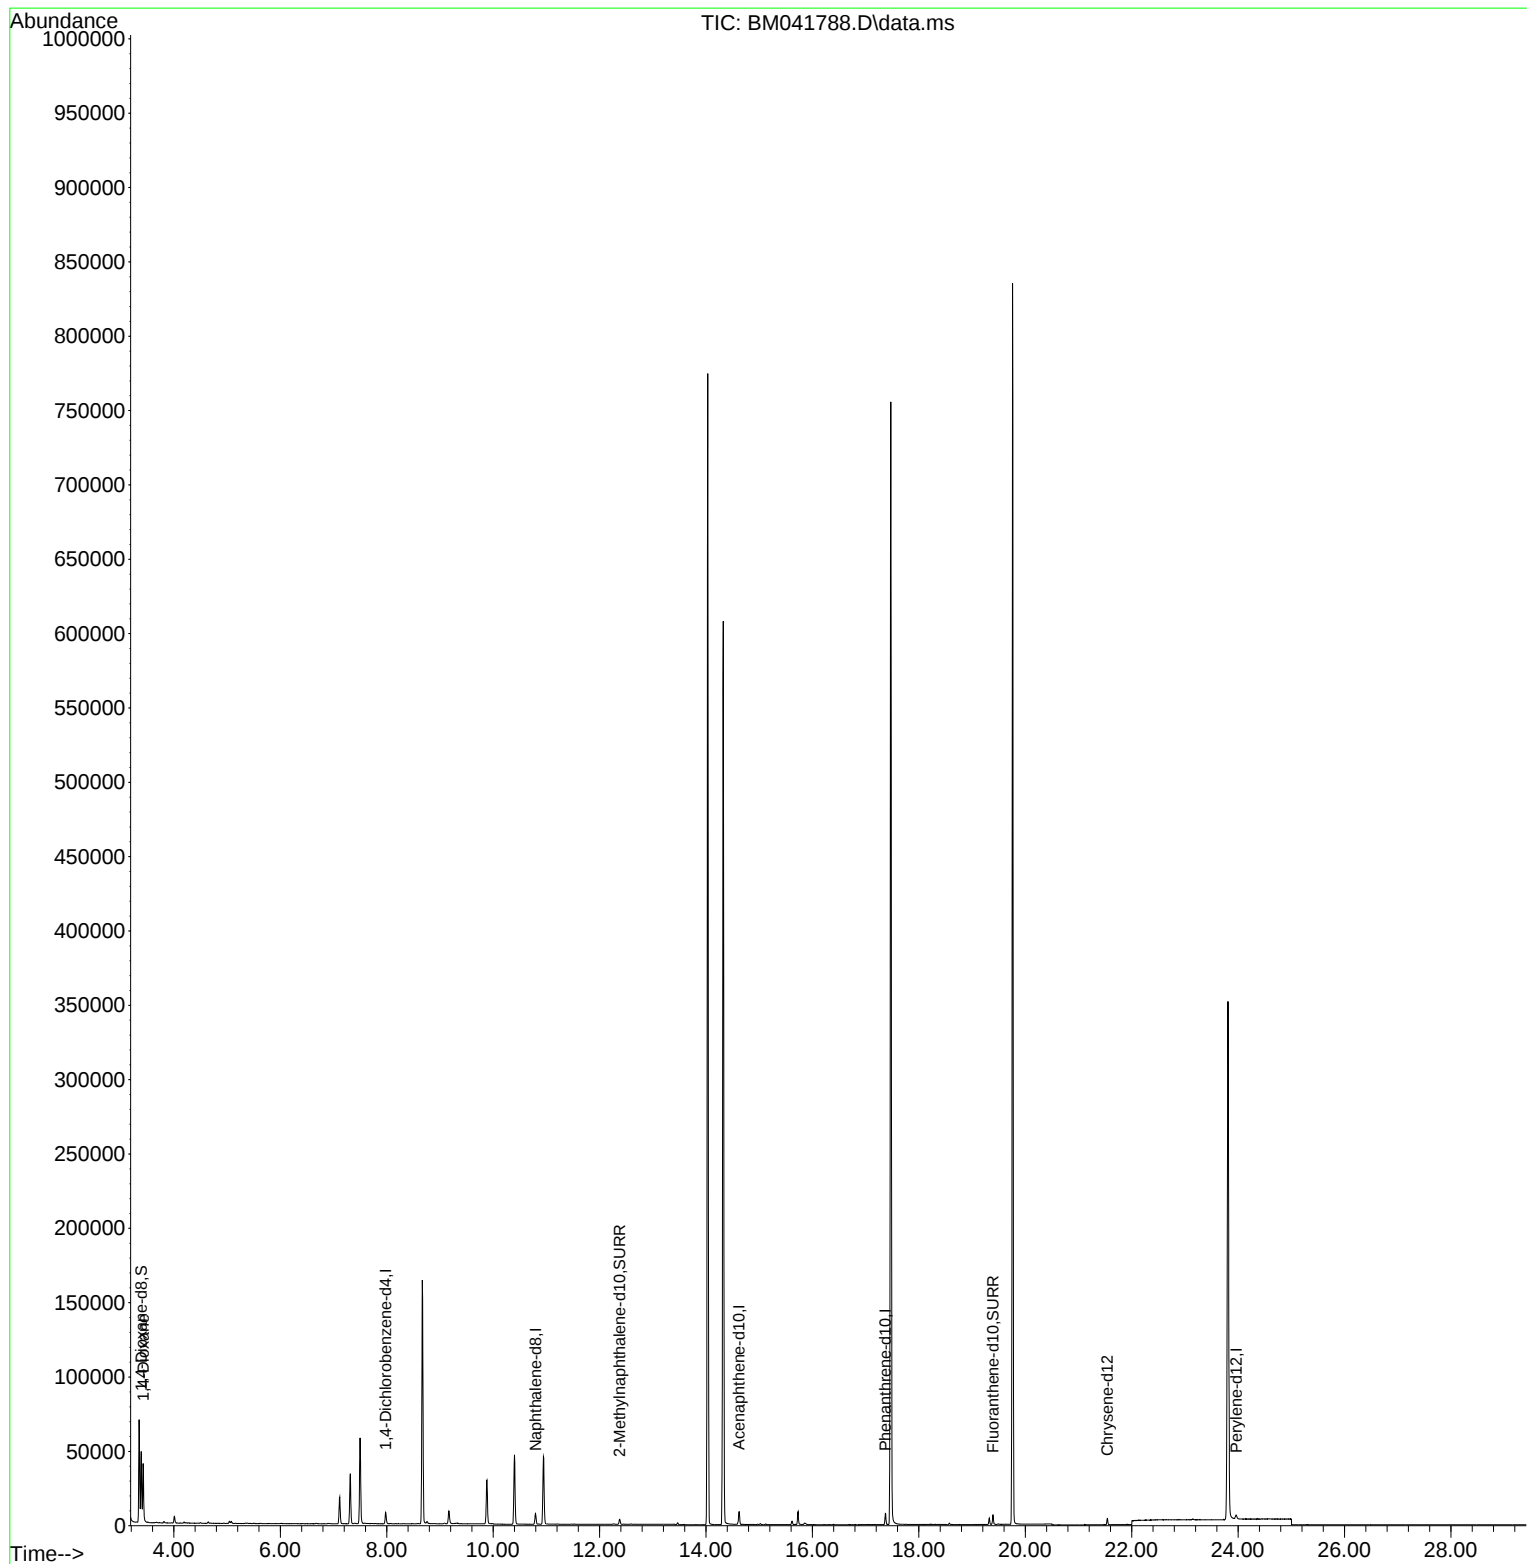

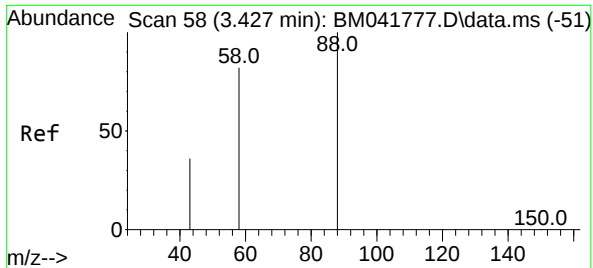

#2
 1,4-Dioxane
 Concen: 3.782 ng/ul
 RT: 3.423 min Scan# 51
 Delta R.T. -0.012 min
 Lab File: BM041788.D
 Acq: 11 Sep 2023 20:47

Instrument :
 BNA_M
 ClientSampleId :
 BBJ77

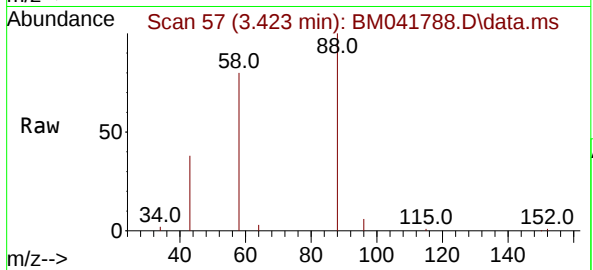

Tgt Ion:	88	Resp:	22019
Ion	Ratio	Lower	Upper
88	100		
43	37.7	33.8	50.6
58	79.9	54.2	81.2

