

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091219\
 Data File : BM022668.D
 Acq On : 12 Sep 2019 15:33
 Operator : HP/JU
 Sample : K4706-03DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF569DL

Quant Time: Sep 12 16:50:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 10 15:06:45 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	10872	0.40	ng/ul	0.00
2) Naphthalene-d8	10.64	136	45268	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	24534	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	58495	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	46937	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	44522	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.23	152	4044	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	9896	0.06	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.69	128	11928	0.092	ng/ul	98
5) 2-Methylnaphthalene	12.30	142	2487	0.028	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091219\
Data File : BM022668.D
Acq On : 12 Sep 2019 15:33
Operator : HP/JU
Sample : K4706-03DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF569DL

Quant Time: Sep 12 16:50:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM091019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 15:06:45 2019
Response via : Initial Calibration

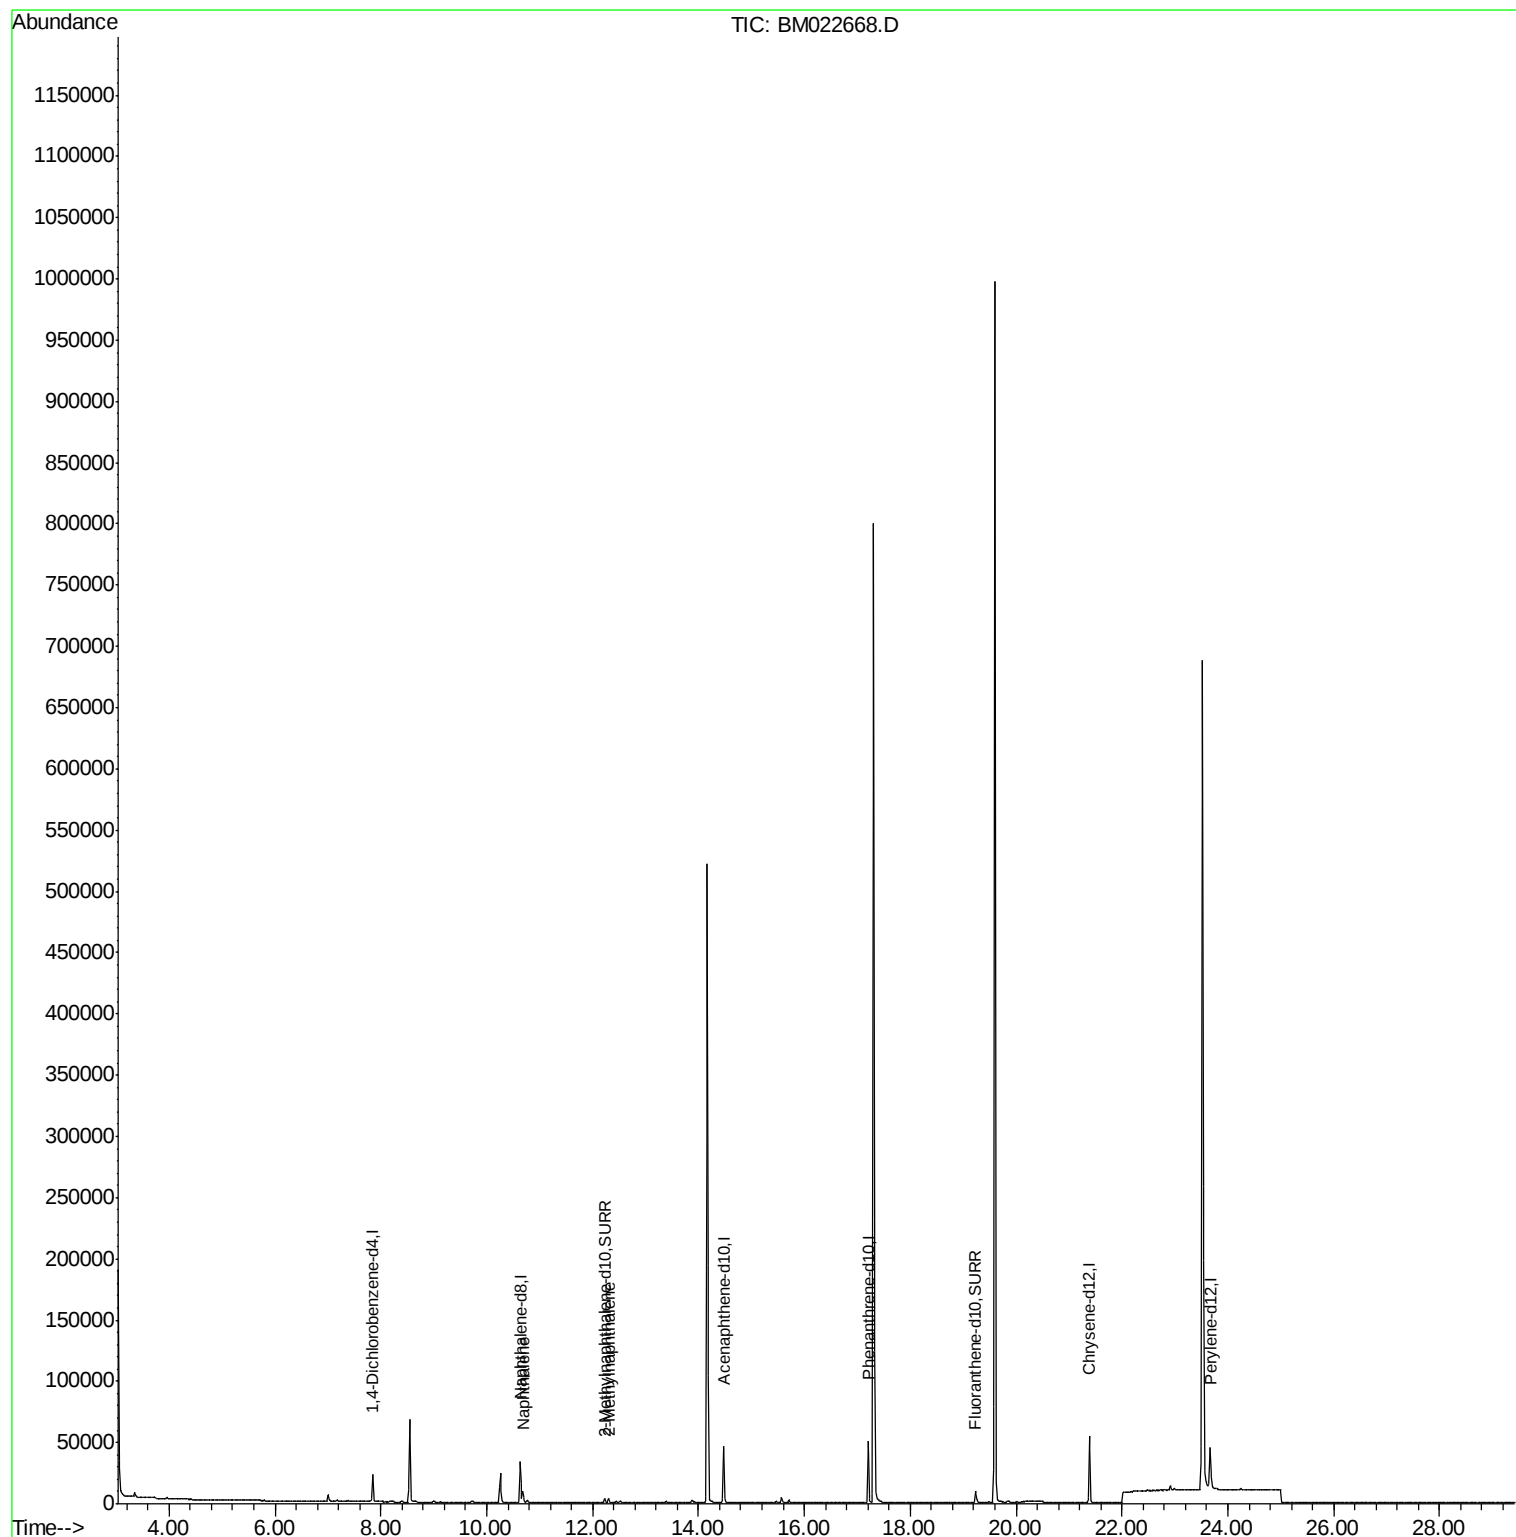

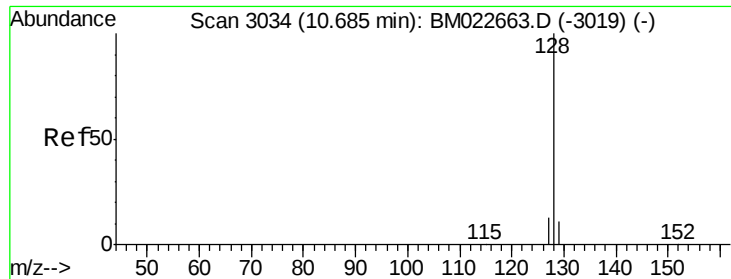

#3

Naphthalene

Concen: 0.092 ng/ul

RT: 10.69 min Scan# 3034

Delta R.T. -0.00 min

Lab File: BM022668.D

Acq: 12 Sep 2019 15:33

Instrument :

BNA_M

ClientSampleId :

BF569DL


Tot Ion:128 Resp: 11928

Ion Ratio Lower Upper

128 100

129 12.5 8.8 13.2




127 13.5 10.4 15.6

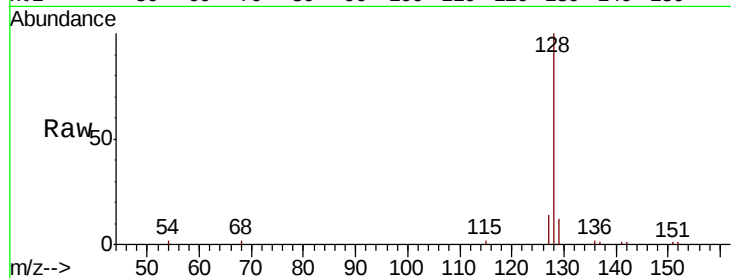

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

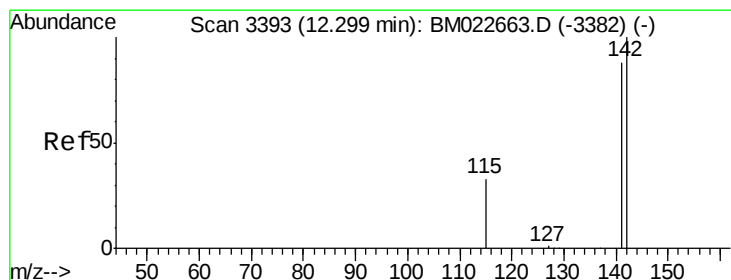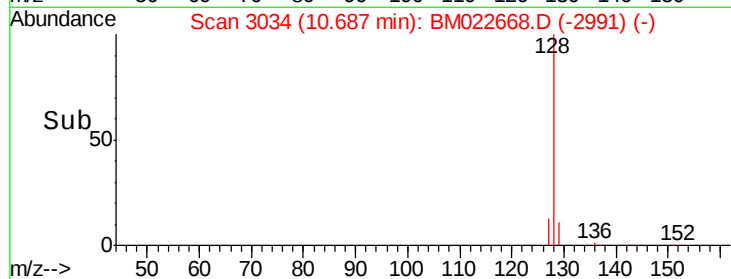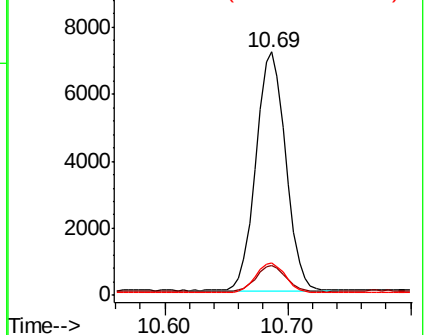

#5

2-Methylnaphthalene

Concen: 0.028 ng/ul

RT: 12.30 min Scan# 3393

Delta R.T. -0.00 min

Lab File: BM022668.D


Acq: 12 Sep 2019 15:33

Tgt Ion:142 Resp: 2487

Ion Ratio Lower Upper

142 100

141 88.3 70.8 106.2

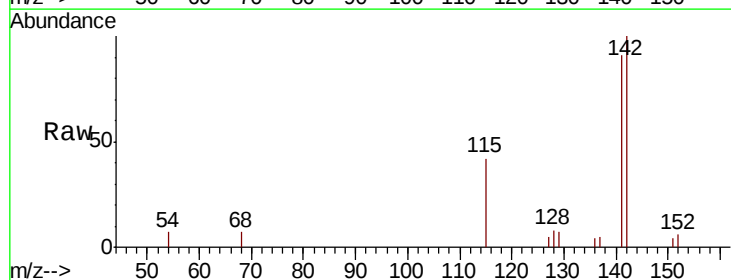

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

