

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091319\
 Data File : BM022679.D
 Acq On : 13 Sep 2019 16:35
 Operator : HP/JU
 Sample : K4706-02DL2 100X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 14 00:42:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 09 07:45:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	202335	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.63	136	888613	20.00	ng/ul	-0.02
36) Acenaphthene-d10	14.47	164	565093	20.00	ng/ul	-0.01
62) Phenanthrene-d10	17.21	188	1212779	20.00	ng/ul	-0.01
78) Chrysene-d12	21.39	240	1176039	20.00	ng/ul	-0.01
86) Perylene-d12	23.66	264	1218108	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.00	99	908	0.05	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.17	67	2414	0.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	2398	0.16	ng/ul	-0.01
13) 4-Methylphenol-d8	8.54	113	1483	0.10	ng/ul	-0.02
19) Nitrobenzene-d5	8.99	128	1823	0.28	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.72	143	987	0.17	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.25	165	2186	0.15	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.76	131	660	0.03	ng/ul	-0.02
44) Dimethylphthalate-d6	13.88	166	13088	0.29	ng/ul	-0.01
47) Acenaphthylene-d8	14.16	160	12165	0.22	ng/ul	-0.02
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.46	176	11729	0.31	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.57	200	563	0.10	ng/ul	-0.02
71) Anthracene-d10	17.30	188	22086	0.36	ng/ul	-0.02
79) Pyrene-d10	19.59	212	18040	0.28	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.51	264	14959	0.23	ng/ul	-0.02

Target Compounds


				Ovalue	
28) Naphthalene	10.68	128	1403317	28.484	ng/ul 99
30) 4-Chloroaniline	10.68	127	180263	8.851	ng/ul# 6
34) 2-Methylnaphthalene	12.29	142	184337	4.966	ng/ul 99
35) 1-Methylnaphthalene	12.52	142	96450	2.720	ng/ul 99
50) Acenaphthene	14.53	153	41250	1.047	ng/ul 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091319\
Data File : BM022679.D
Acq On : 13 Sep 2019 16:35
Operator : HP/JU
Sample : K4706-02DL2 100X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 14 00:42:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090519MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 09 07:45:00 2019
Response via : Initial Calibration




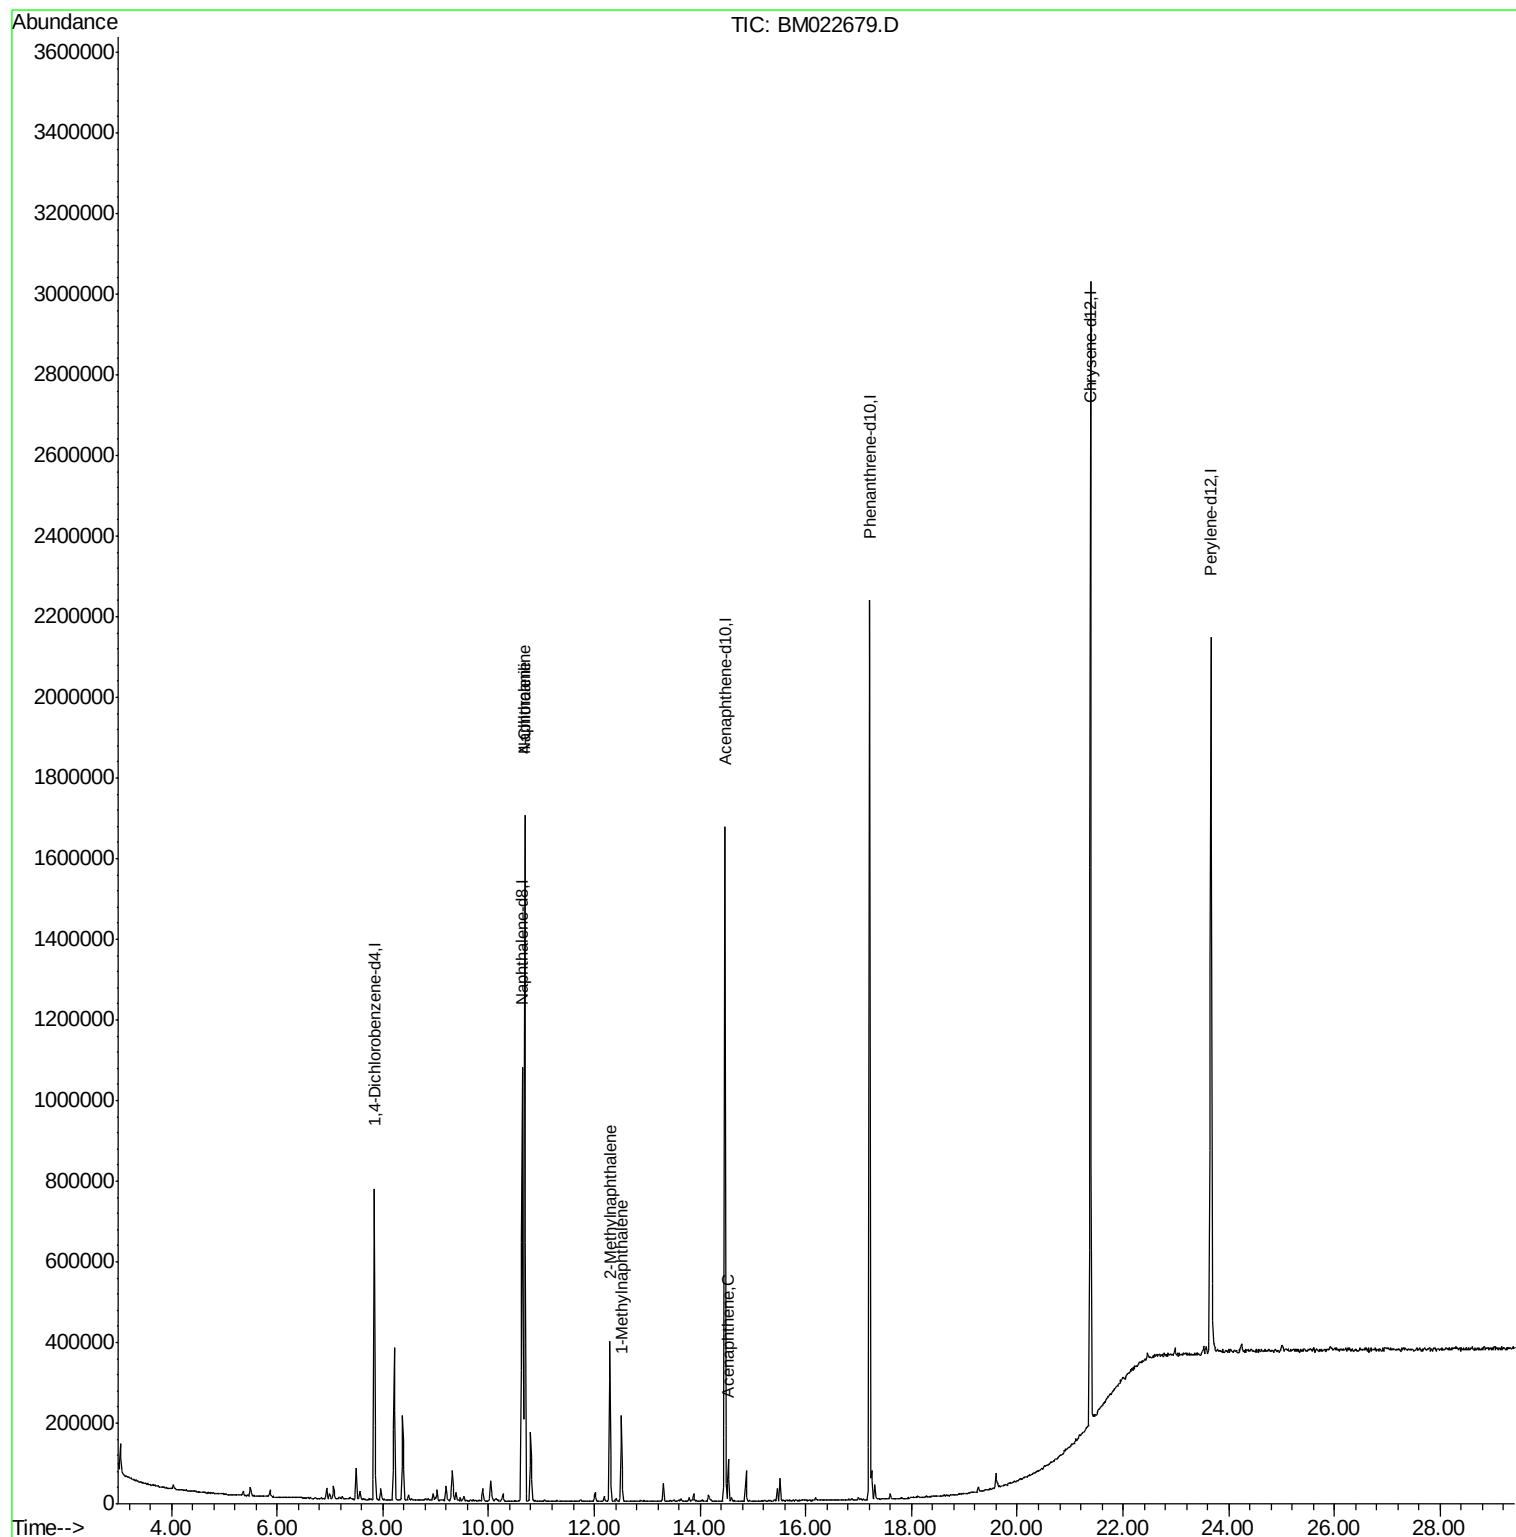


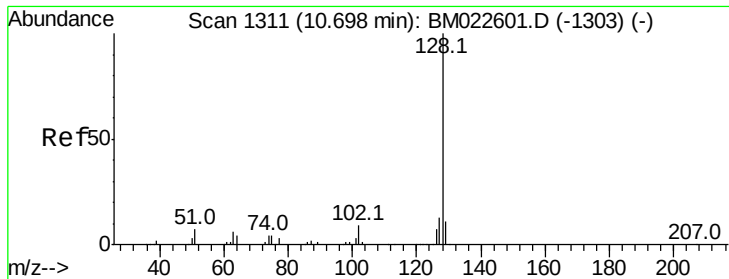

#28
Naphthalene
Concen: 28.484 ng/ul
RT: 10.68 min Scan# 1308
Delta R.T. -0.02 min
Lab File: BM022679.D
Acq: 13 Sep 2019 16:35




Instrument :
BNA_M
ClientSampled :


Tot Ion:128 Resp: 1403317
Ion Ratio Lower Upper
128 100
129 10.9 8.9 13.3
127 13.0 10.6 16.0

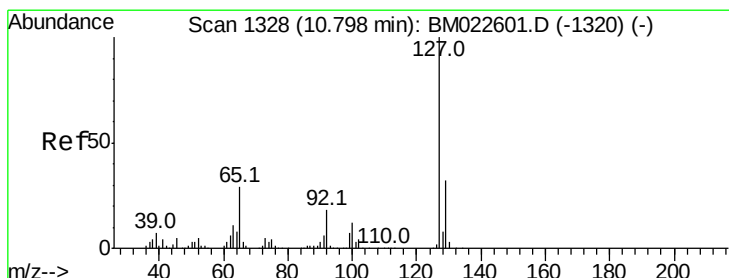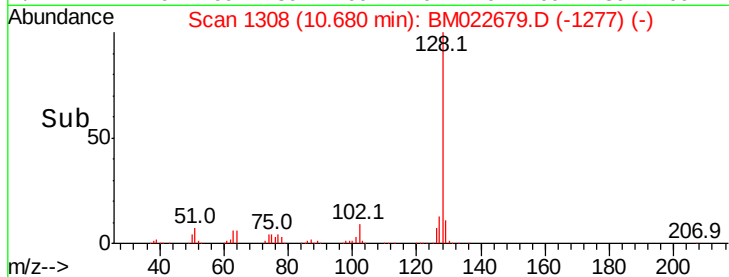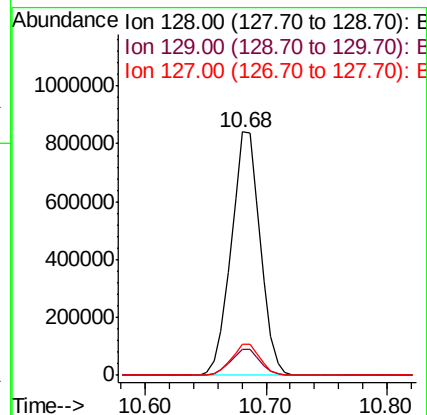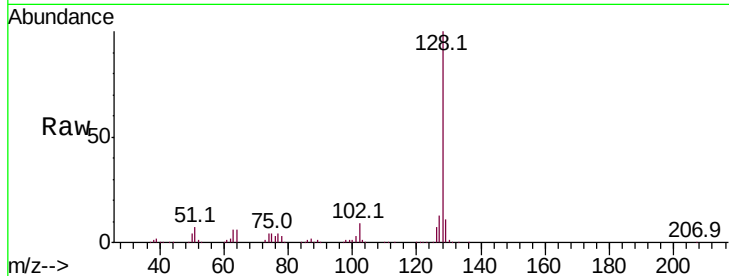

#30
4-Chloroaniline
Concen: 8.851 ng/ul
RT: 10.68 min Scan# 1308
Delta R.T. -0.12 min
Lab File: BM022679.D
Acq: 13 Sep 2019 16:35

Tgt Ion:127 Resp: 180263
Ion Ratio Lower Upper
127 100
129 84.0 25.4 38.2#

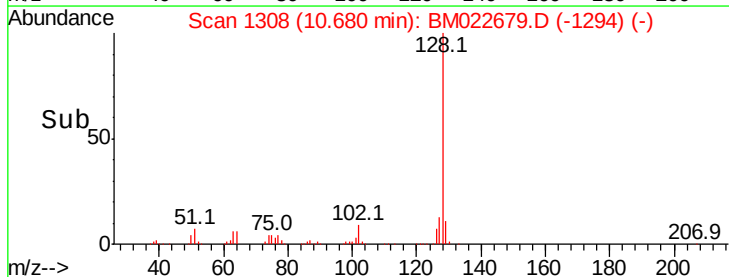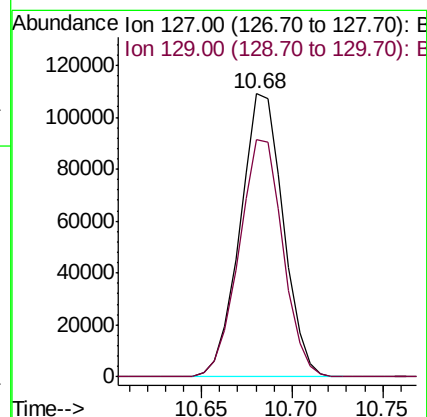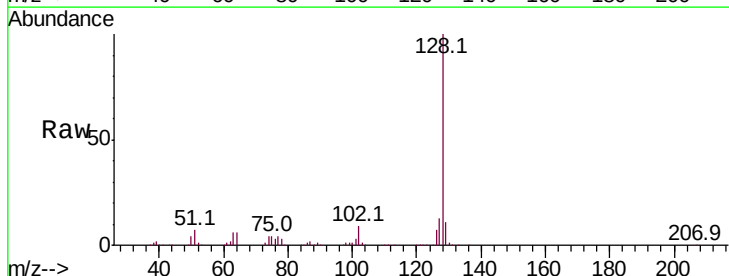

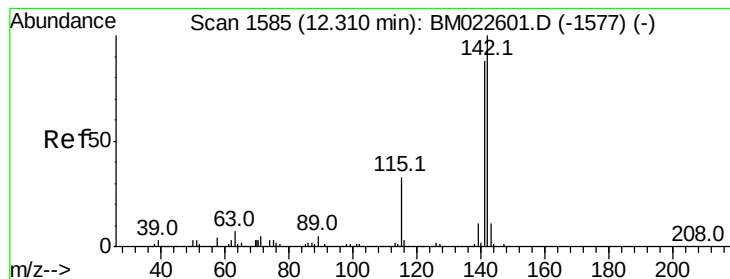

#34

2-Methylnaphthalene

Concen: 4.966 ng/ul

RT: 12.29 min Scan# 1582

Delta R.T. -0.02 min

Lab File: BM022679.D

Acq: 13 Sep 2019 16:35

Instrument :

BNA_M


ClientSampleId :

Tot Ion:142 Resp: 184337

Ion Ratio Lower Upper

142 100

141 89.3 71.0 106.4

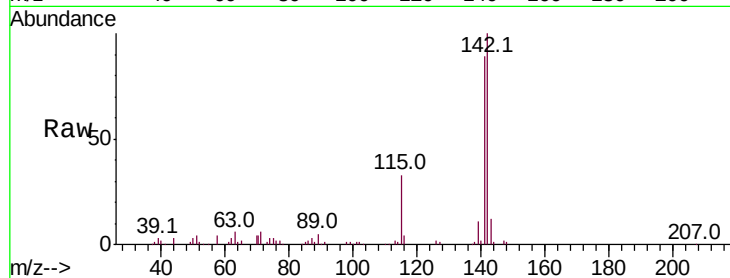

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E



12.29

100000

50000

0

Time-->

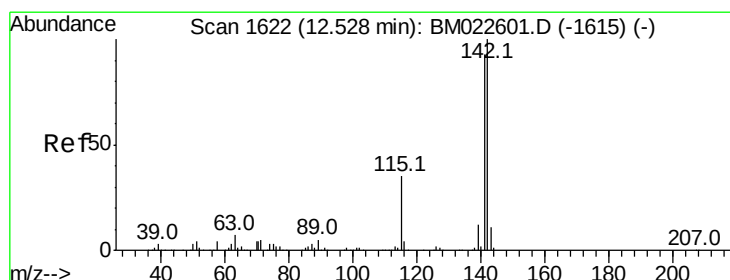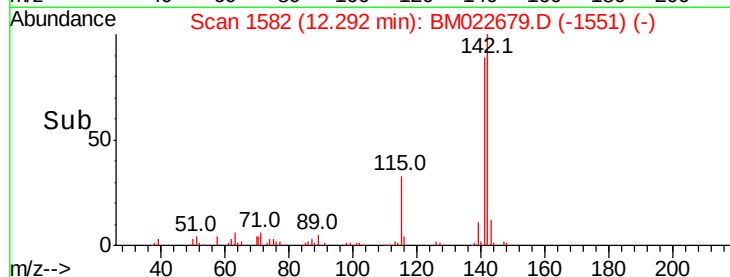

#35

1-Methylnaphthalene

Concen: 2.720 ng/ul

RT: 12.52 min Scan# 1620

Delta R.T. -0.02 min

Lab File: BM022679.D

Acq: 13 Sep 2019 16:35


Tgt Ion:142 Resp: 96450

Ion Ratio Lower Upper

142 100

141 89.4 72.6 108.8

116 3.5 3.0 4.4

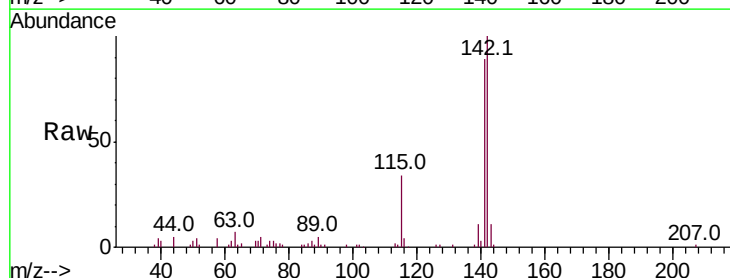

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

12.52

80000


60000


40000

20000

0

Time-->

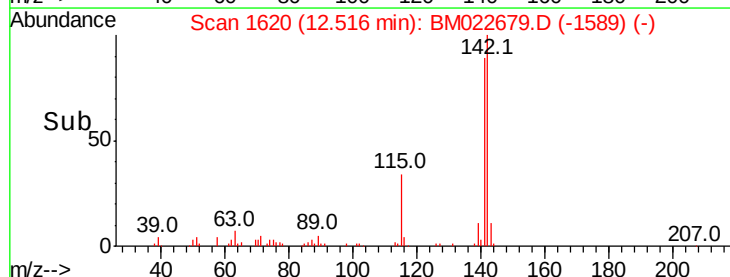

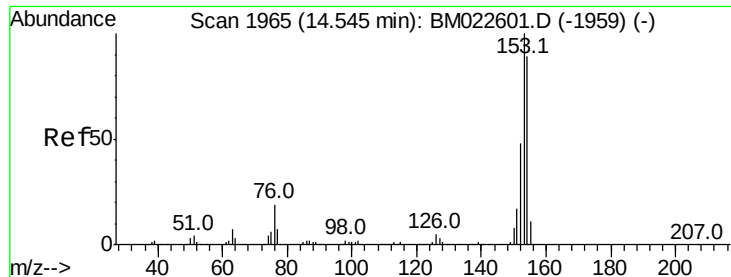

#50

Acenaphthene

Concen: 1.047 ng/ul

RT: 14.53 min Scan# 1963

Delta R.T. -0.02 min

Lab File: BM022679.D

Acq: 13 Sep 2019 16:35

Instrument :

BNA_M

ClientSampleId :


Tot Ion:153 Resp: 41250

Ion Ratio Lower Upper

153 100

152 49.6 37.5 56.3

154 85.8 71.4 107.0

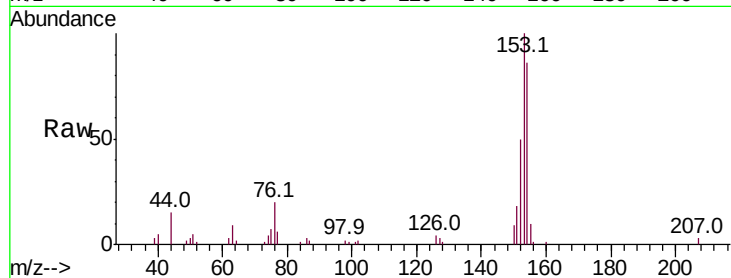

Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

