

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041840.D
 Acq On : 13 Sep 2023 21:14
 Operator : MA/JU
 Sample : 04324-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJG0

Quant Time: Sep 14 03:38:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	6295	0.400	ng/ul	0.00
4) Naphthalene-d8	10.785	136	16580	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.615	164	8575	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.367	188	17620	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	9197	0.400	ng/ul	0.00
23) Perylene-d12	23.953	264	10947	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	20342	2.541	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	6477	0.287	ng/ul	0.00
18) Fluoranthene-d10	19.385	212	13342	0.423	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.414	88	14145	1.683	ng/ul#	67
12) Fluorene	15.610	166	3372	0.070	ng/ul#	13
20) Pyrene	19.757	202	3791	0.051	ng/ul#	1
24) Benzo(b)fluoranthene	23.208	252	1974	0.025	ng/ul#	22
26) Benzo(a)pyrene	23.804	252	7229	0.122	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
Data File : BM041840.D
Acq On : 13 Sep 2023 21:14
Operator : MA/JU
Sample : 04324-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJG0

Quant Time: Sep 14 03:38:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 16:15:23 2023
Response via : Initial Calibration




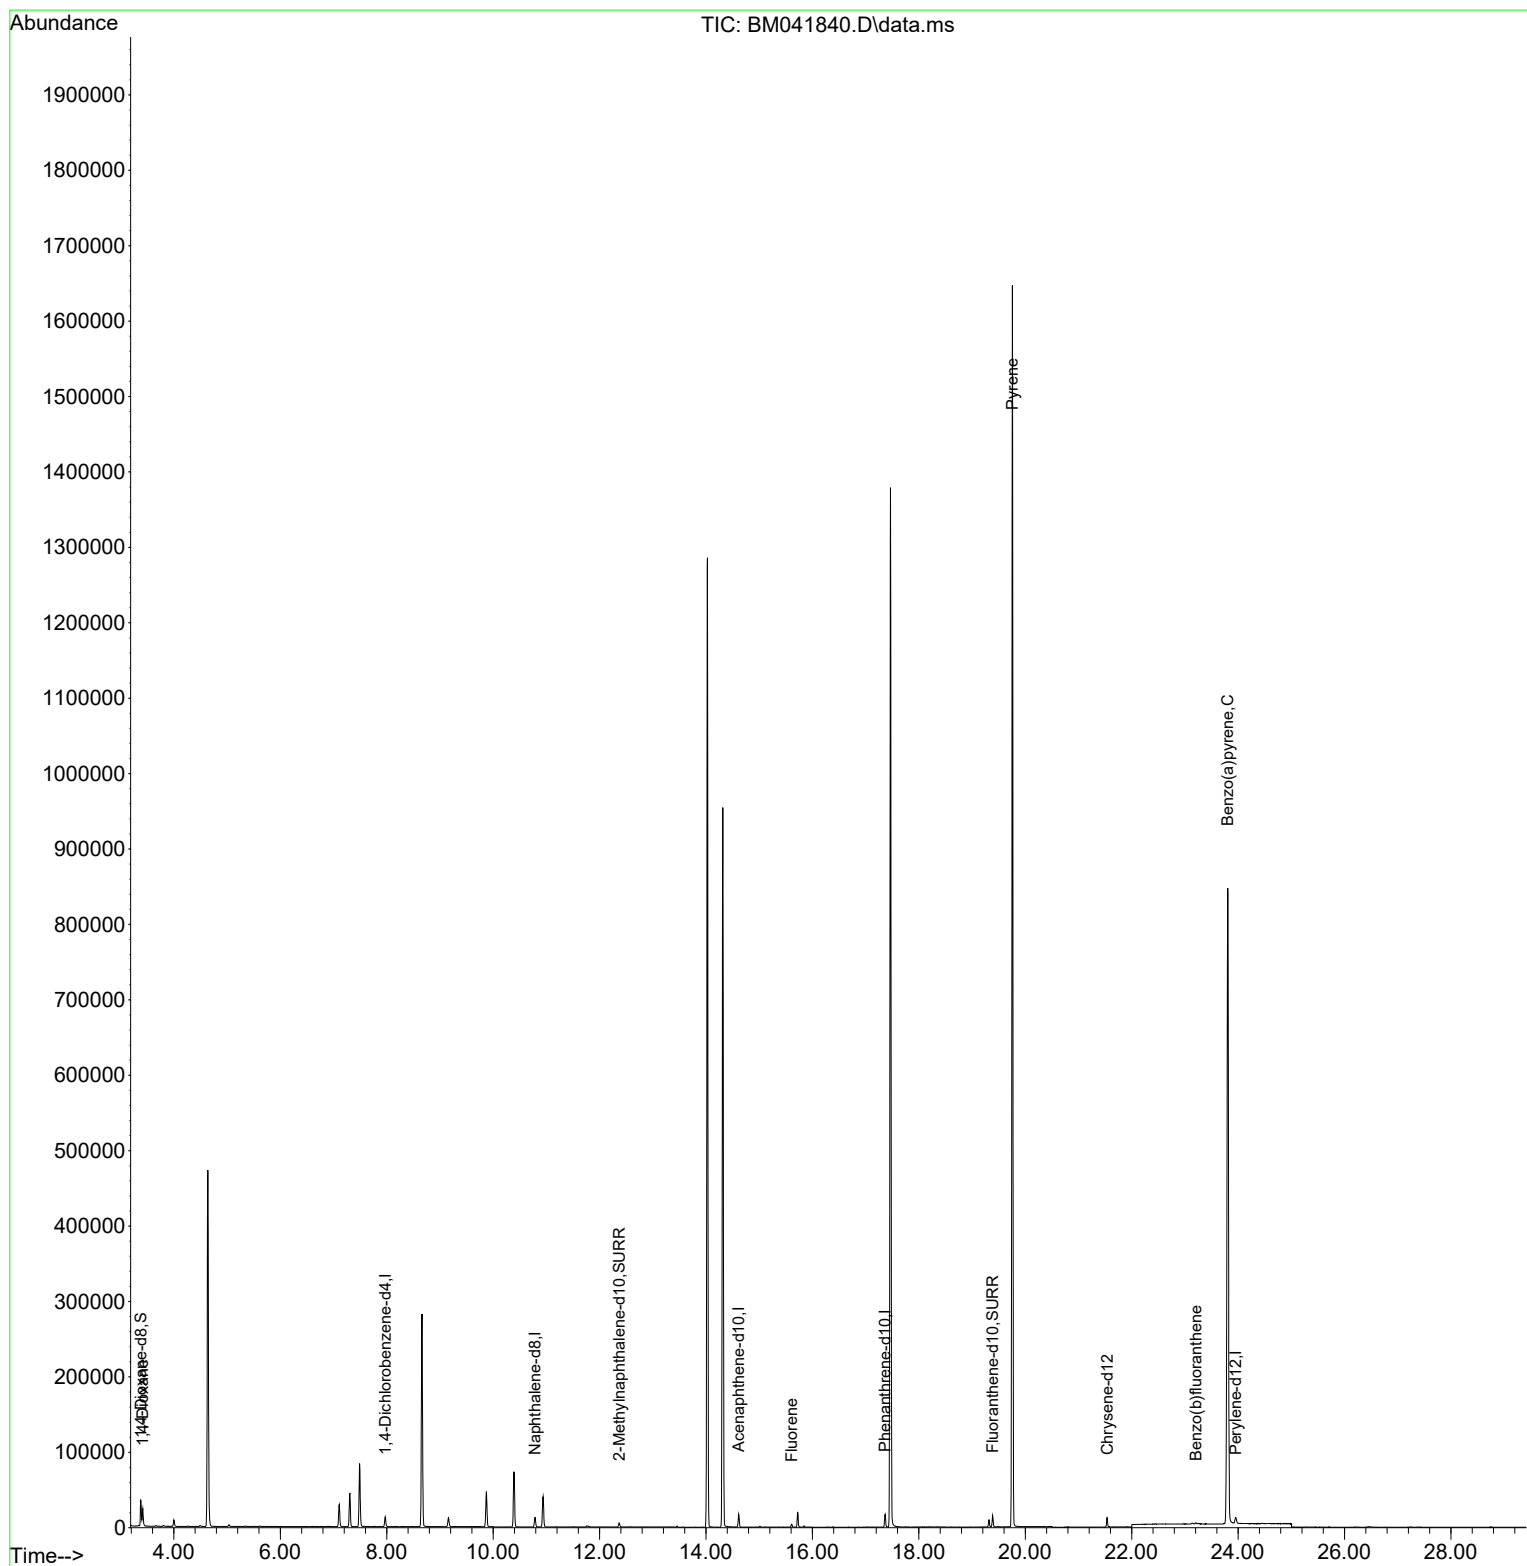


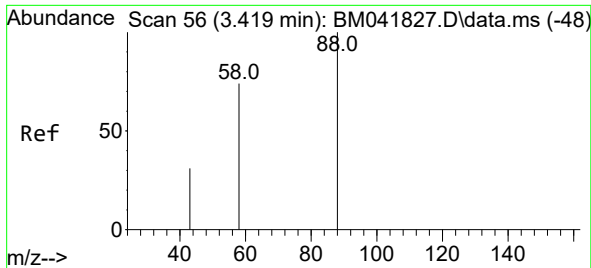

#2
1,4-Dioxane
Concen: 1.683 ng/ul
RT: 3.414 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM041840.D
Acq: 13 Sep 2023 21:14




Instrument :
BNA_M
ClientSampleId :
BBJG0


Tgt Ion: 88 Resp: 14145
Ion Ratio Lower Upper
88 100
43 38.1 69.9 104.9#
58 76.6 55.6 83.4

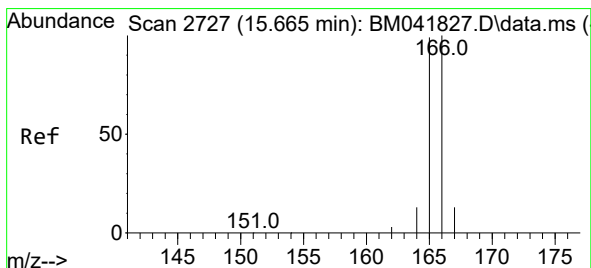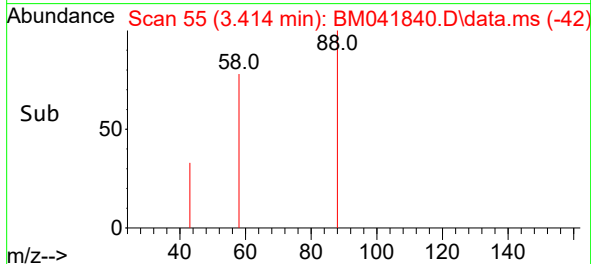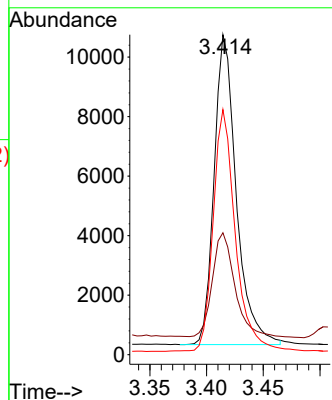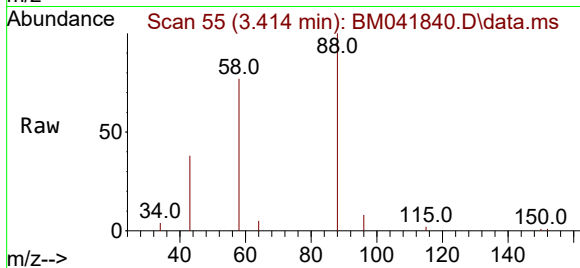

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.610 min Scan# 2715
Delta R.T. -0.056 min
Lab File: BM041840.D
Acq: 13 Sep 2023 21:14

Tgt Ion: 166 Resp: 3372
Ion Ratio Lower Upper
166 100
165 7.5 79.3 118.9#
167 33.6 11.2 16.8#


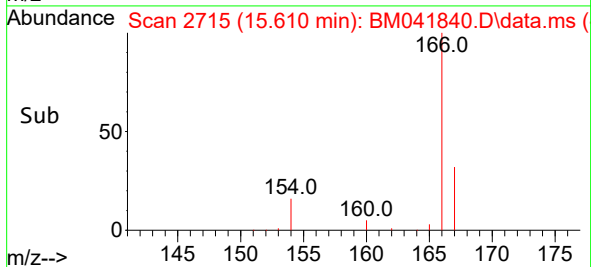
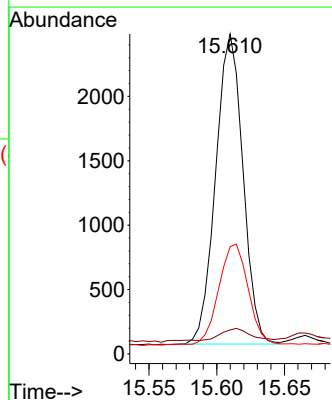
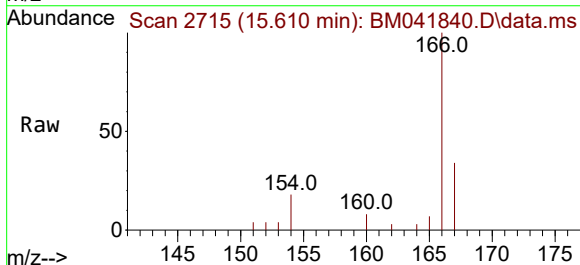


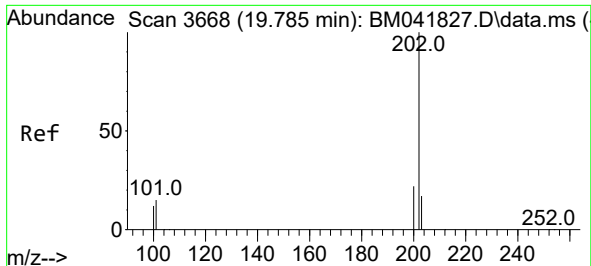

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.757 min Scan# 3662
Delta R.T. -0.028 min
Lab File: BM041840.D
Acq: 13 Sep 2023 21:14




Instrument :
BNA_M
ClientSampleId :
BBJG0


Tgt Ion:202 Resp: 3791
Ion Ratio Lower Upper
202 100
101 173.5 12.6 19.0#
100 1334.4 9.9 14.9#

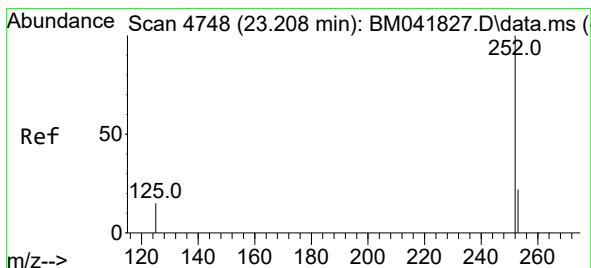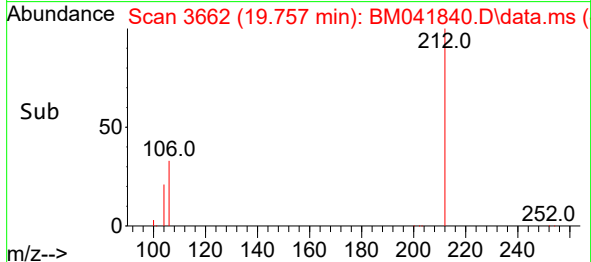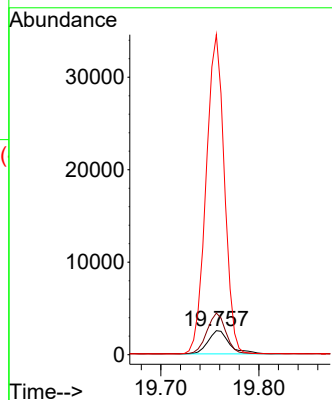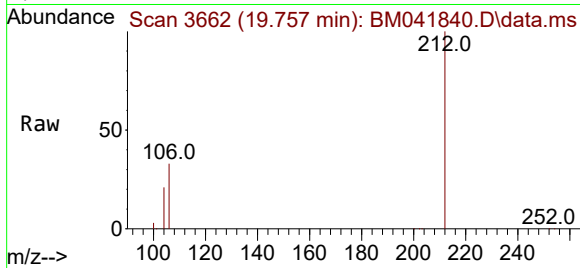

#24
Benzo(b)fluoranthene
Concen: 0.025 ng/ul
RT: 23.208 min Scan# 4748
Delta R.T. -0.000 min
Lab File: BM041840.D
Acq: 13 Sep 2023 21:14

Tgt Ion:252 Resp: 1974
Ion Ratio Lower Upper
252 100
253 56.5 0.0 51.0#
125 65.1 0.0 39.8#

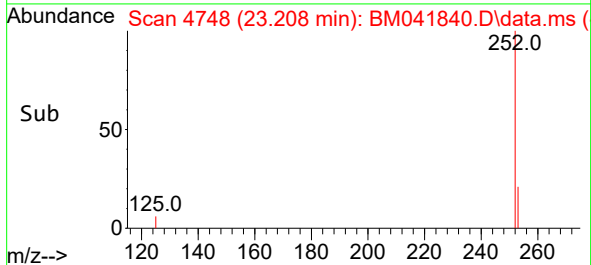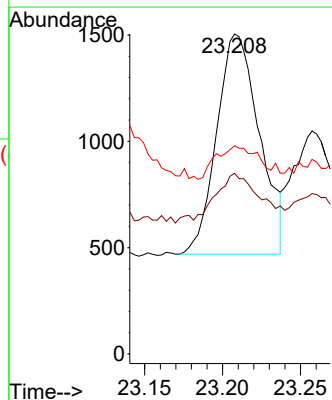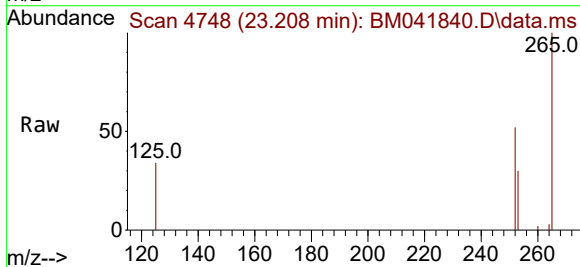

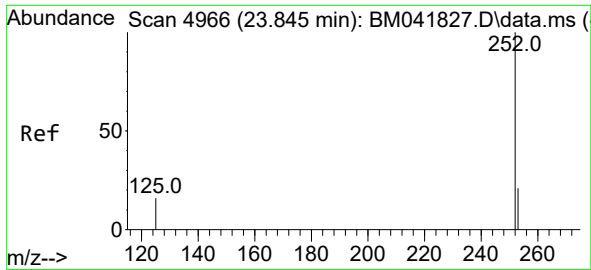

#26

Benzo(a)pyrene

Concen: 0.122 ng/ul

RT: 23.804 min Scan# 49

Delta R.T. -0.041 min

Lab File: BM041840.D


Acq: 13 Sep 2023 21:14

Instrument :

BNA_M

ClientSampleId :

BBJG0

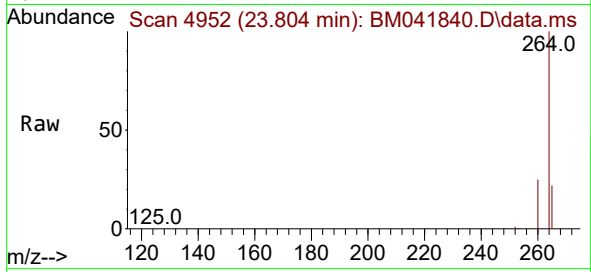

Tgt Ion:252 Resp: 7229

Ion Ratio Lower Upper

252 100

253 42.1 21.8 32.8#

125 40.3 18.8 28.2#

