

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041870.D
 Acq On : 14 Sep 2023 18:48
 Operator : MA/JU
 Sample : PB155434 BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK434

Quant Time: Sep 15 00:30:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	6068	0.400	ng/ul	0.00
4) Naphthalene-d8	10.790	136	16469	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.620	164	8866	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.371	188	20433	0.400	ng/ul	0.00
17) Chrysene-d12	21.545	240	12263	0.400	ng/ul	0.00
23) Perylene-d12	23.971	264	10623	0.400	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	43255	5.604	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.374	152	7785	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.394	212	15954	0.379	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.614	166	3304	0.066	ng/ul#	15
20) Pyrene	19.766	202	3129	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.819	252	4259	0.074	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
Data File : BM041870.D
Acq On : 14 Sep 2023 18:48
Operator : MA/JU
Sample : PB155434 BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK434

Quant Time: Sep 15 00:30:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 16:15:23 2023
Response via : Initial Calibration




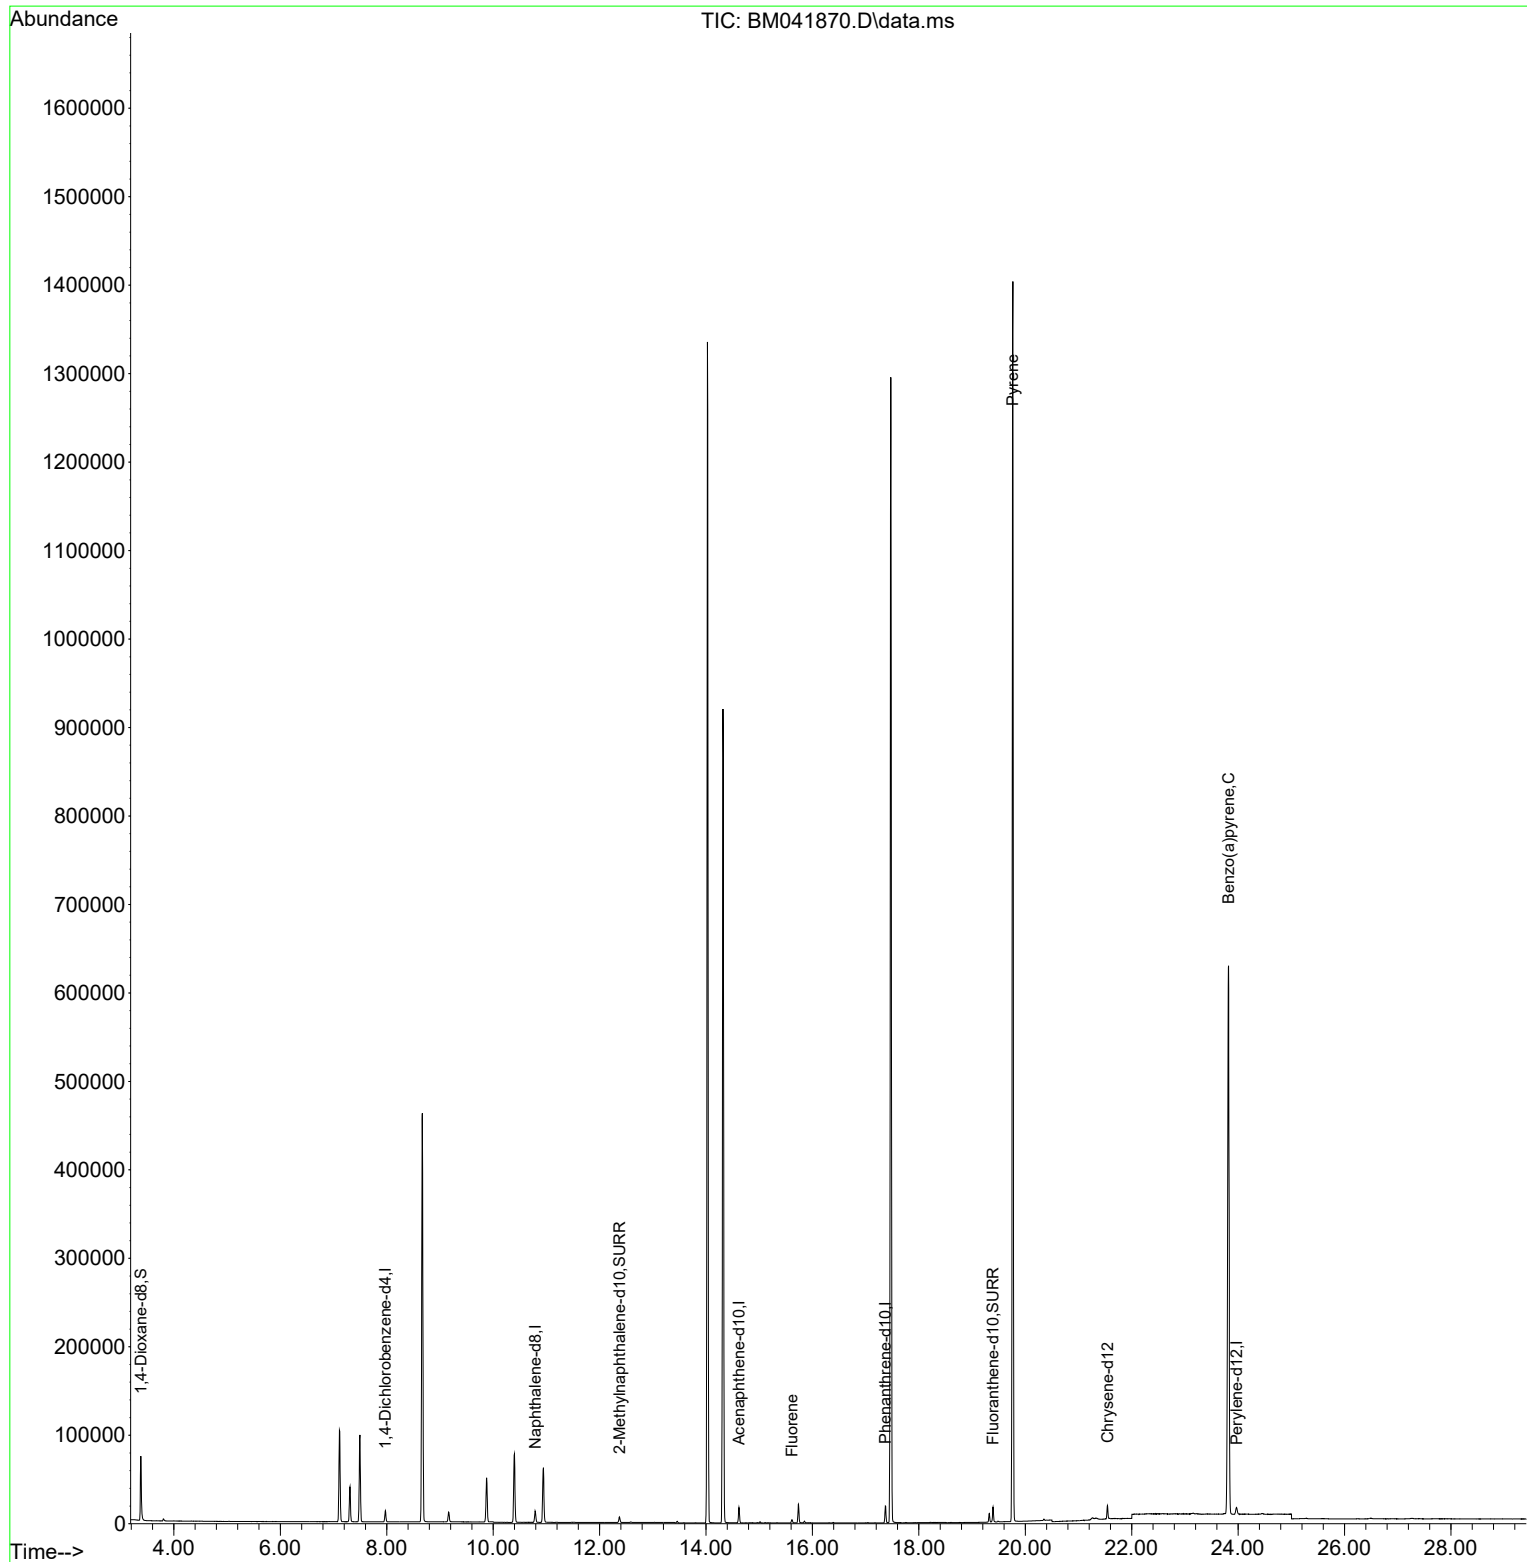


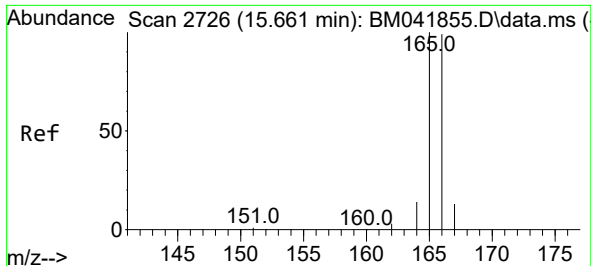

#12
Fluorene
Concen: 0.066 ng/ul
RT: 15.614 min Scan# 21
Delta R.T. -0.051 min
Lab File: BM041870.D
Acq: 14 Sep 2023 18:48




Instrument :
BNA_M
ClientSampleId :
SBLK434


Tgt Ion:166 Resp: 3304
Ion Ratio Lower Upper
166 100
165 9.0 79.3 118.9#
167 34.2 11.2 16.8#

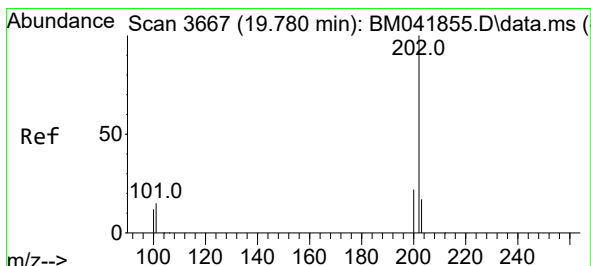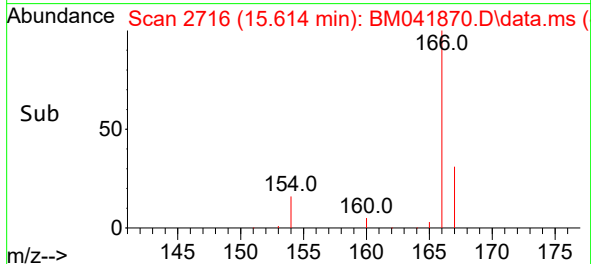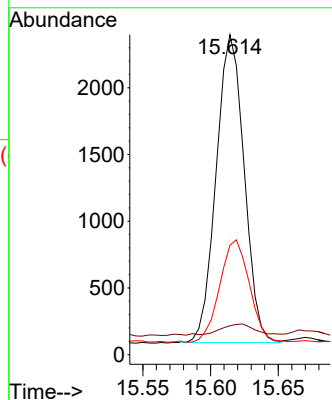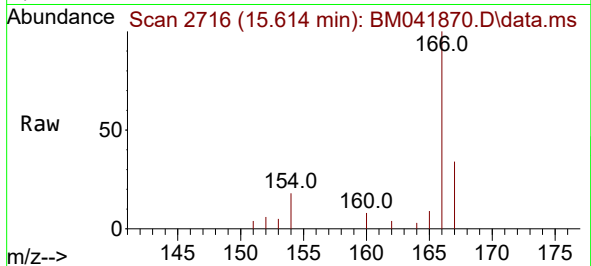

#20
Pyrene
Concen: 0.031 ng/ul
RT: 19.766 min Scan# 3664
Delta R.T. -0.019 min
Lab File: BM041870.D
Acq: 14 Sep 2023 18:48


Tgt Ion:202 Resp: 3129
Ion Ratio Lower Upper
202 100
101 149.1 12.6 19.0#
100 1069.8 9.9 14.9#

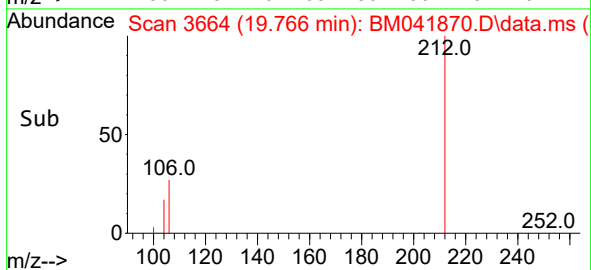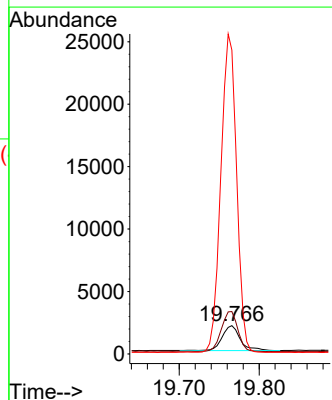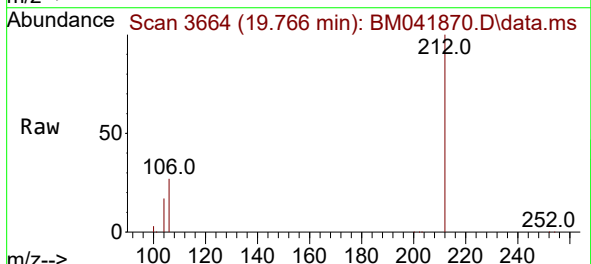

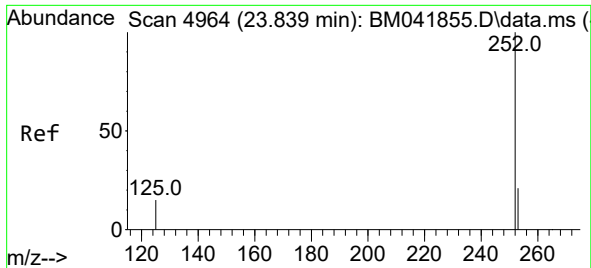

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.819 min Scan# 4957
Delta R.T. -0.026 min
Lab File: BM041870.D
Acq: 14 Sep 2023 18:48

Instrument :
BNA_M
ClientSampleId :
SBLK434

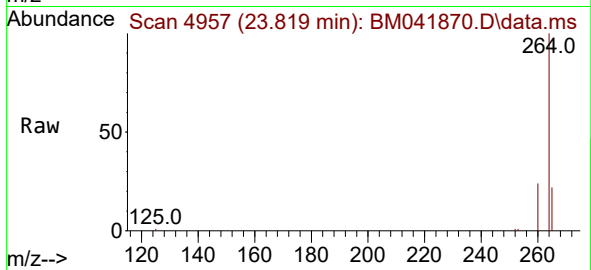

Tgt Ion:252 Resp: 4259
Ion Ratio Lower Upper
252 100
253 68.2 21.8 32.8#
125 87.8 18.8 28.2#

