




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041852.D
 Acq On : 14 Sep 2023 04:37
 Operator : MA/JU
 Sample : 04175-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYX4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :mohammad ahmed 09/15/2023

Quant Time: Sep 14 06:19:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

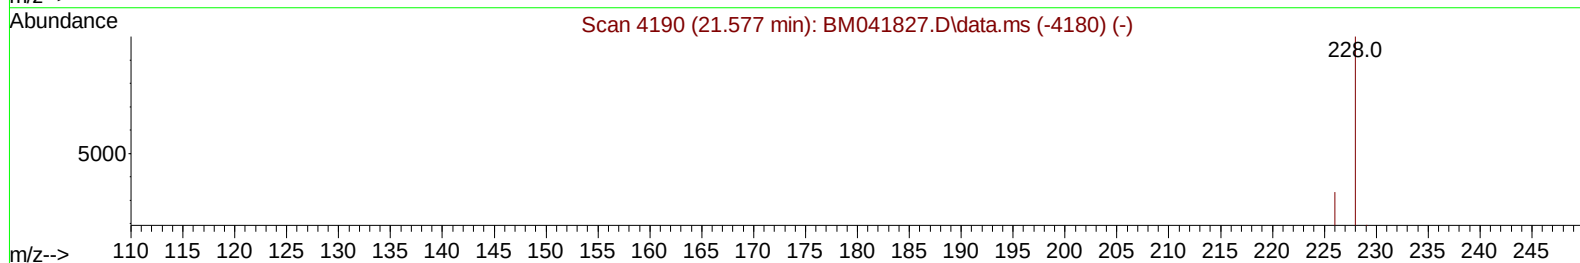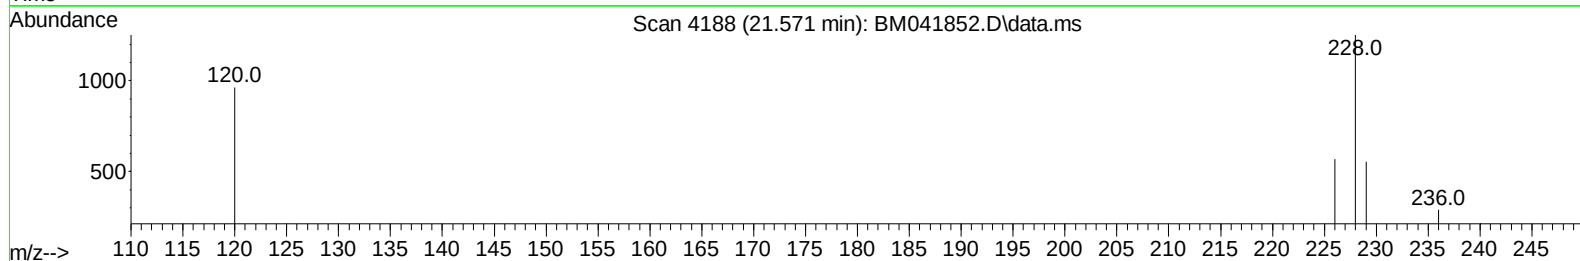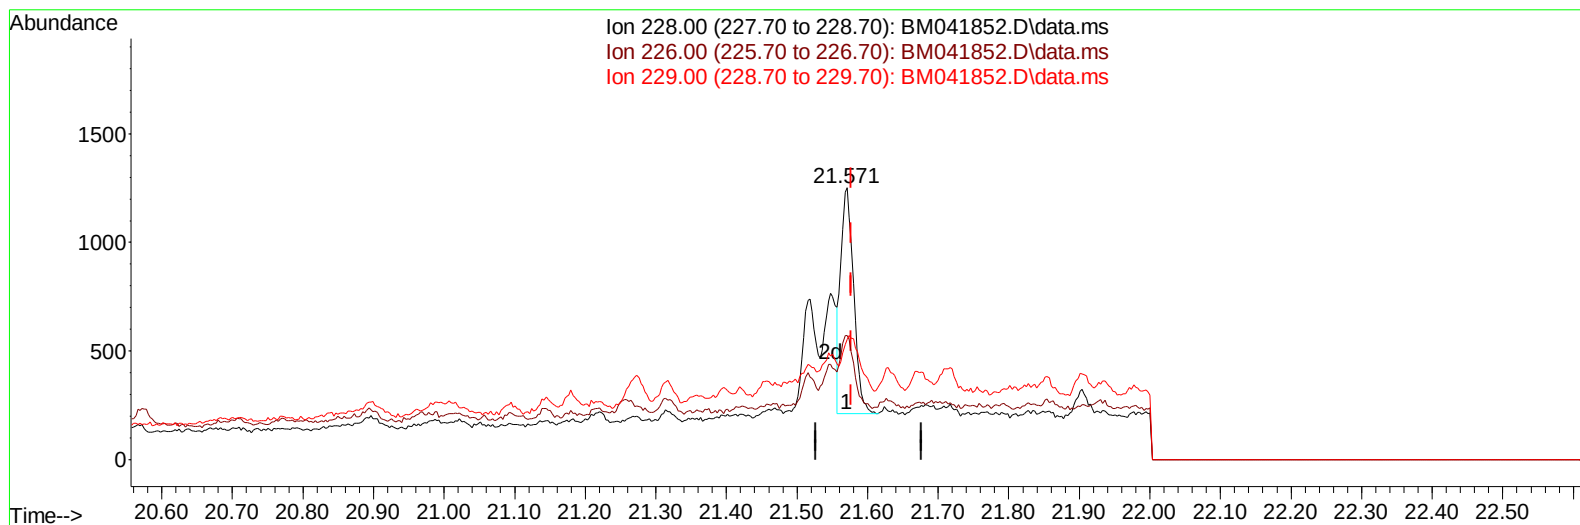

TIC: BM041852.D\data.ms

(22) Chrysene

21.571min (-0.006) 0.02 ng/u1

response 1329

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	33.70	45.56#
229.00	19.60	44.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041852.D
 Acq On : 14 Sep 2023 04:37
 Operator : MA/JU
 Sample : 04175-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYX4

Manual IntegrationsAPPROVED

Quant Time: Sep 14 06:19:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :mohammad ahmed 09/15/2023

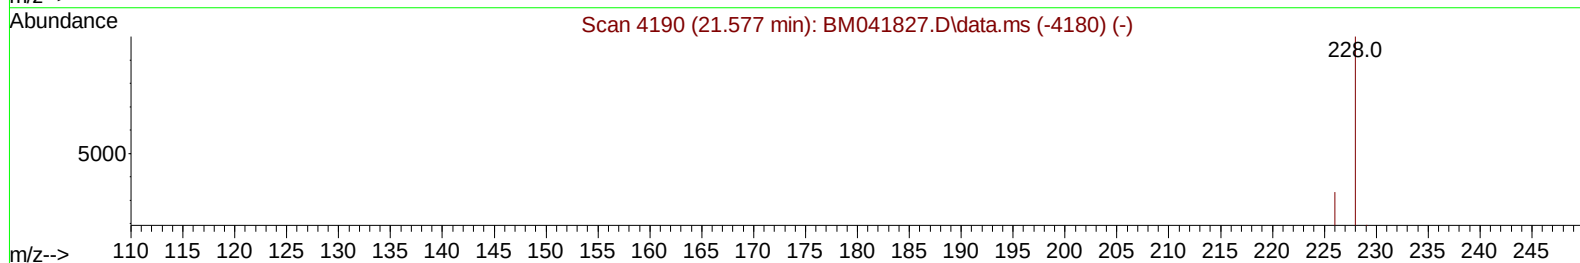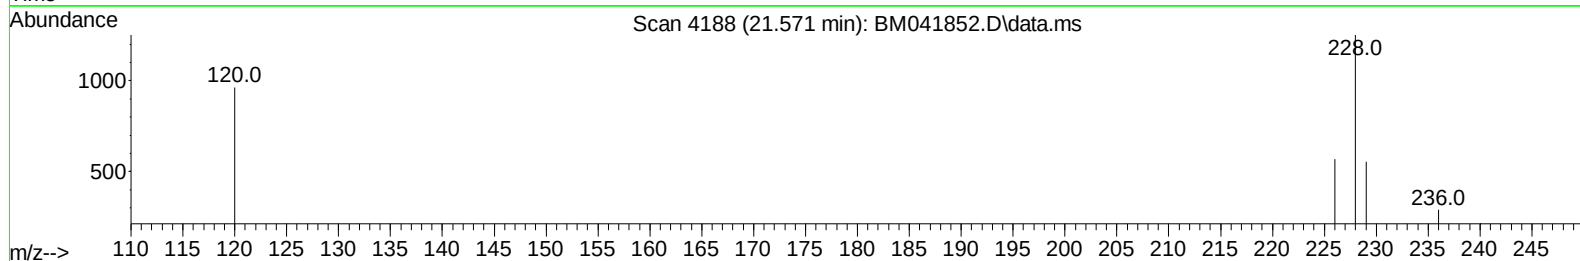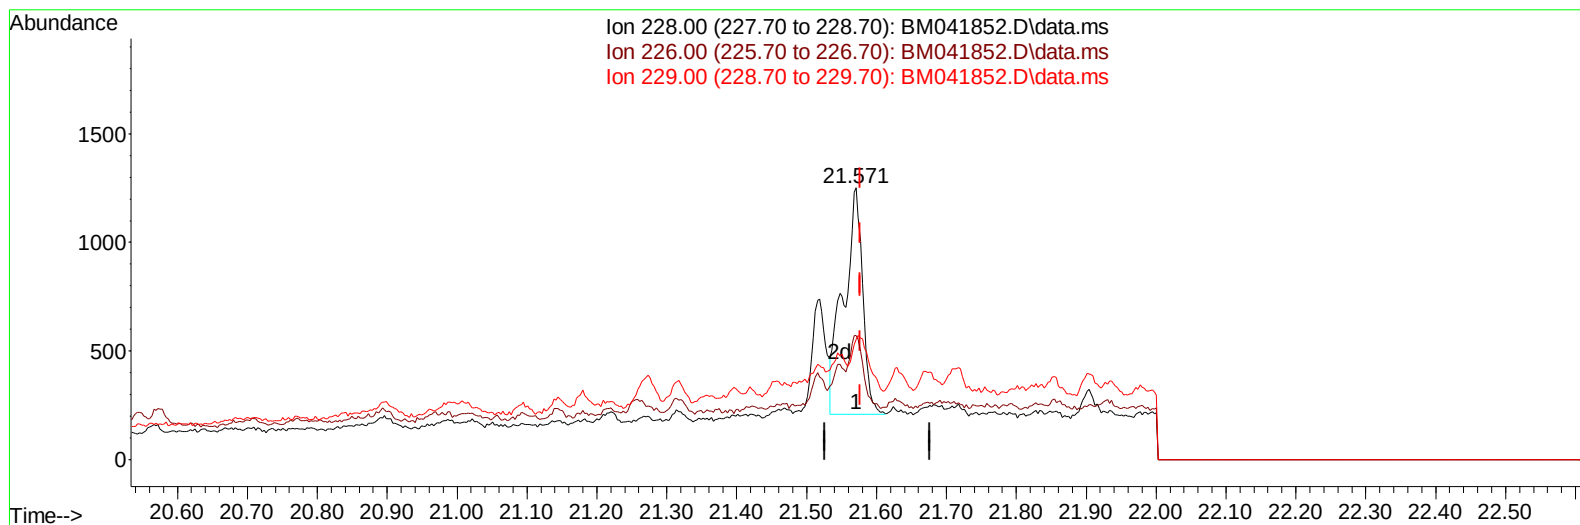

TIC: BM041852.D\data.ms

(22) Chrysene

21.571min (-0.006) 0.03 ng/ul m

response 1997

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	33.70	45.56#
229.00	19.60	44.28#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041852.D
 Acq On : 14 Sep 2023 04:37
 Operator : MA/JU
 Sample : 04175-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EZYX4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/14/2023
 Supervised By :mohammad ahmed 09/15/2023

Quant Time: Sep 14 06:19:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.971	152		5619	0.400	ng/ul	0.00
4) Naphthalene-d8	10.785	136		14627	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.615	164		8358	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.363	188		18071	0.400	ng/ul	0.00
17) Chrysene-d12	21.533	240		11402	0.400	ng/ul	0.00
23) Perylene-d12	23.947	264		12833	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.381	96		39758	5.563	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152		6384	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.385	212		13428	0.343	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.834	128		3336	0.068	ng/ul#	90
15) Phenanthrene	17.405	178		3527	0.045	ng/ul#	87
22) Chrysene	21.571	228		1997m	0.026	ng/ul	
24) Benzo(b)fluoranthene	23.202	252		2205	0.024	ng/ul#	1
29) Benzo(g,h,i)perylene	27.223	276		2203	0.024	ng/ul#	40

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
Data File : BM041852.D
Acq On : 14 Sep 2023 04:37
Operator : MA/JU
Sample : 04175-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EZYX4

Manual IntegrationsAPPROVED

Quant Time: Sep 14 06:19:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 16:15:23 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/14/2023
Supervised By :mohammad ahmed 09/15/2023

