

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041834.D
 Acq On : 13 Sep 2023 17:29
 Operator : MA/JU
 Sample : 04324-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJA6

Quant Time: Sep 13 18:11:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	6294	0.400	ng/ul	0.00
4) Naphthalene-d8	10.790	136	16275	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.615	164	8592	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.367	188	17836	0.400	ng/ul	0.00
17) Chrysene-d12	21.539	240	9601	0.400	ng/ul	0.00
23) Perylene-d12	23.956	264	11337	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	16740	2.091	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	5228	0.236	ng/ul	0.00
18) Fluoranthene-d10	19.390	212	11615	0.353	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.414	88	591	0.070	ng/ul	84
24) Benzo(b)fluoranthene	23.211	252	2443	0.030	ng/ul#	32


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
Data File : BM041834.D
Acq On : 13 Sep 2023 17:29
Operator : MA/JU
Sample : 04324-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJA6

Quant Time: Sep 13 18:11:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 16:15:23 2023
Response via : Initial Calibration




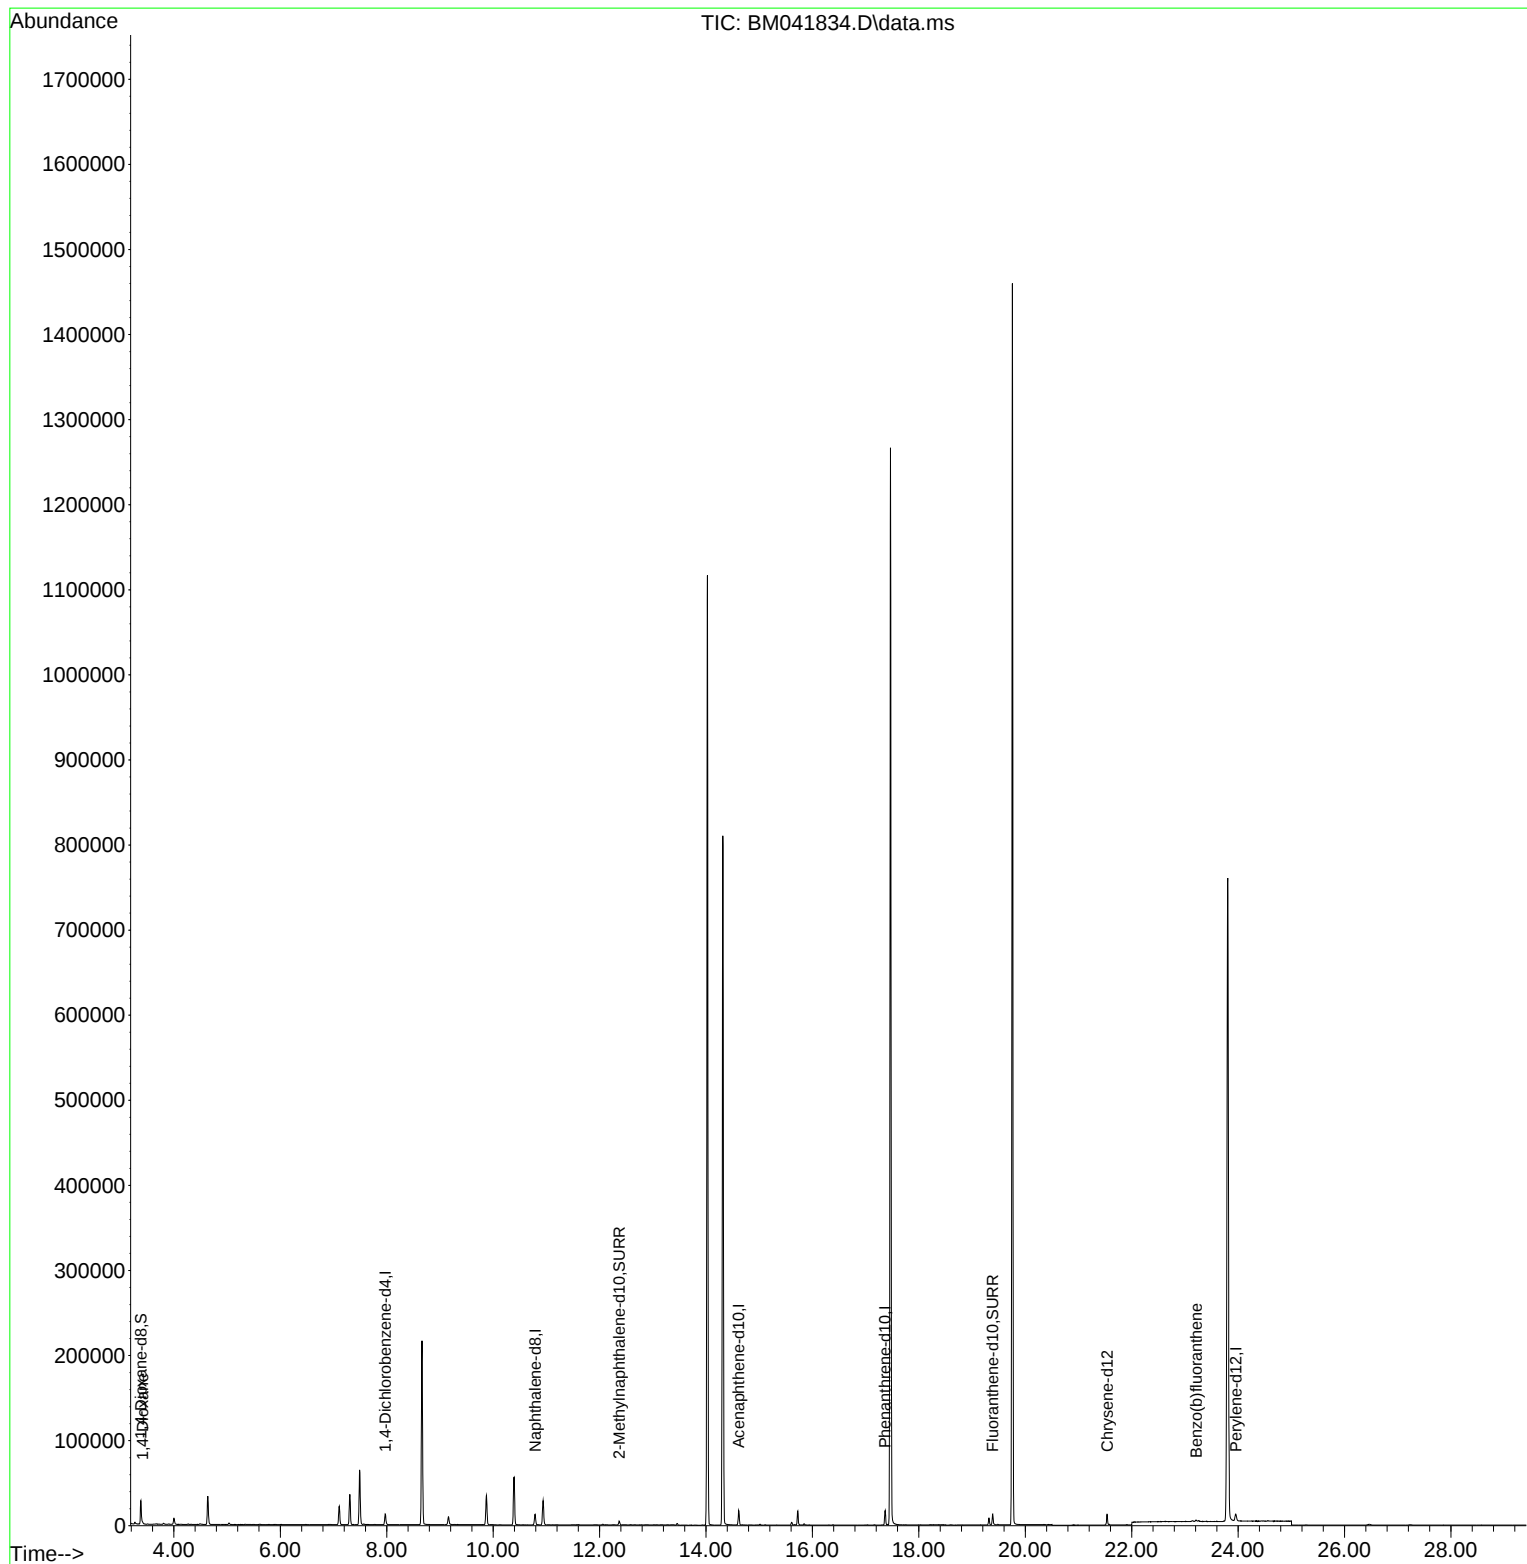


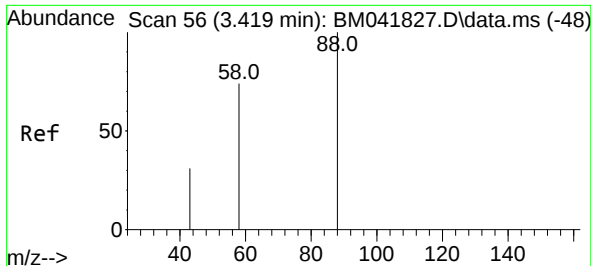

#2
1,4-Dioxane
Concen: 0.070 ng/ul
RT: 3.414 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM041834.D
Acq: 13 Sep 2023 17:29

Instrument :
BNA_M
ClientSampleId :
BBJA6

Tgt Ion: 88 Resp: 591
Ion Ratio Lower Upper
88 100
43 103.6 69.9 104.9
58 57.6 55.6 83.4

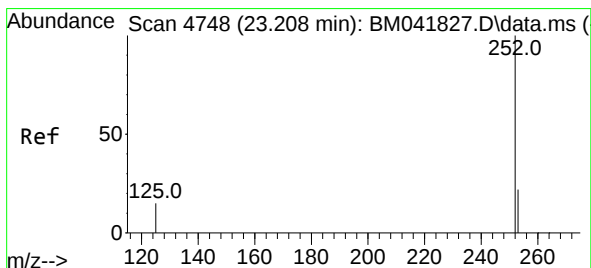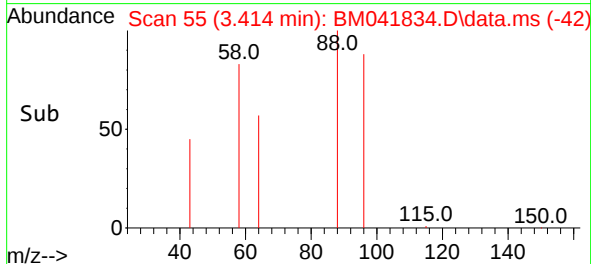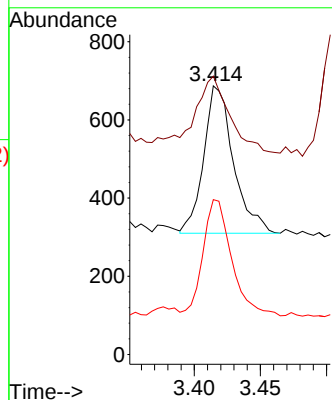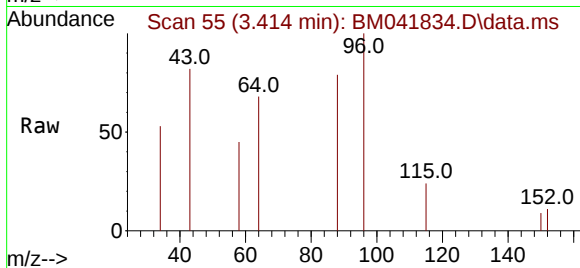

#24
Benzo(b)fluoranthene
Concen: 0.030 ng/ul
RT: 23.211 min Scan# 4749
Delta R.T. 0.003 min
Lab File: BM041834.D
Acq: 13 Sep 2023 17:29

Tgt Ion: 252 Resp: 2443
Ion Ratio Lower Upper
252 100
253 52.9 0.0 51.0#
125 59.2 0.0 39.8#

