

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
 Data File : BM041839.D
 Acq On : 13 Sep 2023 20:36
 Operator : MA/JU
 Sample : 04324-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKG8

Quant Time: Sep 14 03:38:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 13 16:15:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	4879	0.400	ng/ul	0.00
4) Naphthalene-d8	10.790	136	13023	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.615	164	6618	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.367	188	13439	0.400	ng/ul	0.00
17) Chrysene-d12	21.536	240	6741	0.400	ng/ul	0.00
23) Perylene-d12	23.956	264	8048	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	17913	2.886	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	5981	0.338	ng/ul	0.00
18) Fluoranthene-d10	19.389	212	11995	0.519	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.414	88	1370	0.210	ng/ul#	85
24) Benzo(b)fluoranthene	23.211	252	1932	0.034	ng/ul#	23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091323\
Data File : BM041839.D
Acq On : 13 Sep 2023 20:36
Operator : MA/JU
Sample : 04324-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBKG8

Quant Time: Sep 14 03:38:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 13 16:15:23 2023
Response via : Initial Calibration




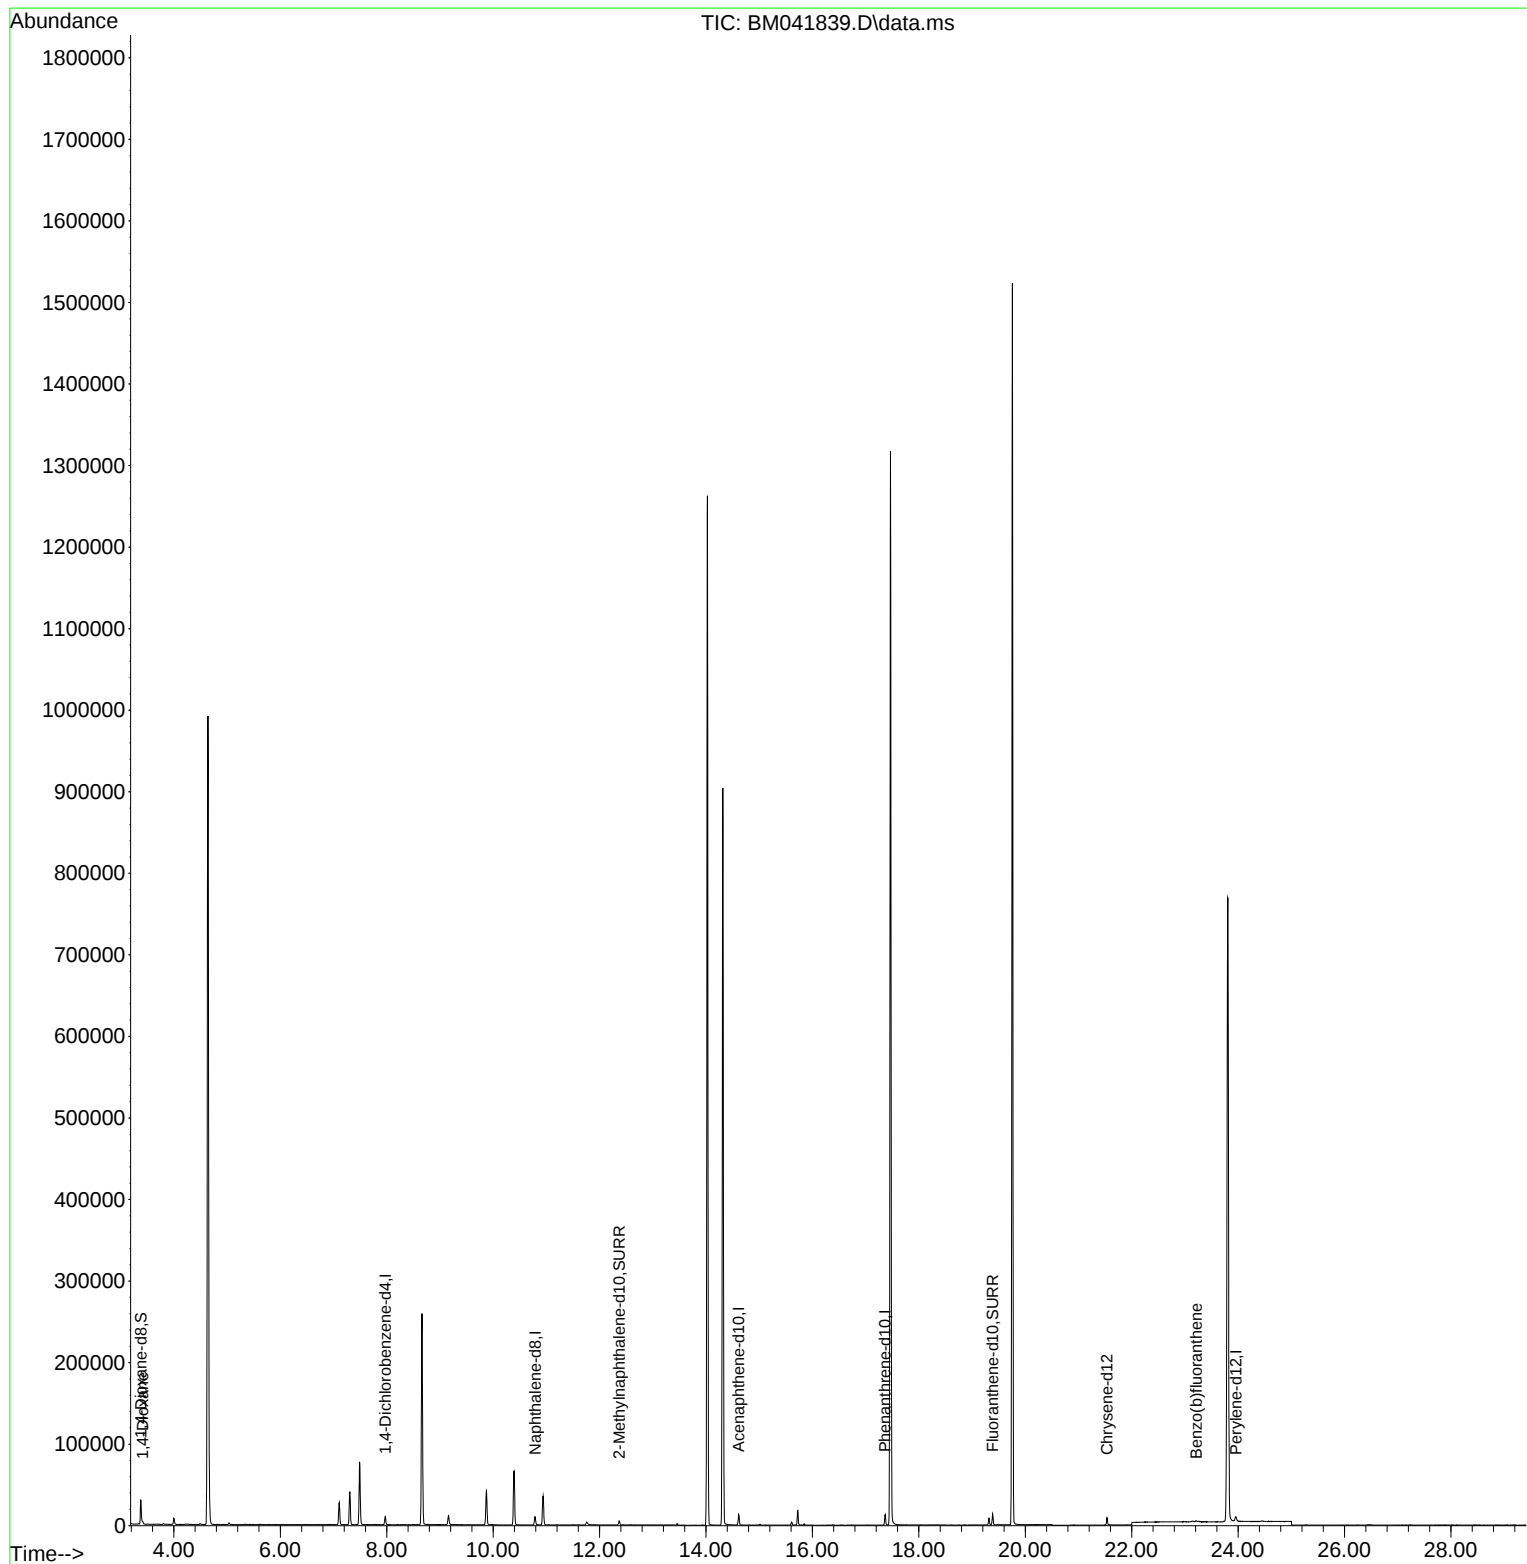


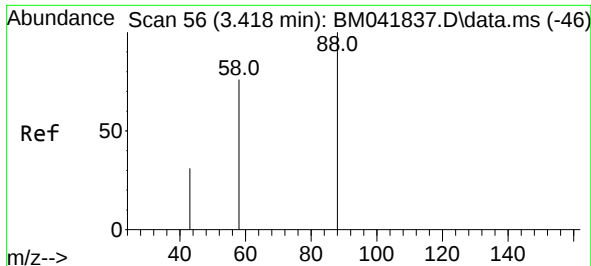

#2
1,4-Dioxane
Concen: 0.210 ng/ul
RT: 3.414 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM041839.D
Acq: 13 Sep 2023 20:36

Instrument :
BNA_M
ClientSampleId :
BBKG8

Tgt Ion: 88 Resp: 1370
Ion Ratio Lower Upper
88 100
43 65.4 69.9 104.9#
58 65.4 55.6 83.4

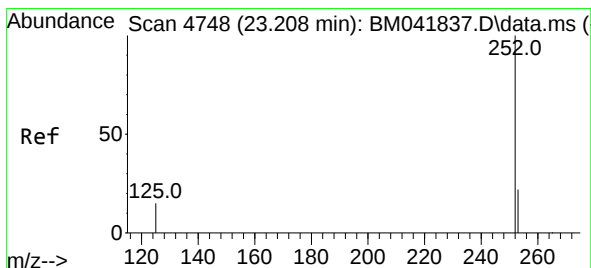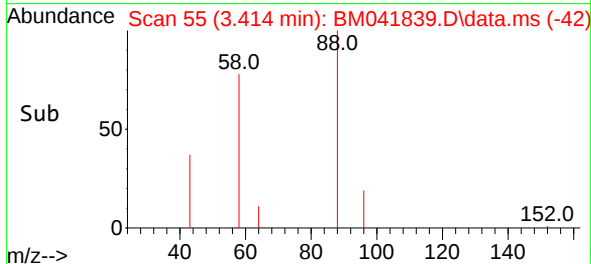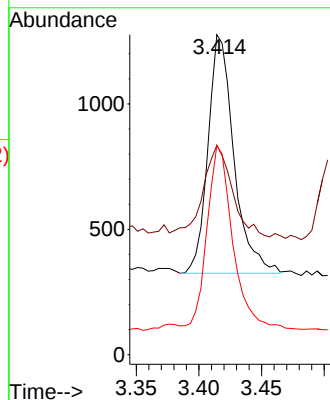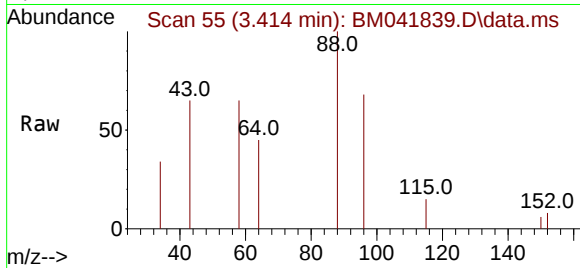

#24
Benzo(b)fluoranthene
Concen: 0.034 ng/ul
RT: 23.211 min Scan# 4749
Delta R.T. 0.003 min
Lab File: BM041839.D
Acq: 13 Sep 2023 20:36

Tgt Ion: 252 Resp: 1932
Ion Ratio Lower Upper
252 100
253 56.4 0.0 51.0#
125 64.9 0.0 39.8#

