

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091622\
 Data File : BM036561.D
 Acq On : 16 Sep 2022 14:10
 Operator : CG/JU
 Sample : N4601-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5753

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 09/19/2022
 Supervised By :mohammad ahmed 09/19/2022

Quant Time: Sep 16 22:59:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 16 02:39:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.028	152	322088	20.000	ng/u1	0.00
20) Naphthalene-d8	10.839	136	1457584	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	954330	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.386	188	1993511	20.000	ng/u1	0.00
79) Chrysene-d12	21.550	240	1941338	20.000	ng/u1	0.00
88) Perylene-d12	23.997	264	1918214	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	30181	3.513	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.169	99	525092	18.243	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.345	67	366594	20.972	ng/u1	0.00
11) 2-Chlorophenol-d4	7.551	132	435057	20.994	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	369467	17.372	ng/u1	-0.01
21) Nitrobenzene-d5	9.186	128	211632	21.451	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	192979	21.838	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	405165	19.784	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.969	131	348493	10.235	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	1413374	21.959	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	1665621	21.816	ng/u1	0.00
54) 4-Nitrophenol-d4	14.821	143	110929	8.886	ng/u1	0.00
60) Fluorene-d10	15.633	176	1305327	22.630	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	108669	13.778	ng/u1	-0.01
73) Anthracene-d10	17.480	188	2024627	22.212	ng/u1	0.00
81) Pyrene-d10	19.762	212	2411405	25.249	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.838	264	2195757	23.430	ng/u1	0.00
Target Compounds					Qvalue	
30) Naphthalene	10.886	128	158993	2.002	ng/u1	99
36) 2-Methylnaphthalene	12.486	142	166829	3.153	ng/u1	99
37) 1-Methylnaphthalene	12.704	142	155909	2.931	ng/u1	100
50) Acenaphthylene	14.368	152	99108	1.135	ng/u1#	96
72) Phenanthrene	17.427	178	443673	4.041	ng/u1	100
80) Fluoranthene	19.433	202	638789	5.458	ng/u1	98
82) Pyrene	19.792	202	591017	4.771	ng/u1	99
85) Benzo(a)anthracene	21.533	228	372932m	3.066	ng/u1	
87) Chrysene	21.591	228	606451	5.253	ng/u1	96
90) Benzo(b)fluoranthene	23.250	252	815709	6.706	ng/u1	98
91) Benzo(k)fluoranthene	23.297	252	231841m	1.907	ng/u1	
93) Benzo(a)pyrene	23.891	252	337915	3.160	ng/u1	99
94) Indeno(1,2,3-cd)pyrene	26.538	276	260557	2.087	ng/u1	98
96) Benzo(g,h,i)perylene	27.320	276	212441	1.962	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091622\
 Data File : BM036561.D
 Acq On : 16 Sep 2022 14:10
 Operator : CG/JU
 Sample : N4601-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 A5753

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 09/19/2022
 Supervised By :mohammad ahmed 09/19/2022


Quant Time: Sep 16 22:59:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Sep 16 02:39:54 2022
 Response via : Initial Calibration

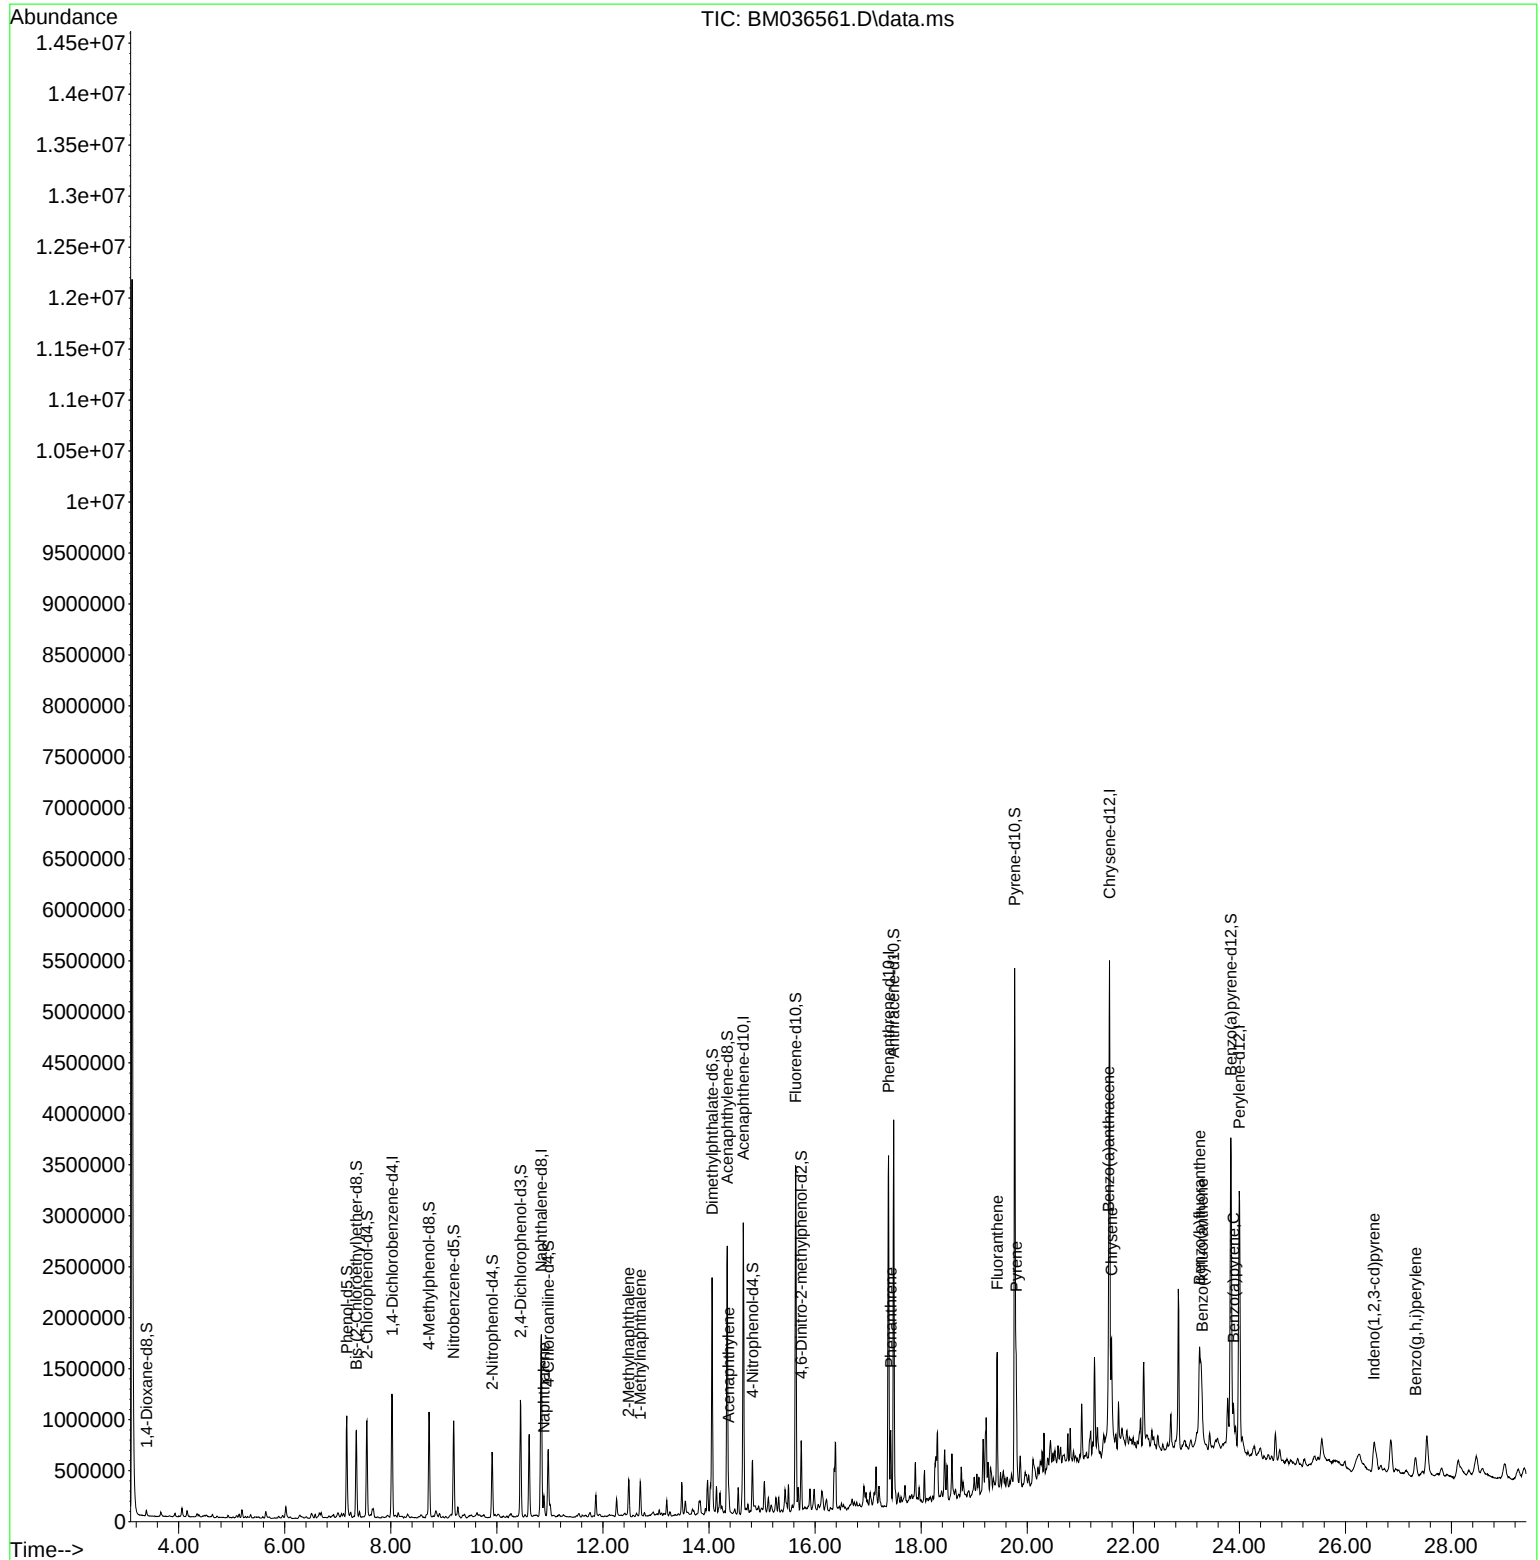



#30
Naphthalene
Concen: 2.002 ng/ul
RT: 10.886 min Scan# 1327
Delta R.T. -0.006 min
Lab File: BM036561.D
Acq: 16 Sep 2022 14:10




Instrument :
BNA_M
ClientSampleId :
A5753




Tgt Ion:128 Resp: 158993
Ion Ratio Lower Upper
128 100
129 10.1 8.7 13.1
127 13.2 10.3 15.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

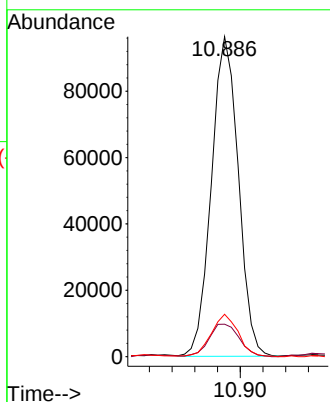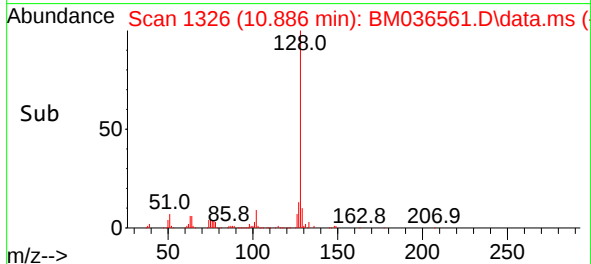


#36
2-Methylnaphthalene
Concen: 3.153 ng/ul
RT: 12.486 min Scan# 1598
Delta R.T. -0.006 min
Lab File: BM036561.D
Acq: 16 Sep 2022 14:10

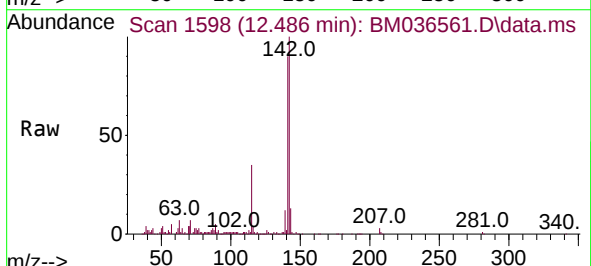

Tgt Ion:142 Resp: 166829
Ion Ratio Lower Upper
142 100
141 89.8 70.7 106.1

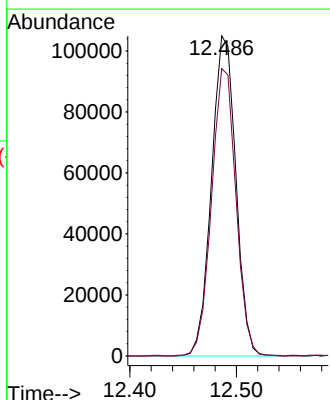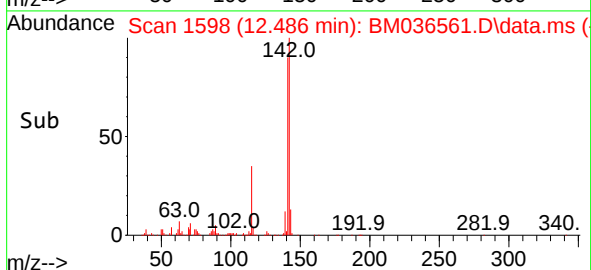

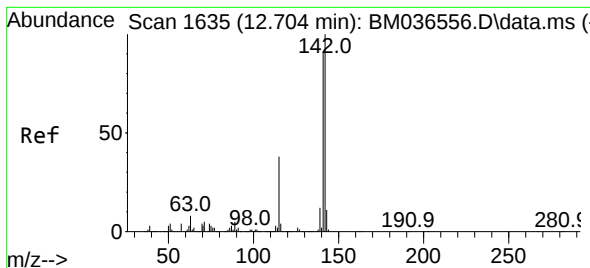

#37

1-Methylnaphthalene

Concen: 2.931 ng/ul

RT: 12.704 min Scan# 1635

Delta R.T. -0.006 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10

Instrument :

BNA_M

ClientSampleId :





A5753

Tgt Ion:	142	Resp:	155909
Ion Ratio	Lower	Upper	
142	100		
141	92.0	73.4	110.2
116	4.1	3.1	4.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

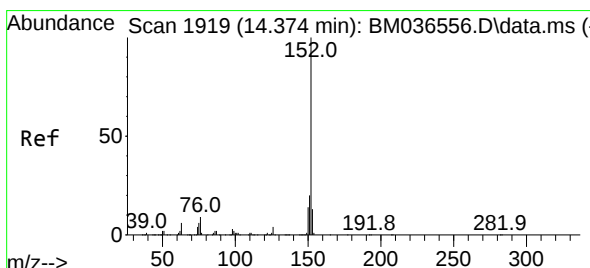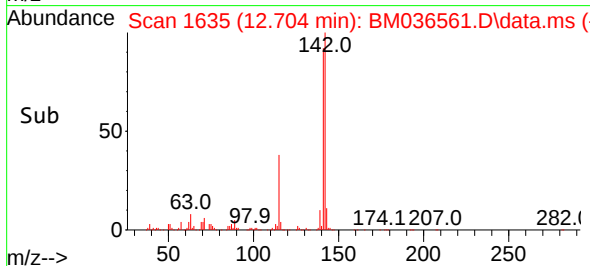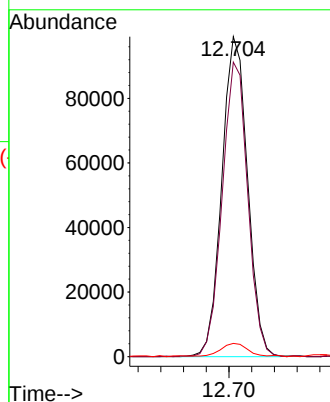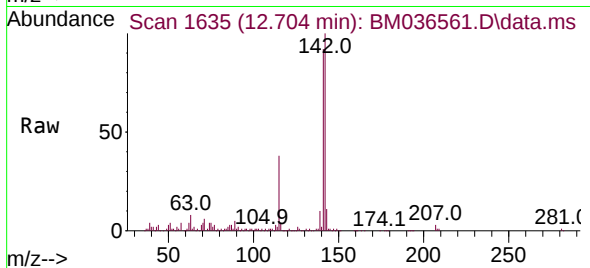

#50

Acenaphthylene

Concen: 1.135 ng/ul




RT: 14.368 min Scan# 1918


Delta R.T. -0.006 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10


Tgt Ion:	152	Resp:	99108
Ion Ratio	Lower	Upper	
152	100		
151	20.7	15.7	23.5
153	15.7	10.5	15.7

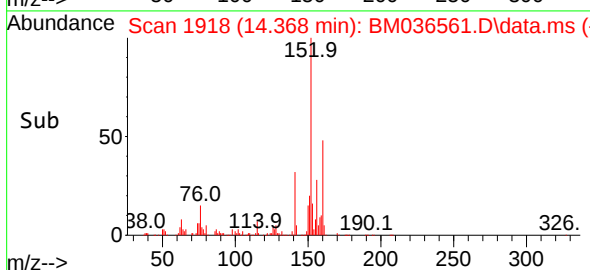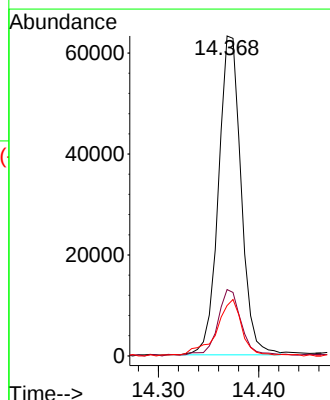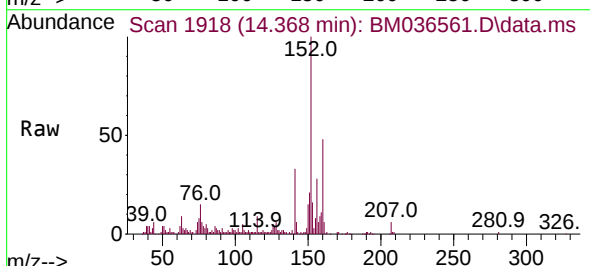

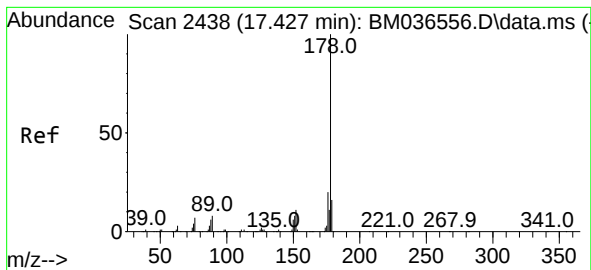

#72
Phenanthrene
Concen: 4.041 ng/ul
RT: 17.427 min Scan# 2438
Delta R.T. -0.006 min
Lab File: BM036561.D
Acq: 16 Sep 2022 14:10




Instrument :
BNA_M
ClientSampleId :
A5753




Tgt Ion:178 Resp: 443673
Ion Ratio Lower Upper
178 100
179 15.5 12.2 18.2
176 19.6 15.7 23.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

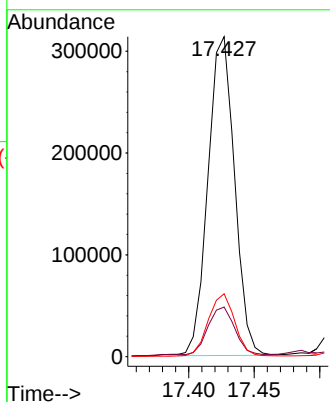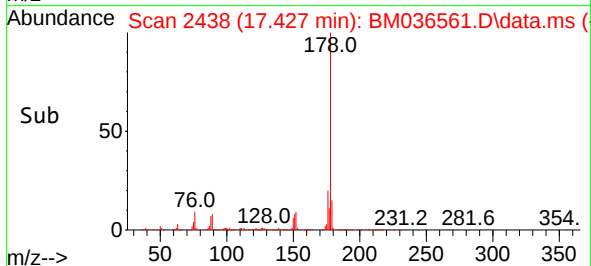


#80
Fluoranthene
Concen: 5.458 ng/ul
RT: 19.433 min Scan# 2779
Delta R.T. -0.000 min
Lab File: BM036561.D
Acq: 16 Sep 2022 14:10

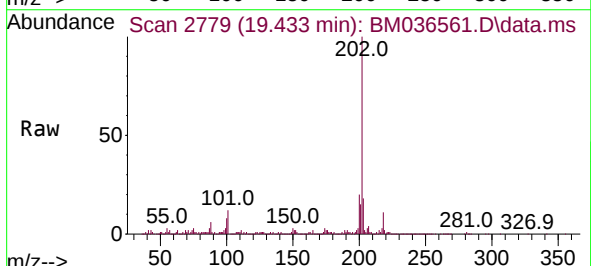

Tgt Ion:202 Resp: 638789
Ion Ratio Lower Upper
202 100
101 11.9 9.8 14.6
100 8.4 7.4 11.2

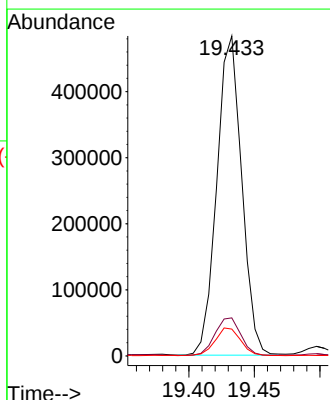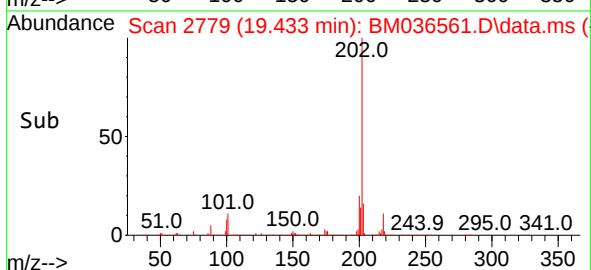



#82

Pyrene

Concen: 4.771 ng/ul

RT: 19.792 min Scan# 2840

Delta R.T. -0.006 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10

Instrument :

BNA_M

ClientSampleId :





A5753

Tgt Ion:	202	Resp:	59101
Ion Ratio	Lower	Upper	
202	100		
101	13.8	10.9	16.3
100	11.7	8.7	13.1

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

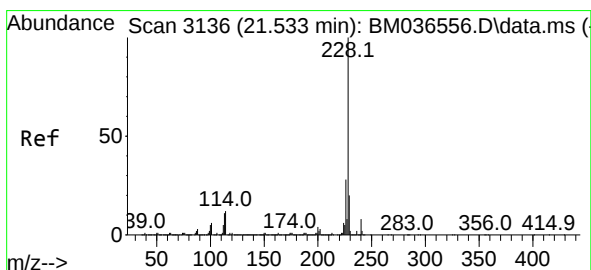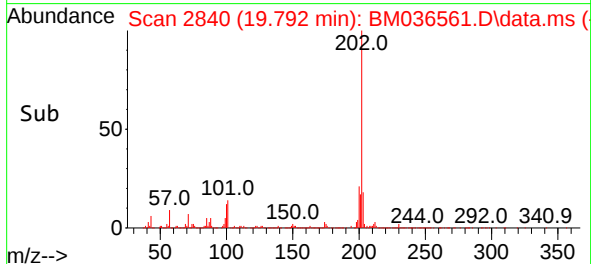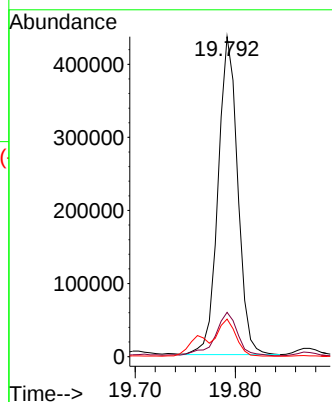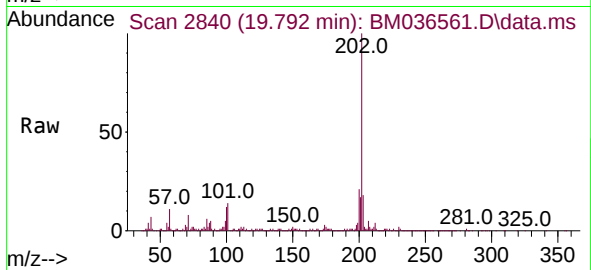

#85

Benzo(a)anthracene

Concen: 3.066 ng/ul m




RT: 21.533 min Scan# 3136


Delta R.T. -0.006 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10


Tgt Ion:	228	Resp:	372932
Ion Ratio	Lower	Upper	
228	100		
229	23.8	15.8	23.8
226	30.3	21.9	32.9

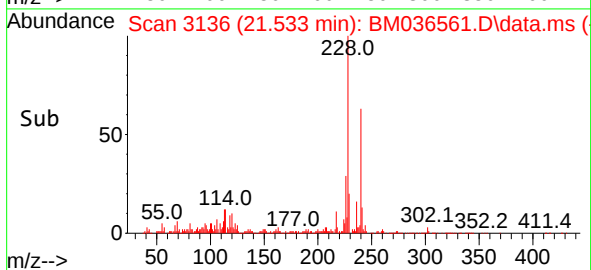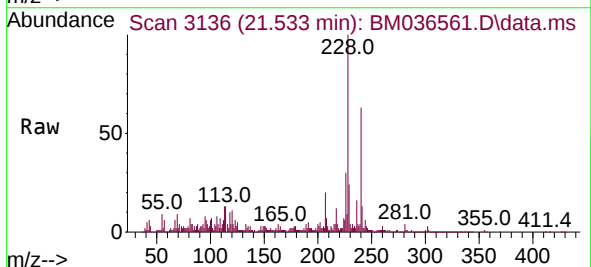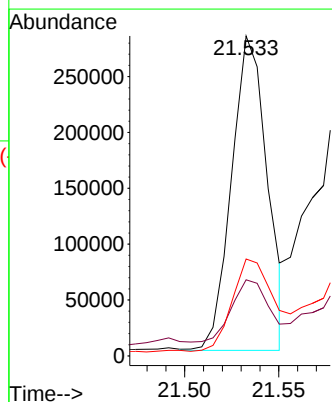



#87
Chrysene
Concen: 5.253 ng/ul
RT: 21.591 min Scan# 3146
Delta R.T. -0.000 min
Lab File: BM036561.D
Acq: 16 Sep 2022 14:10




Instrument :
BNA_M
ClientSampleId :
A5753



Tgt Ion:228 Resp: 60645
Ion Ratio Lower Upper
228 100
226 29.9 24.4 36.6
229 22.8 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

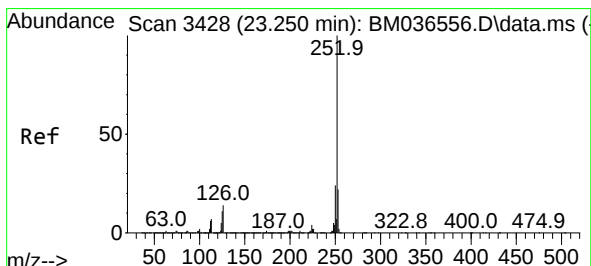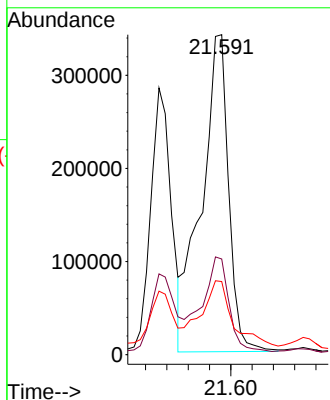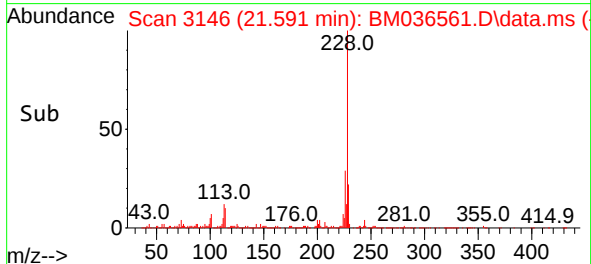

#90
Benzo(b)fluoranthene
Concen: 6.706 ng/ul
RT: 23.250 min Scan# 3428
Delta R.T. -0.000 min
Lab File: BM036561.D
Acq: 16 Sep 2022 14:10

Tgt Ion:252 Resp: 815709
Ion Ratio Lower Upper
252 100
253 22.7 17.6 26.4
125 12.0 9.1 13.7

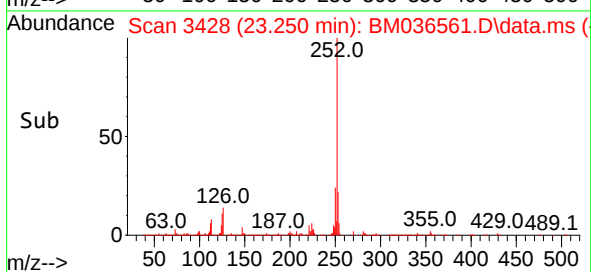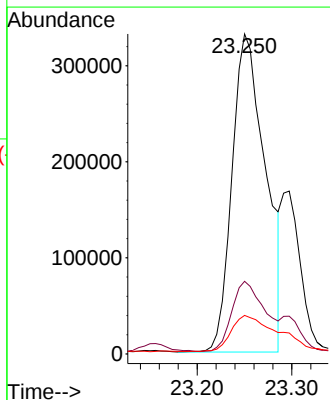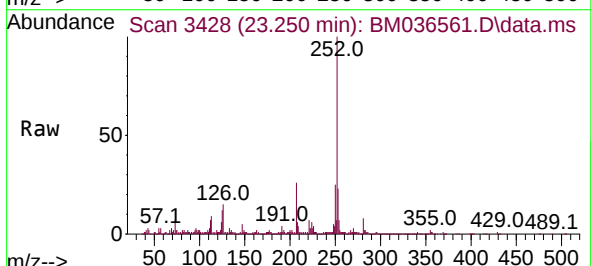



#91

Benzo(k)fluoranthene

Concen: 1.907 ng/ul m

RT: 23.297 min Scan# 34

Delta R.T. -0.006 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10

Instrument :

BNA_M

ClientSampleId :

A5753





Tgt Ion:252 Resp: 23184

Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.8	26.8
125	12.8	8.2	12.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

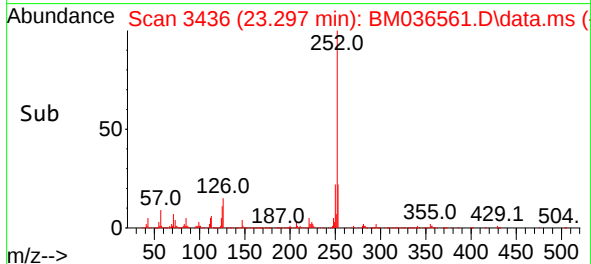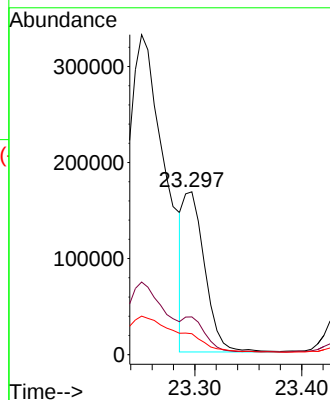

#93

Benzo(a)pyrene

Concen: 3.160 ng/ul

RT: 23.891 min Scan# 3537




Delta R.T. -0.000 min


Lab File: BM036561.D

Acq: 16 Sep 2022 14:10

Tgt Ion:252 Resp: 337915

Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.5	26.3
125	12.6	9.5	14.3

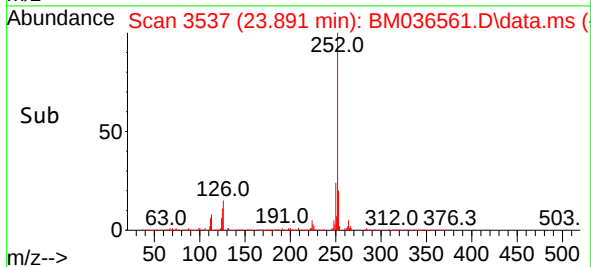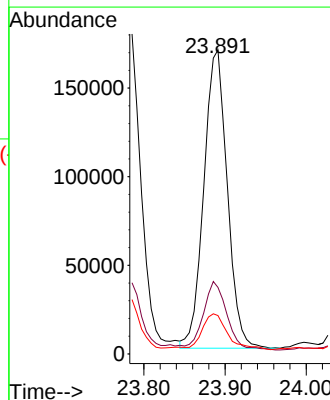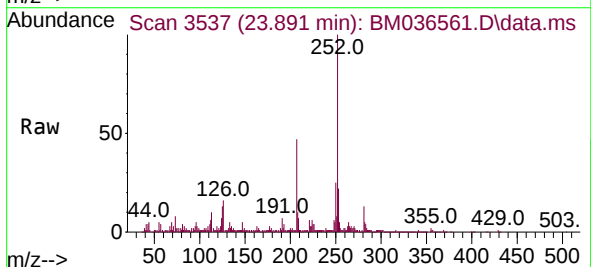



#94

Indeno(1,2,3-cd)pyrene

Concen: 2.087 ng/ul

RT: 26.538 min Scan# 3987

Delta R.T. -0.012 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10

Instrument :

BNA_M

ClientSampleId :





A5753

Tgt Ion:	276	Resp:	26055
Ion Ratio	Lower	Upper	
276	100		
138	23.6	20.2	30.4
277	24.3	19.7	29.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 09/19/2022
Supervised By :mohammad ahmed 09/19/2022

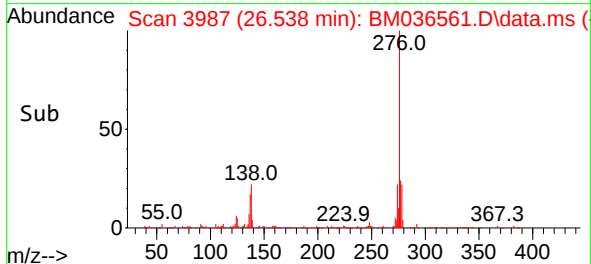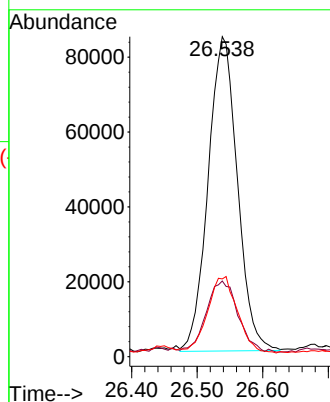

#96

Benzo(g,h,i)perylene

Concen: 1.962 ng/ul

RT: 27.320 min Scan# 4120

Delta R.T. -0.012 min

Lab File: BM036561.D

Acq: 16 Sep 2022 14:10

Tgt Ion:	276	Resp:	212441
Ion Ratio	Lower	Upper	
276	100		
138	24.2	18.7	28.1
277	25.0	19.2	28.8

