
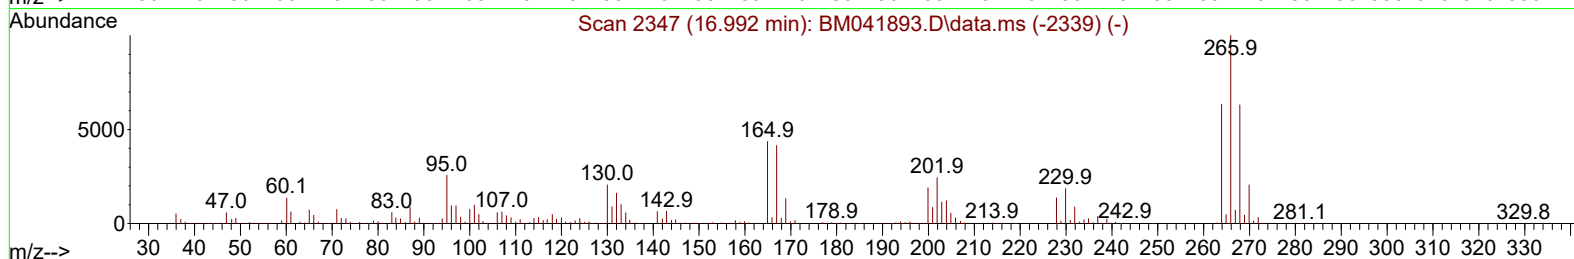
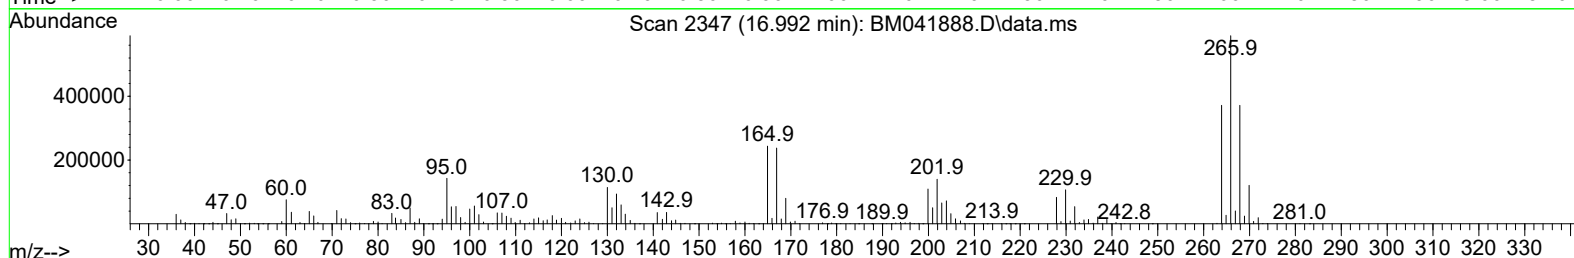


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041888.D
Acq On : 18 Sep 2023 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 05:46:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

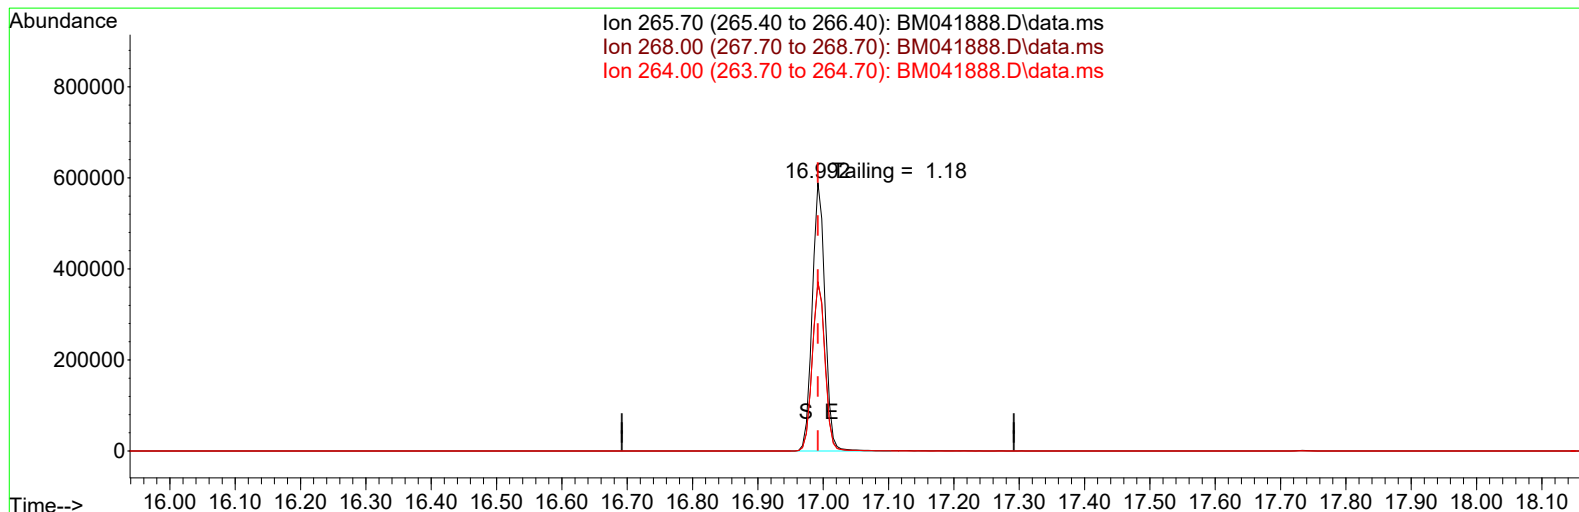

TIC: BM041888.D\data.ms

(70) Pentachlorophenol (C)




16.992min (-0.000) 0.00 ng

response 802781

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.99
264.00	63.30	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041888.D
Acq On : 18 Sep 2023 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 05:46:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

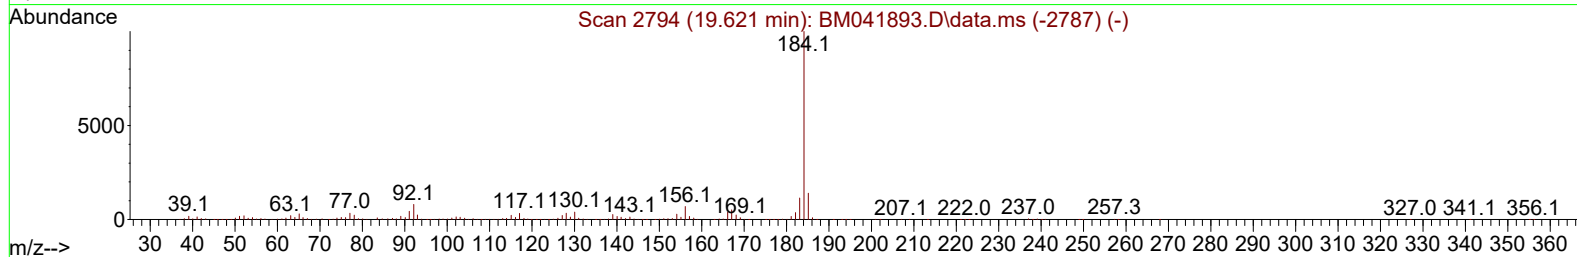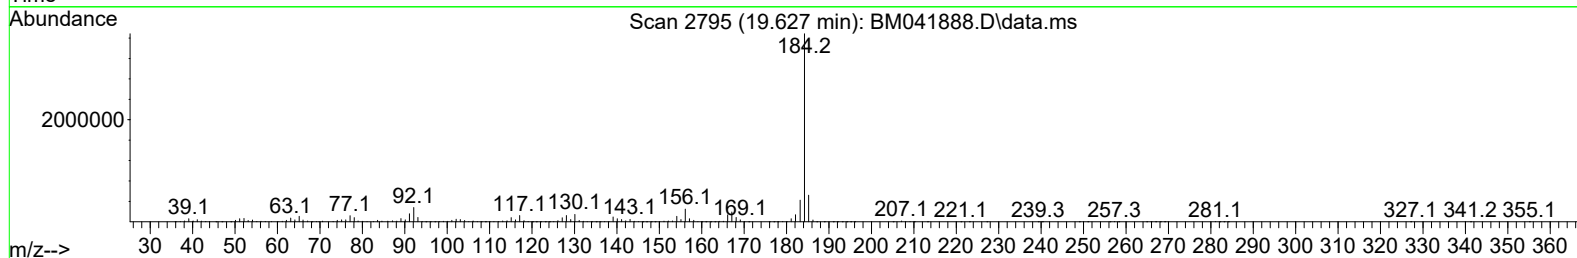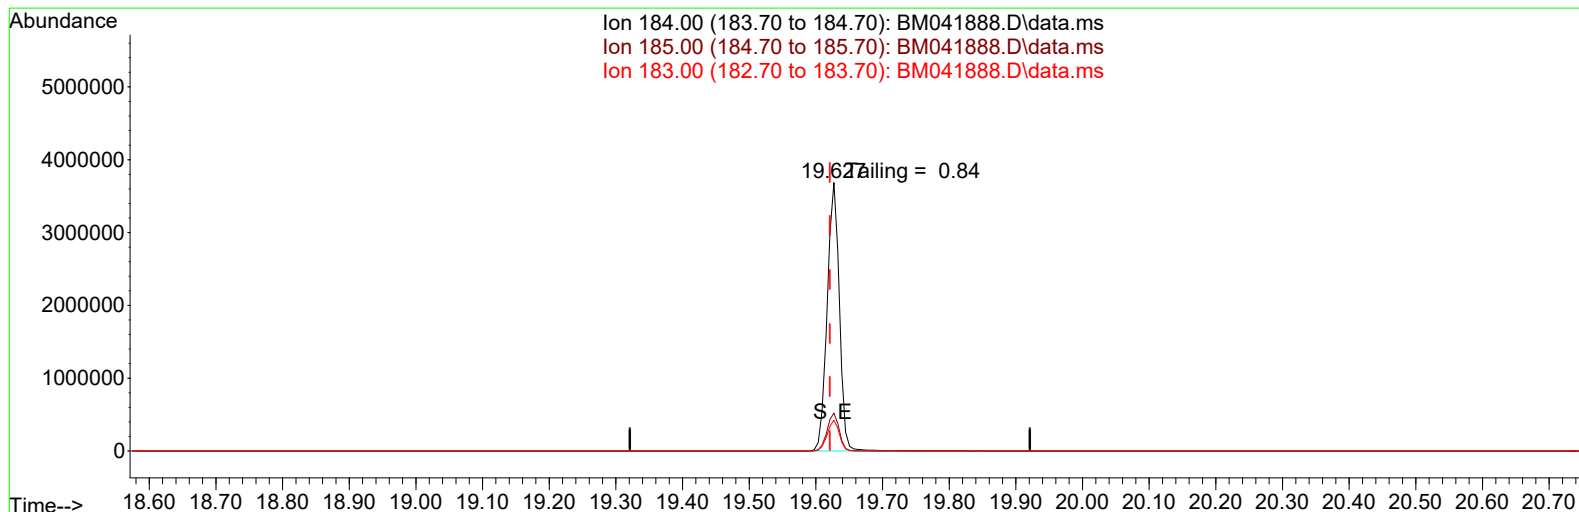

TIC: BM041888.D\data.ms

(77) Benzidine**19.627min (+ 0.006) 1203043.38 ng****response 4690282**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.13
183.00	11.40	11.47
0.00	0.00	0.00