

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041898.D
Acq On : 18 Sep 2023 16:53
Operator : MA/JU
Sample : PB155592BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155592BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	386	394	406	rBV	6762024	9729996	50.83%	10.818%
2	7.110	659	667	682	rBV	6182033	10379434	54.22%	11.540%
3	7.963	805	812	820	rBV	1157299	1762587	9.21%	1.960%
4	9.157	1005	1015	1027	rBV	4028019	6660913	34.79%	7.406%
5	10.781	1284	1291	1301	rBV	1480031	2458061	12.84%	2.733%
6	13.233	1700	1708	1715	rBV	9621480	14262400	74.50%	15.857%
7	14.610	1936	1942	1950	rBV	2210705	3286070	17.17%	3.653%
8	16.104	2189	2196	2214	rBV	7710700	11352440	59.30%	12.622%
9	17.363	2404	2410	2421	rBV	2699606	3825379	19.98%	4.253%
10	19.974	2848	2854	2859	rBV	15358342	19143997	100.00%	21.284%
11	21.539	3115	3120	3125	rBV	2835083	3647209	19.05%	4.055%
12	23.956	3524	3531	3541	rVB	1644382	3436287	17.95%	3.820%




Sum of corrected areas: 89944773

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041898.D
Acq On : 18 Sep 2023 16:53
Operator : MA/JU
Sample : PB155592BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155592BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

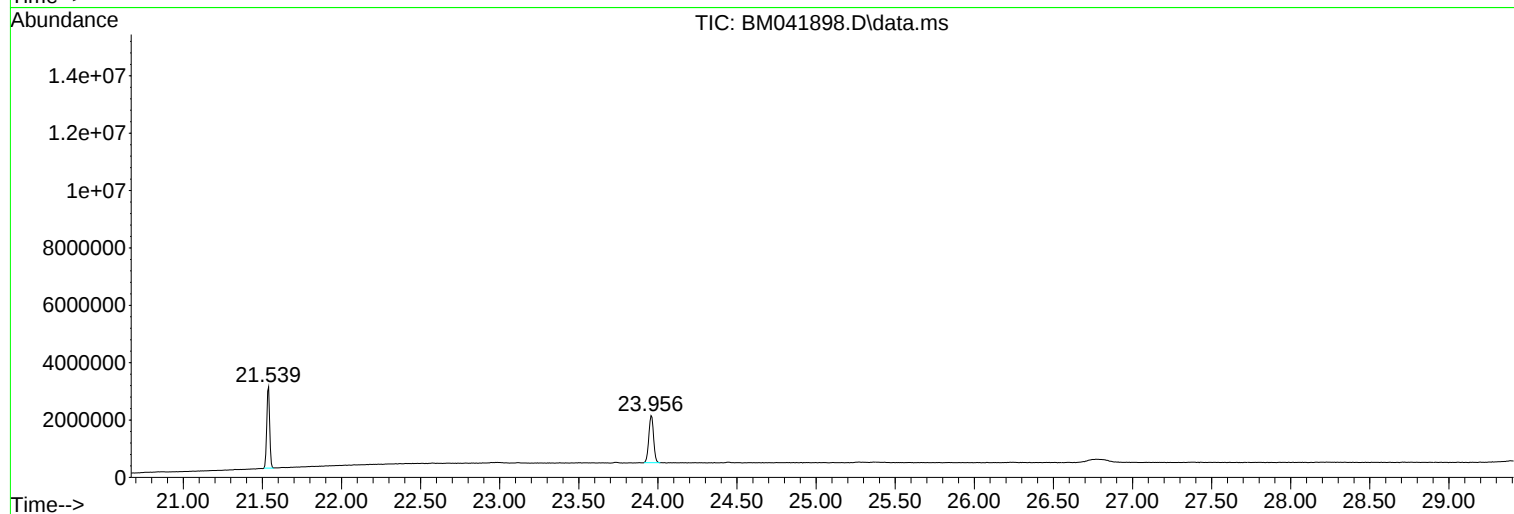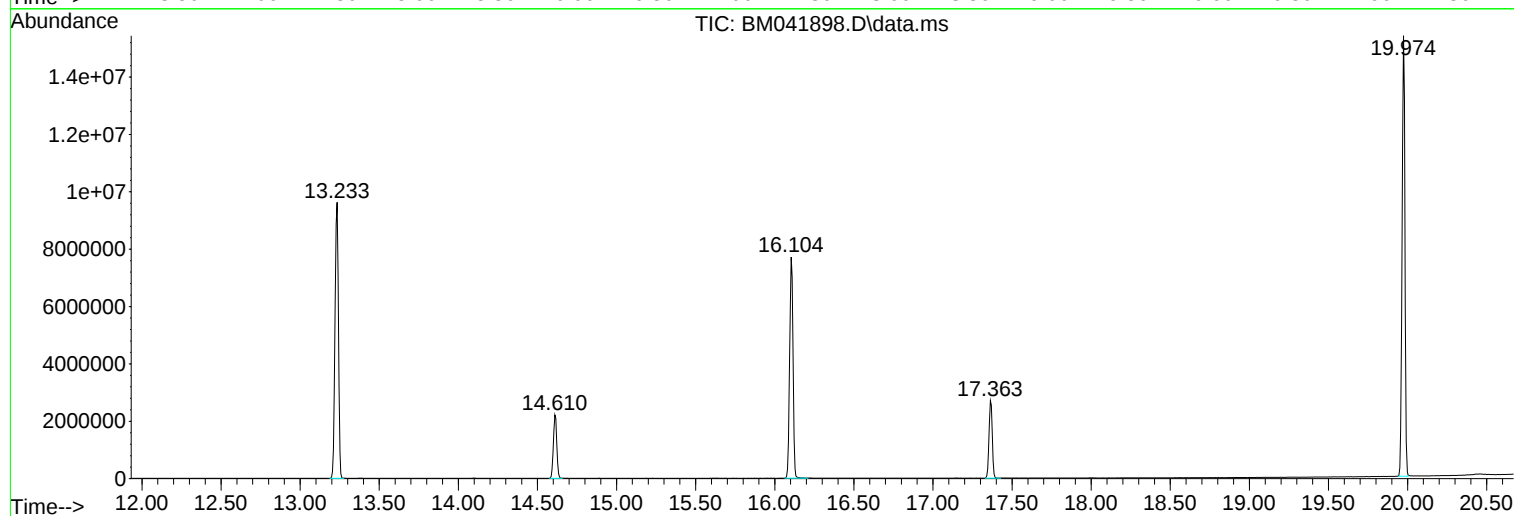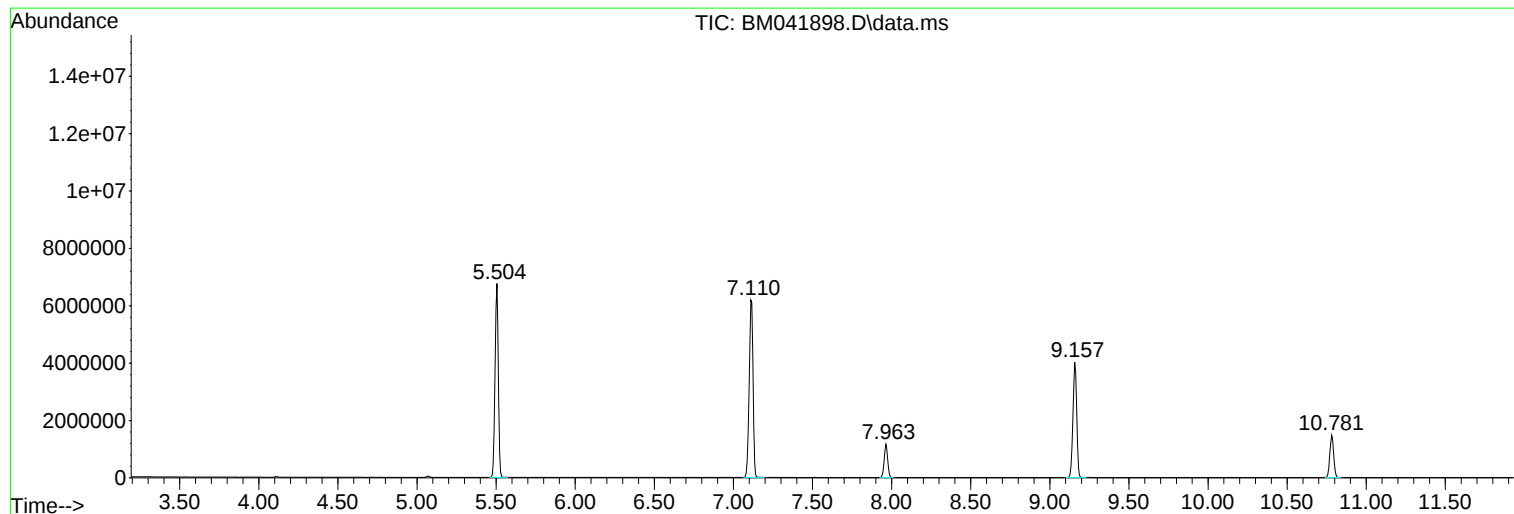

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041898.D
Acq On : 18 Sep 2023 16:53
Operator : MA/JU
Sample : PB155592BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155592BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041898.D
Acq On : 18 Sep 2023 16:53
Operator : MA/JU
Sample : PB155592BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155592BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------