
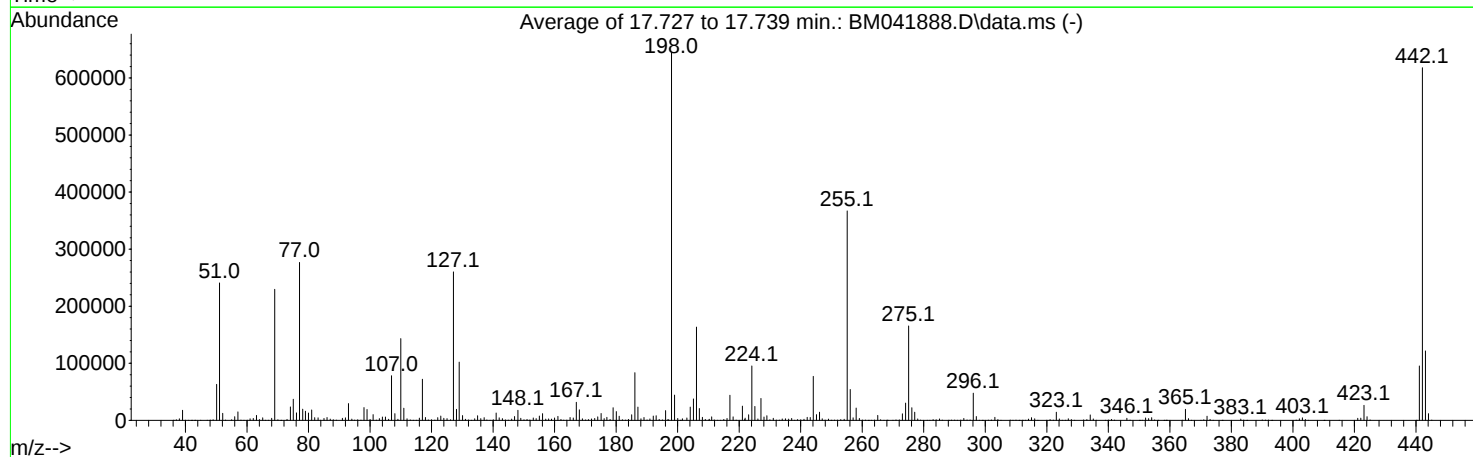


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
 Data File : BM041888.D
 Acq On : 18 Sep 2023 10:12
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 19 04:49:34 2023

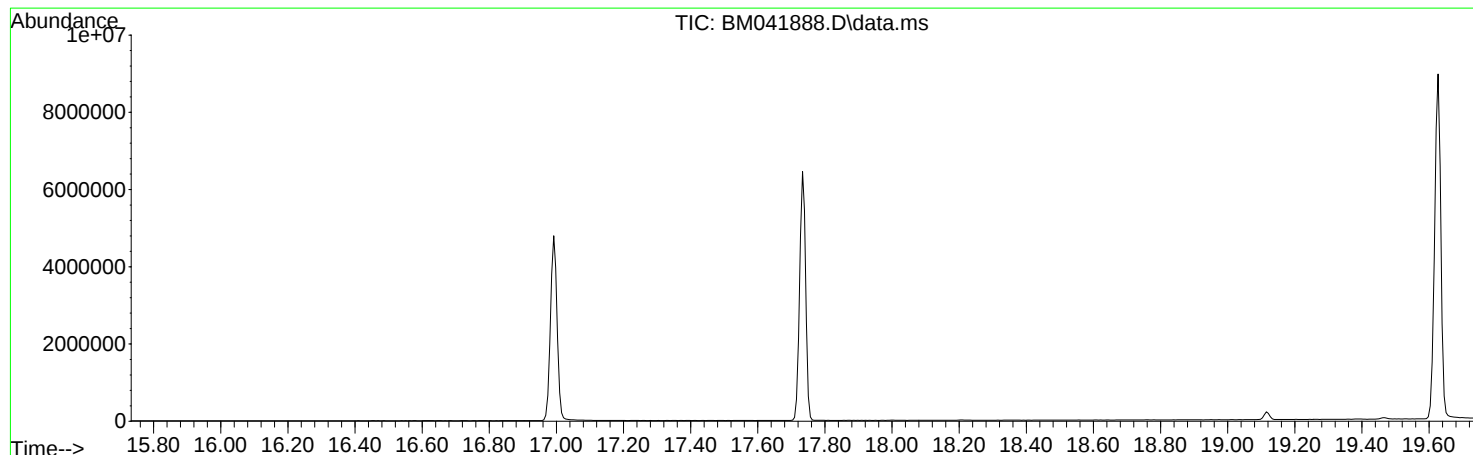




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	240964	PASS
68	69	0.00	2	1.6	3593	PASS
69	198	0.00	100	35.6	229632	PASS
70	69	0.00	2	0.5	1108	PASS
127	198	10	80	40.4	260139	PASS
197	198	0.00	2	0.3	1802	PASS
198	198	100	100	100.0	644629	PASS
199	198	5	9	6.9	44243	PASS
275	198	10	60	25.6	165312	PASS
365	198	1	100	3.0	19432	PASS
441	198	0.01	100	14.8	95333	PASS
442	442	50	100	100.0	617963	PASS
443	442	15	24	19.7	121712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041888.D
Acq On : 18 Sep 2023 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 19 05:46:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

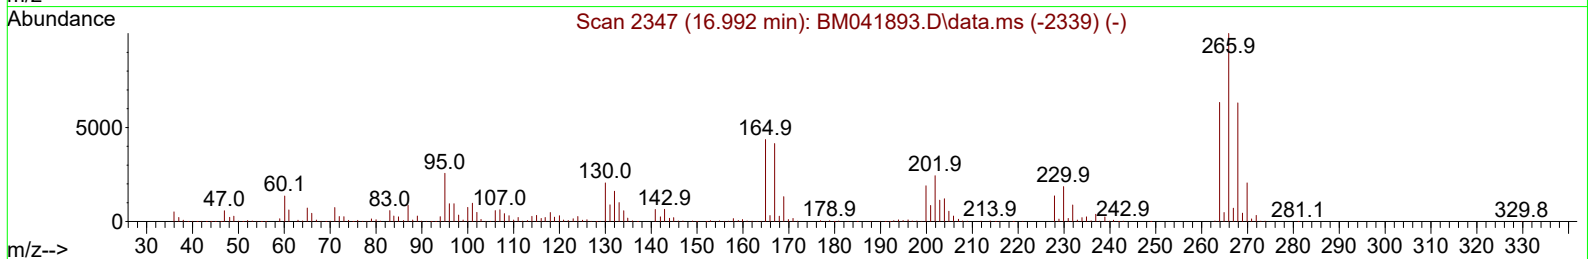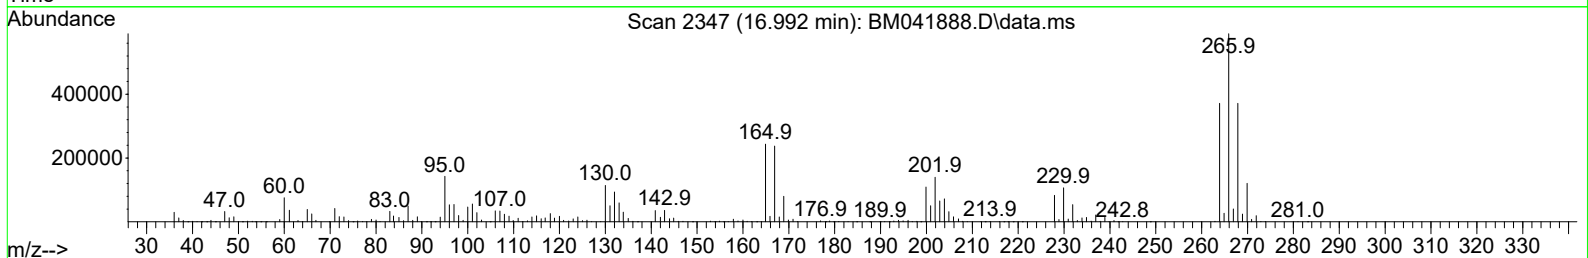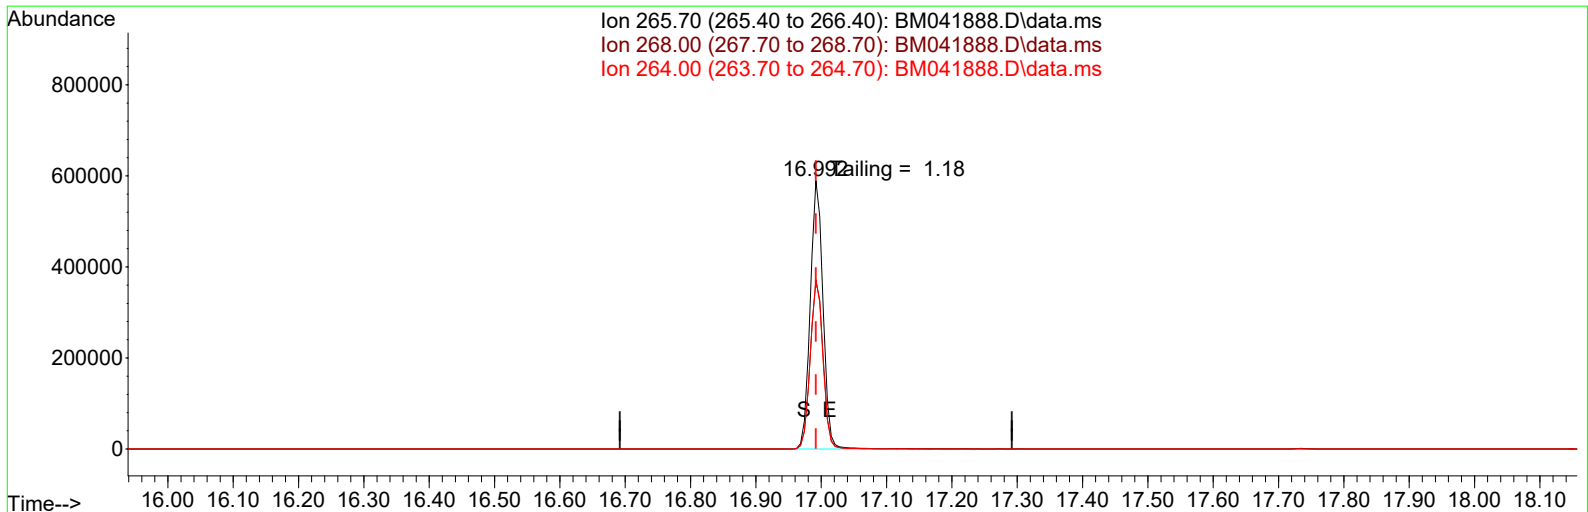

TIC: BM041888.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.000) 0.00 ng




response 802781

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.99
264.00	63.30	63.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091823\
Data File : BM041888.D
Acq On : 18 Sep 2023 10:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 19 05:46:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

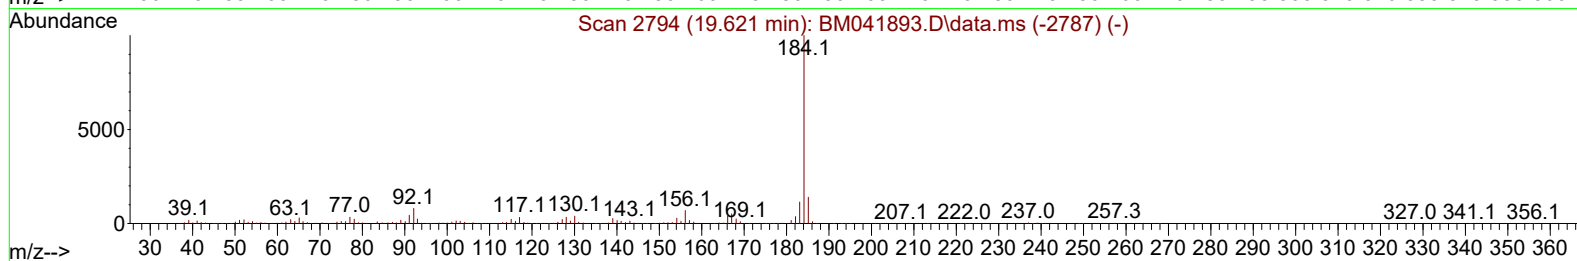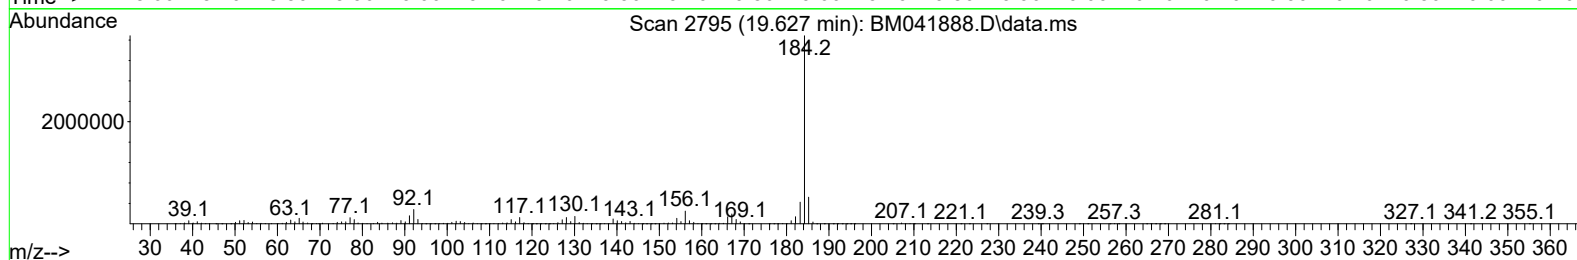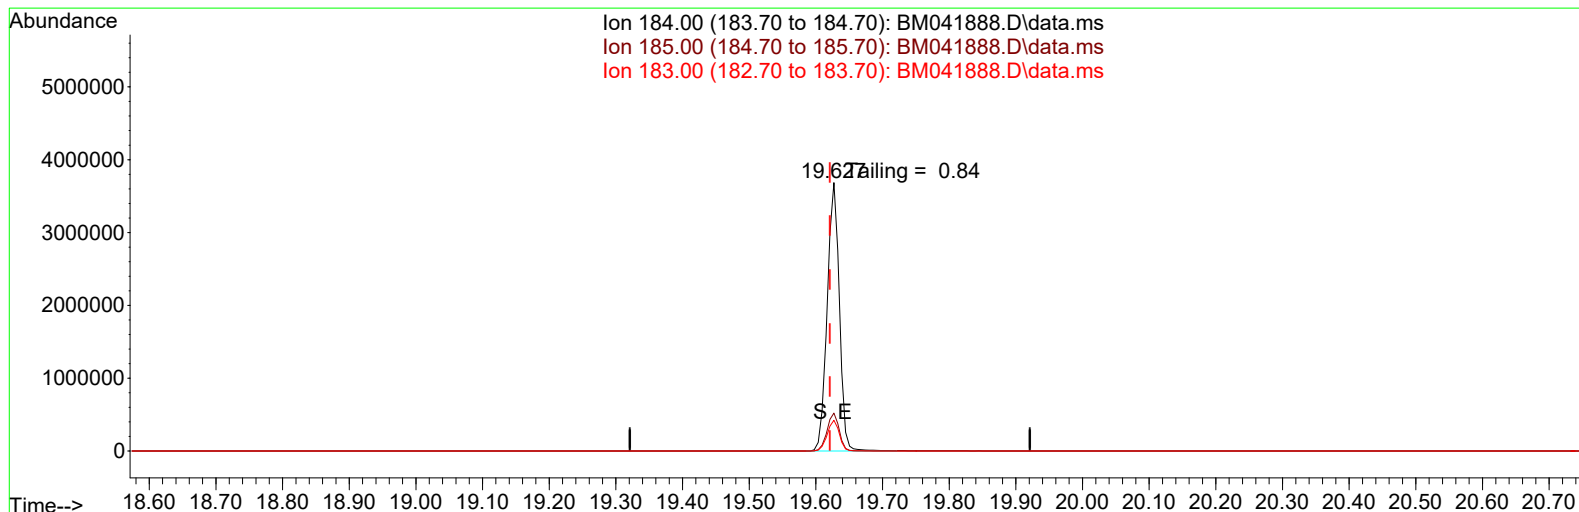

TIC: BM041888.D\data.ms

(77) Benzidine

19.627min (+ 0.006) 1203043.38 ng

response 4690282

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.13
183.00	11.40	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2023	BNA_M	<u>BM041888.D</u>
Compound Name	Response	Retention Time
DDT	2277458	20.821
DDD	26913	20.427
DDE	376	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27289	2304747	1.18

Instrument :
BNA_M
ClientSampleId :
DFTPP