

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091918\
 Data File : BM016793.D
 Acq On : 19 Sep 2018 12:51
 Operator : SJ/JU
 Sample : PB112992BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 20 01:55:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 20 01:54:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	256981	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1063767	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	556386	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	1181664	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	1262442	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1340534	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.27	96	30263	5.04	ng/uL	0.00
5) Phenol-d5	6.89	99	531429	24.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	338672	25.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	449659	25.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	422008	25.16	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	205327	29.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	191224	30.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	400191	24.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.64	131	456530	23.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1176980	26.35	ng/ul	0.00
47) Acenaphthylene-d8	14.06	160	1414345	24.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	163359	22.28	ng/ul	0.00
58) Fluorene-d10	15.36	176	1032891	26.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	108492	22.37	ng/ul	0.00
71) Anthracene-d10	17.21	188	1583633	27.78	ng/ul	0.00
79) Pyrene-d10	19.50	212	1717922	28.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	1918129	27.43	ng/ul	0.00


Target Compounds					Ovalue	
46) 2,6-Dinitrotoluene	13.78	165	8036	1.198	ng/ul#	41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091918\
Data File : BM016793.D
Acq On : 19 Sep 2018 12:51
Operator : SJ/JU
Sample : PB112992BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 20 01:55:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 20 01:54:47 2018
Response via : Initial Calibration

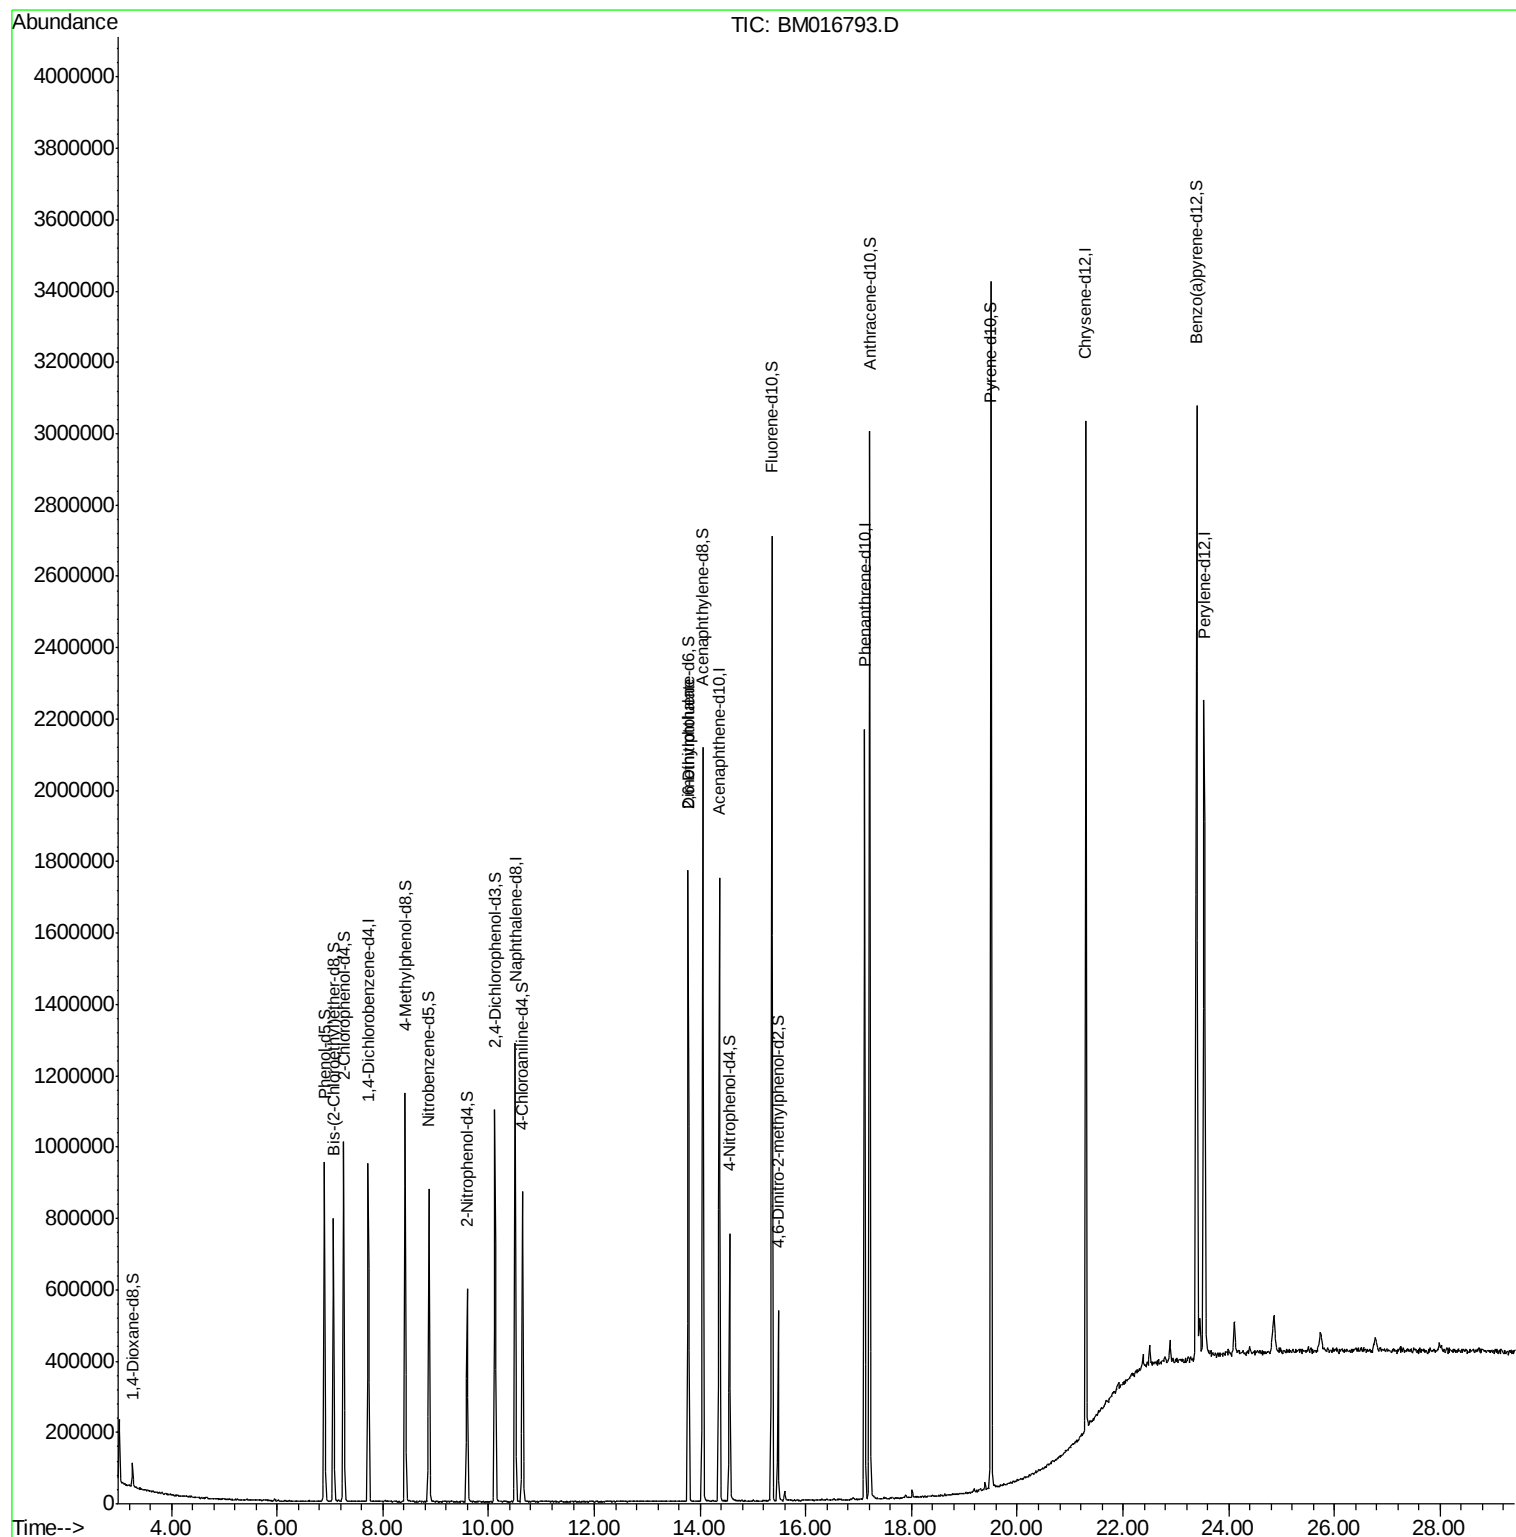

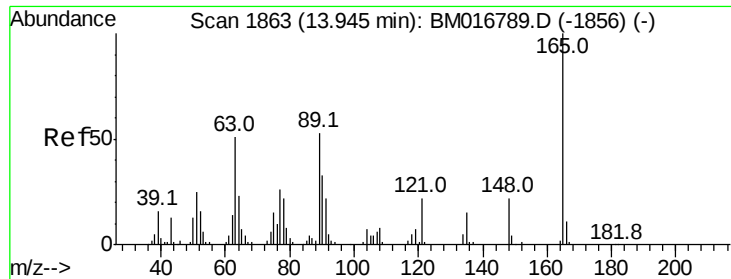

#46

2,6-Dinitrotoluene

Concen: 1.198 ng/ul

RT: 13.78 min Scan# 1835

Delta R.T. -0.16 min

Lab File: BM016793.D

Acq: 19 Sep 2018 12:51

Instrument :

BNA_M

ClientSampleId :


Tot Ion:165 Resp: 8036

Ion Ratio Lower Upper

165 100

89 0.0 43.8 65.8#

121 30.9 17.8 26.6#

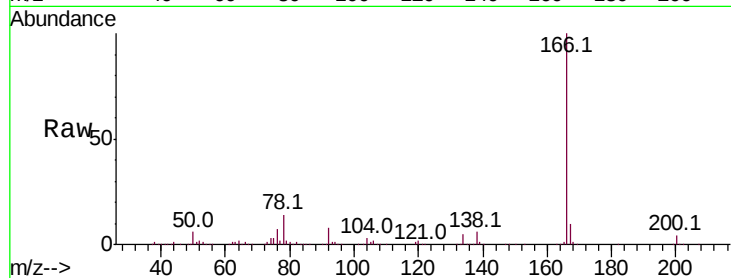

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

