

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091918\
 Data File : BM016804.D
 Acq On : 19 Sep 2018 20:02
 Operator : SJ/JU
 Sample : J4896-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C08M4

Quant Time: Sep 20 03:07:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Sep 20 03:06:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	261760	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1067903	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	580259	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.11	188	1337098	20.00	ng/ul	0.00
78) Chrysene-d12	21.30	240	1575437	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1705827	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	52726	8.61	ng/uL	0.00
5) Phenol-d5	6.89	99	450528	20.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	282313	20.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	384818	21.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	359090	21.02	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	172099	24.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	157365	24.67	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	342776	21.15	ng/ul	0.00
29) 4-Chloroaniline-d4	10.64	131	443523	22.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1020308	21.90	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	1196357	19.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.56	143	175462	22.95	ng/ul	0.00
58) Fluorene-d10	15.36	176	930440	22.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	111297	20.28	ng/ul	0.00
71) Anthracene-d10	17.21	188	1595887	24.74	ng/ul	0.00
79) Pyrene-d10	19.50	212	1870459	24.47	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	2203826	24.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.82	163	160242	3.519	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM091918\
Data File : BM016804.D
Acq On : 19 Sep 2018 20:02
Operator : SJ/JU
Sample : J4896-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C08M4

Quant Time: Sep 20 03:07:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Sep 20 03:06:22 2018
Response via : Initial Calibration

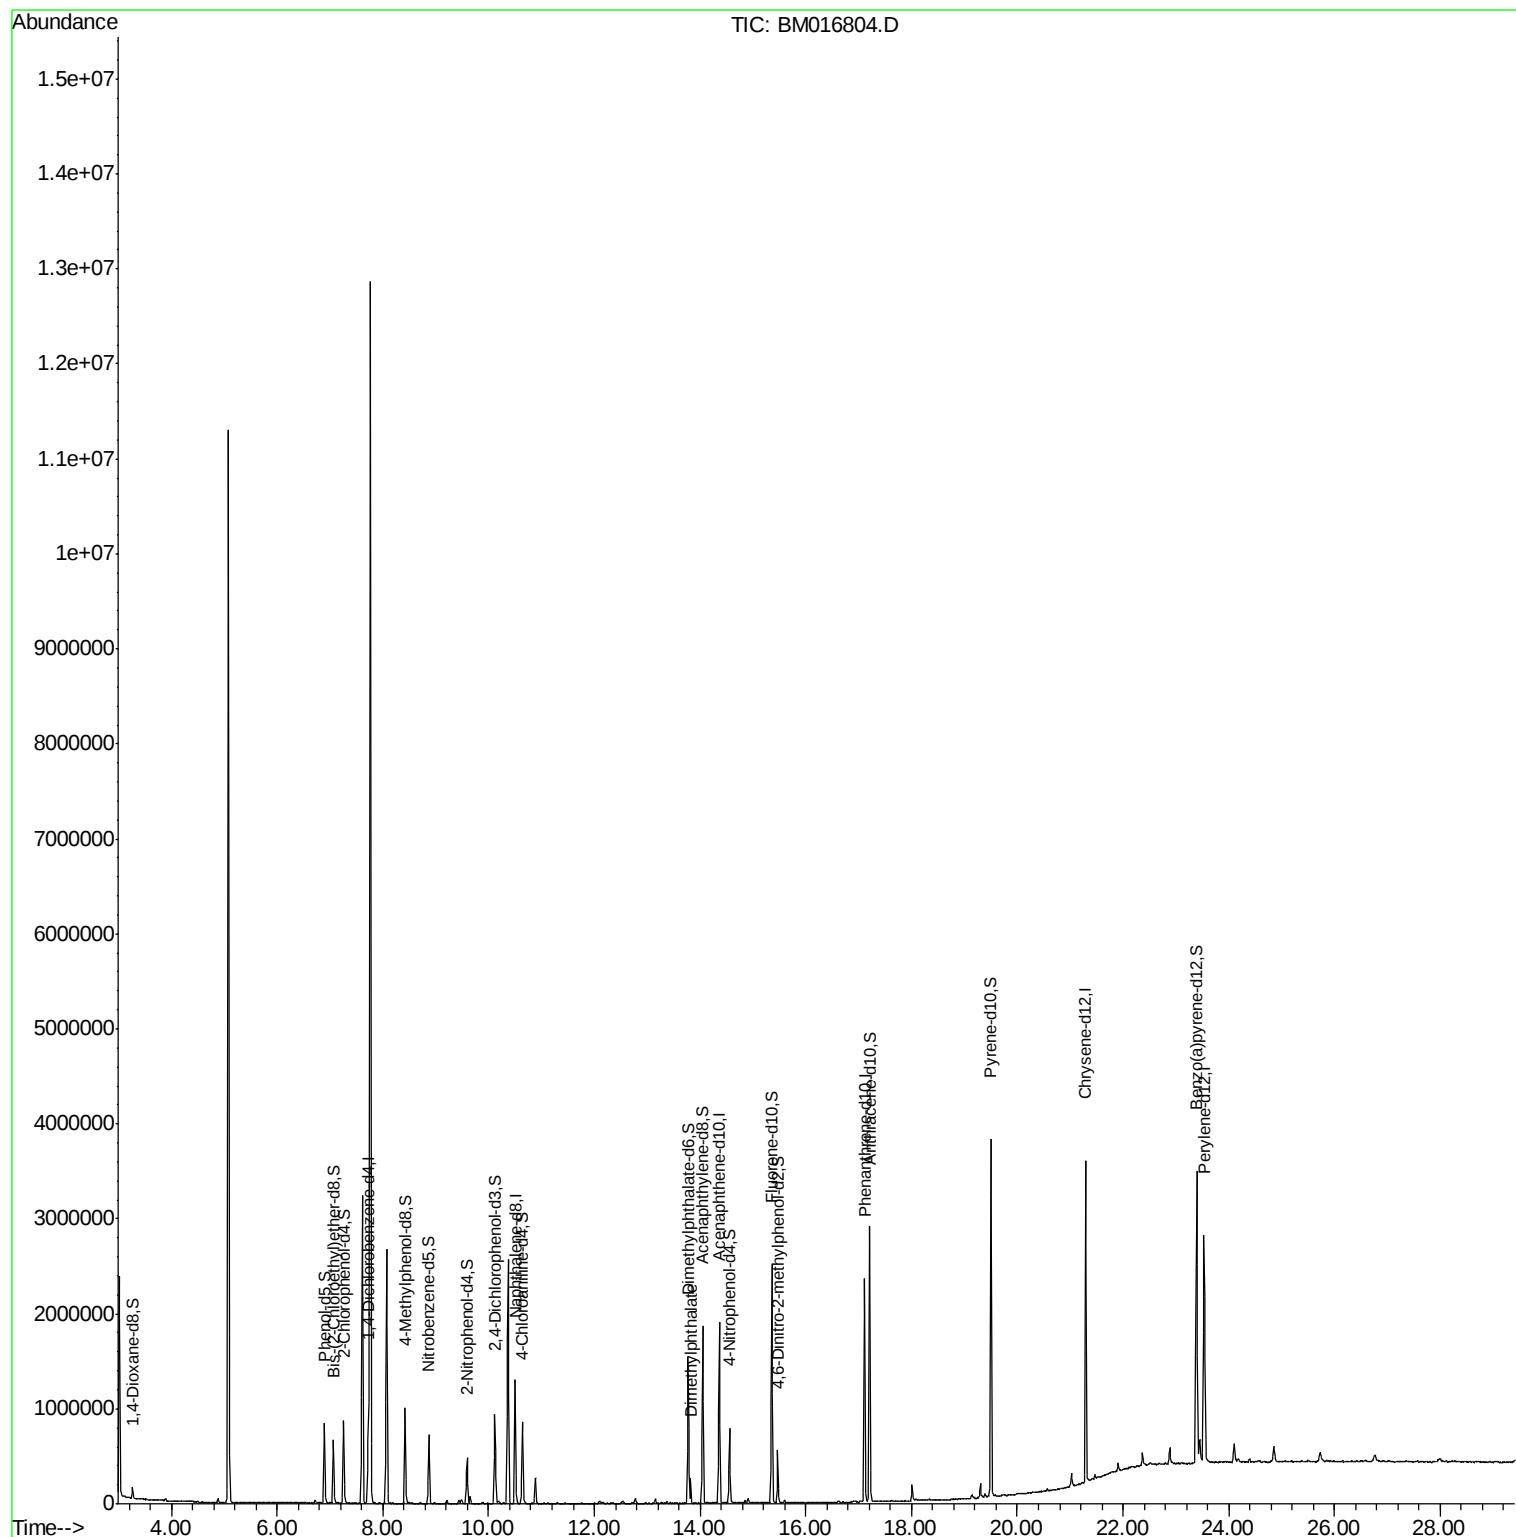

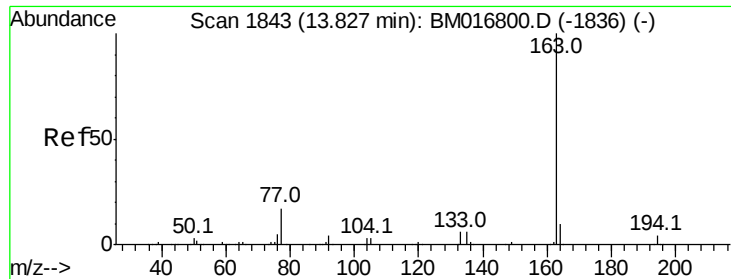

#45

Dimethylphthalate

Concen: 3.519 ng/ul

RT: 13.82 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM016804.D

Acq: 19 Sep 2018 20:02

Instrument :

BNA_M

ClientSampleId :

C08M4


Tot Ion:163 Resp: 160242

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 10.9 8.4 12.6

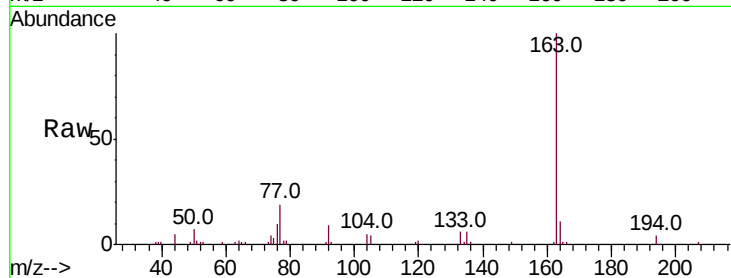

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

