
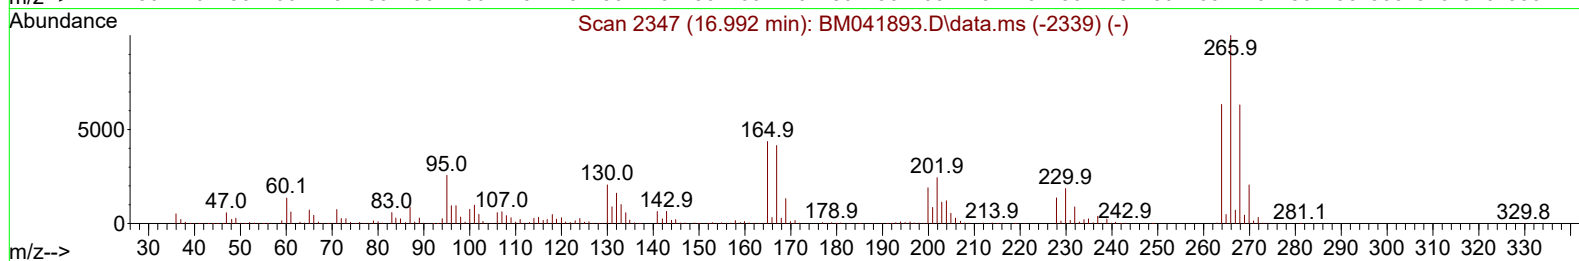
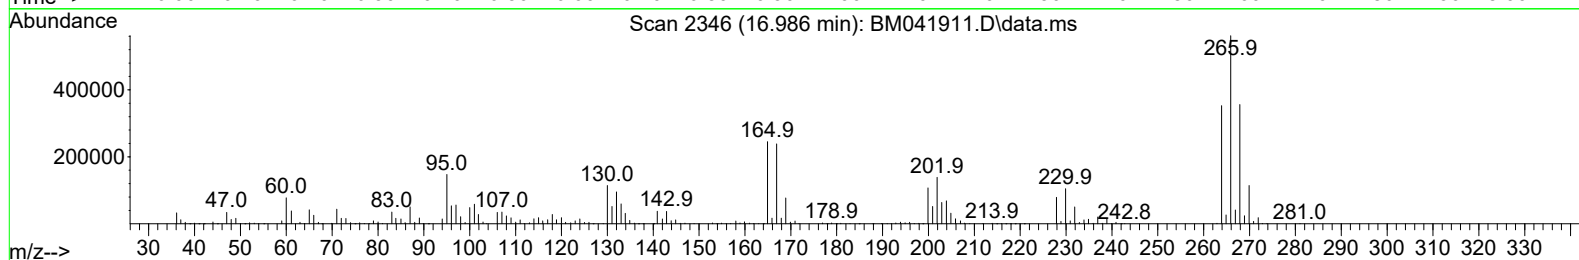


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041911.D
Acq On : 19 Sep 2023 20:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 05:55:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

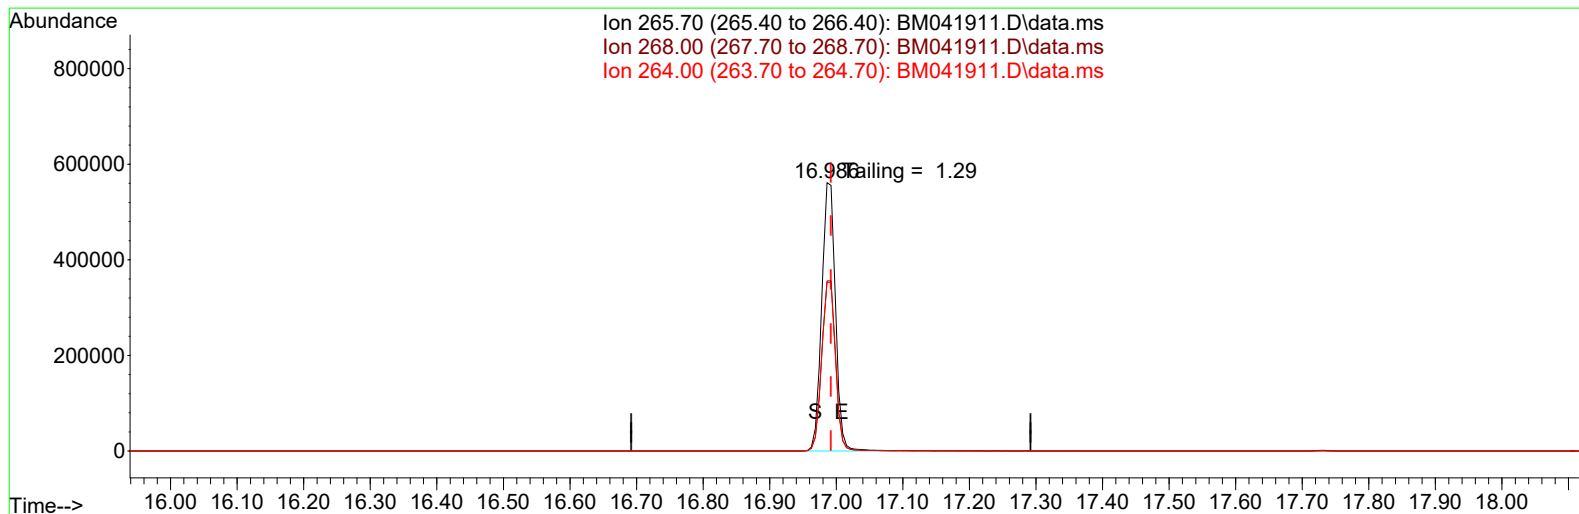

TIC: BM041911.D\data.ms

(70) Pentachlorophenol (C)




16.986min (-0.006) 220073.29 ng

response 807320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.39
264.00	63.30	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041911.D
Acq On : 19 Sep 2023 20:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 05:55:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

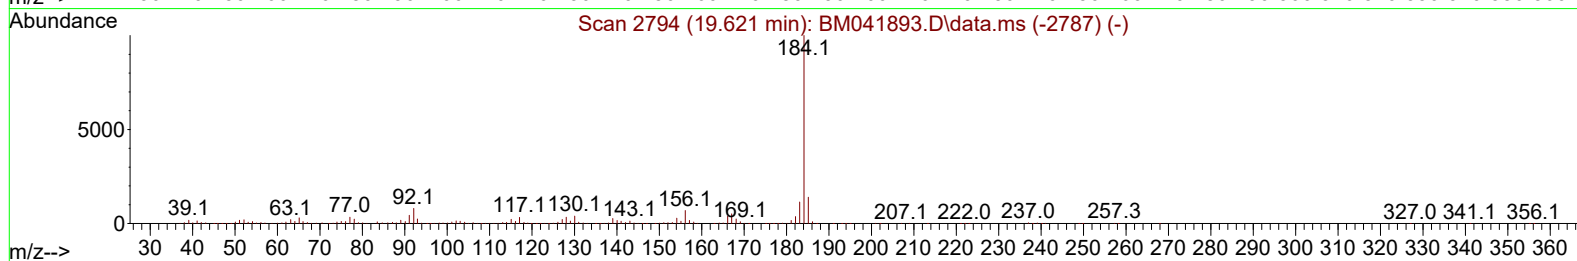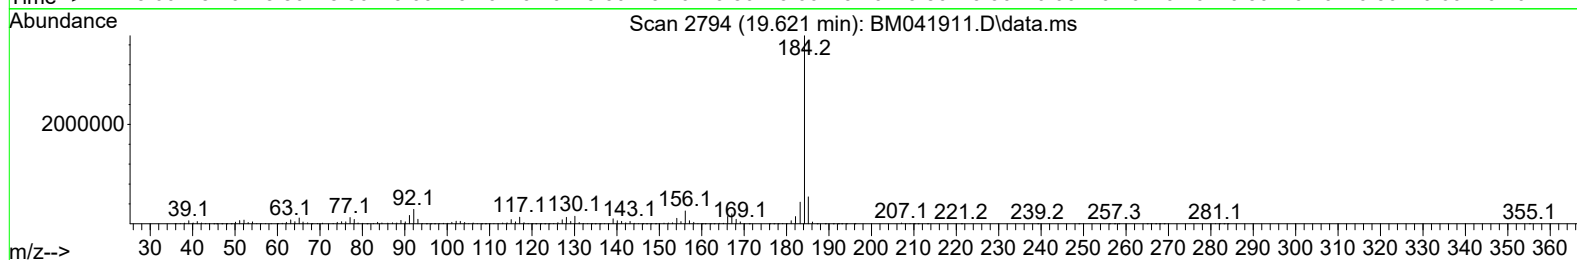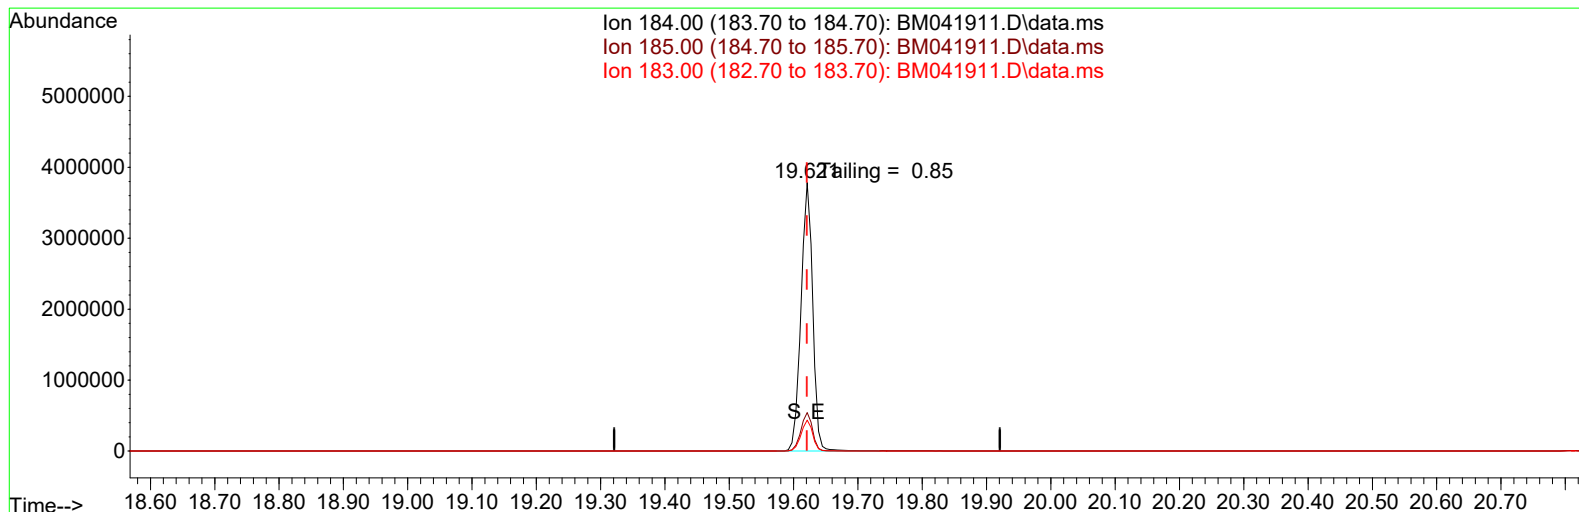

TIC: BM041911.D\data.ms

(77) Benzidine**19.621min (+ 0.000) 228492.28 ng****response 4789898**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.30
183.00	11.40	11.53
0.00	0.00	0.00