

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
 Data File : BM041901.D
 Acq On : 19 Sep 2023 09:16
 Operator : MA/JU
 Sample : PB155456BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB155456BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.064	314	319	326	rBV	233380	330776	1.72%	0.366%
2	5.505	386	394	405	rBV	6838434	9961881	51.79%	11.023%
3	7.110	658	667	684	rBV	6383655	10602872	55.13%	11.732%
4	7.963	804	812	819	rBV	1107418	1692270	8.80%	1.872%
5	9.157	1006	1015	1026	rBV	4107919	6777855	35.24%	7.500%
6	10.781	1282	1291	1302	rBV	1435666	2368195	12.31%	2.620%
7	13.228	1700	1707	1716	rBV	9667812	14621281	76.02%	16.178%
8	14.610	1935	1942	1952	rBV	2195701	3167147	16.47%	3.504%
9	16.104	2189	2196	2211	rBV	7948721	11506099	59.82%	12.731%
10	17.363	2403	2410	2419	rBV	2650935	3687211	19.17%	4.080%
11	19.974	2847	2854	2859	rBV	15026209	19233973	100.00%	21.282%
12	21.533	3114	3119	3125	rBV	2733722	3384114	17.59%	3.744%
13	23.951	3524	3530	3539	rVB	1475772	3043651	15.82%	3.368%




Sum of corrected areas: 90377325

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041901.D
Acq On : 19 Sep 2023 09:16
Operator : MA/JU
Sample : PB155456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155456BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

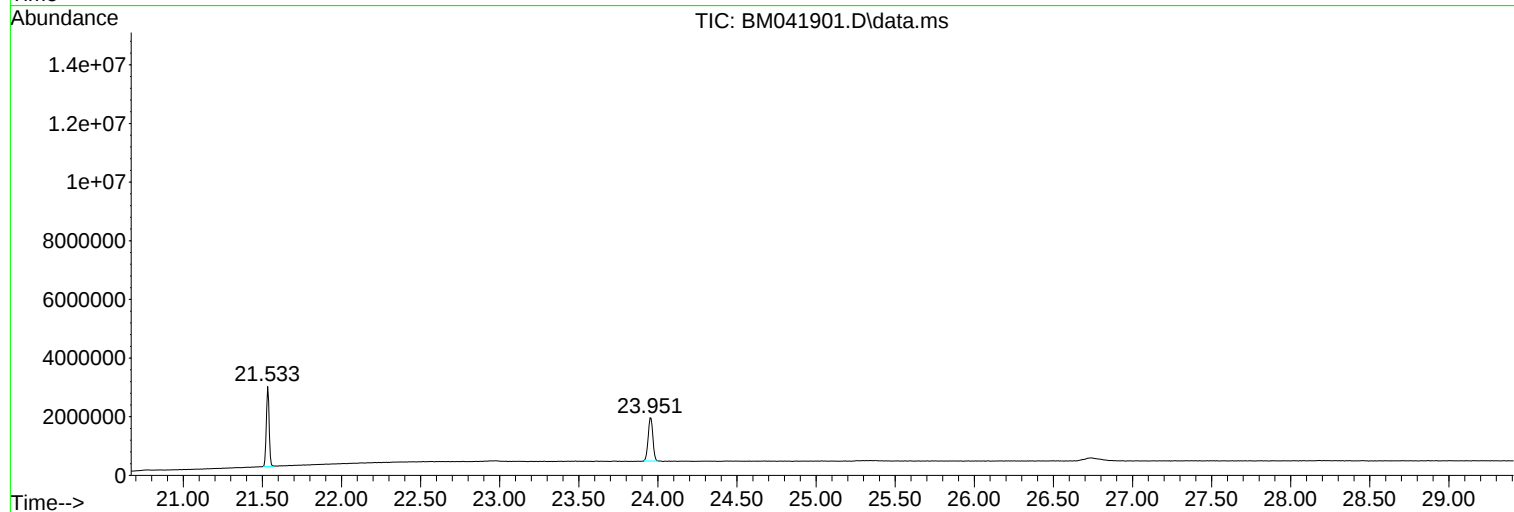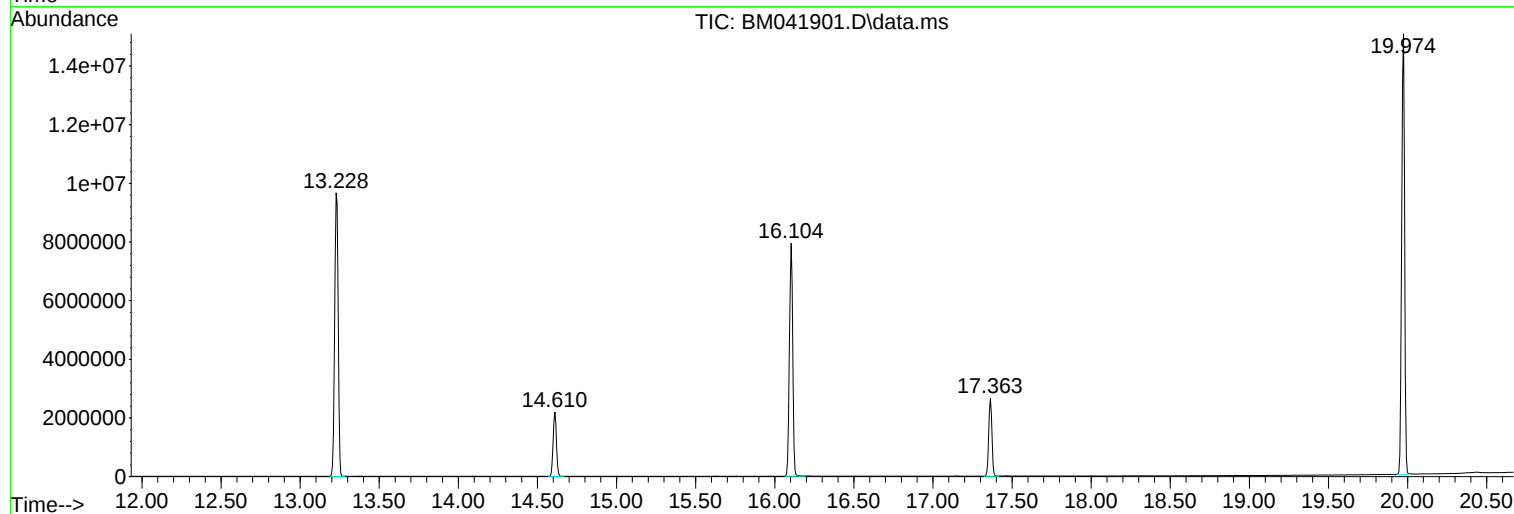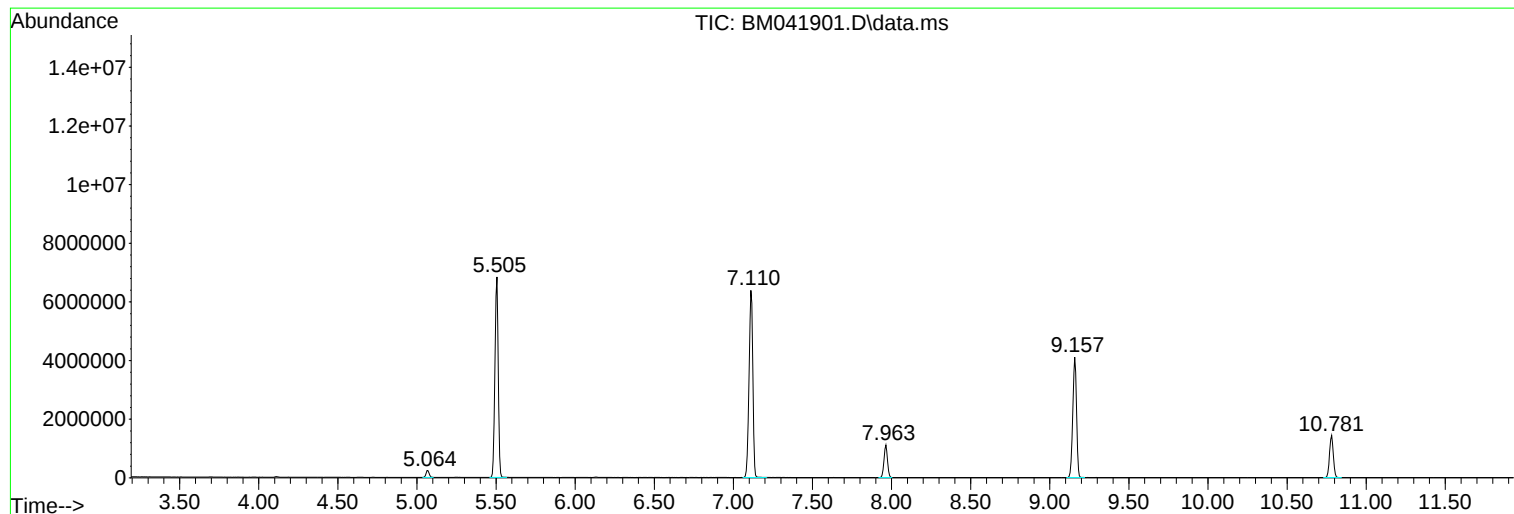

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041901.D
Acq On : 19 Sep 2023 09:16
Operator : MA/JU
Sample : PB155456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB155456BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.064	3.91 ng	330776	1,4-Dichlorobenzene-d4	7.963	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9

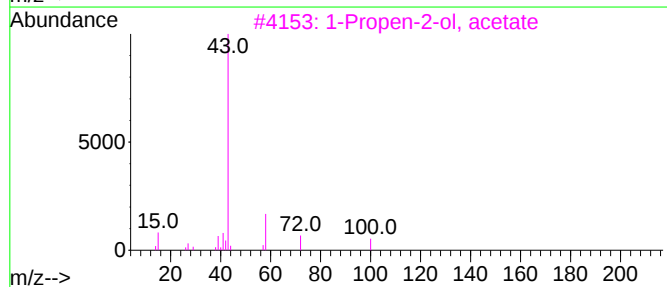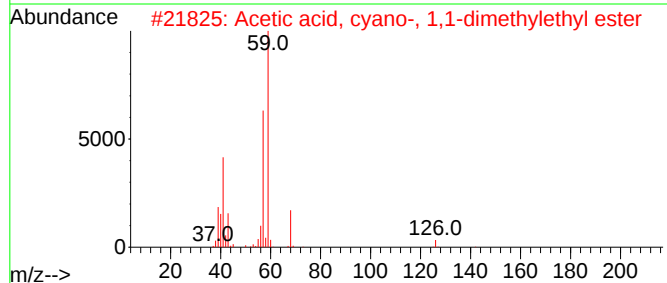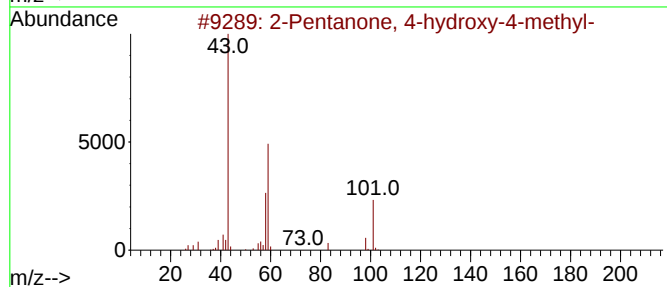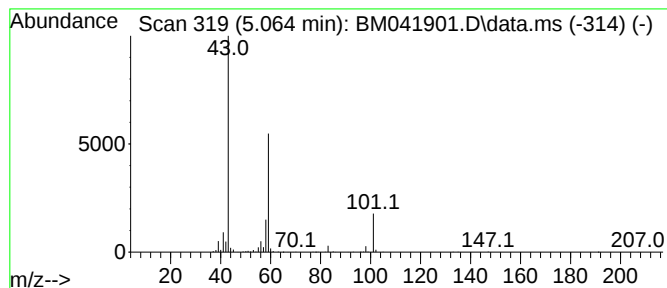

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041901.D
Acq On : 19 Sep 2023 09:16
Operator : MA/JU
Sample : PB155456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155456BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.064	3.9	ng	330776	1	7.963	1692270	20.0