

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
 Data File : BM041916.D
 Acq On : 19 Sep 2023 23:15
 Operator : MA/JU
 Sample : PB155451BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB155451BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.058	312	318	333	rVB	3033876	4275366	23.11%	5.344%
2	5.499	386	393	406	rBV	4350815	6384784	34.51%	7.981%
3	7.104	658	666	677	rBV	4203942	6790272	36.70%	8.488%
4	7.963	805	812	820	rBV	1074584	1652921	8.93%	2.066%
5	9.157	1006	1015	1025	rBV	3877953	6301095	34.05%	7.877%
6	10.781	1283	1291	1302	rBV	1384312	2301526	12.44%	2.877%
7	13.228	1699	1707	1718	rBV	9203893	13549479	73.23%	16.937%
8	14.610	1934	1942	1957	rBV	2102178	3069316	16.59%	3.837%
9	16.098	2188	2195	2214	rBV	4795605	6909282	37.34%	8.637%
10	17.363	2403	2410	2420	rBV	2534749	3612863	19.53%	4.516%
11	19.968	2847	2853	2858	rBV	14704299	18503777	100.00%	23.130%
12	21.533	3113	3119	3128	rBV	2694105	3504555	18.94%	4.381%
13	23.945	3523	3529	3538	rVB	1544585	3143308	16.99%	3.929%




Sum of corrected areas: 79998544

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041916.D
Acq On : 19 Sep 2023 23:15
Operator : MA/JU
Sample : PB155451BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155451BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

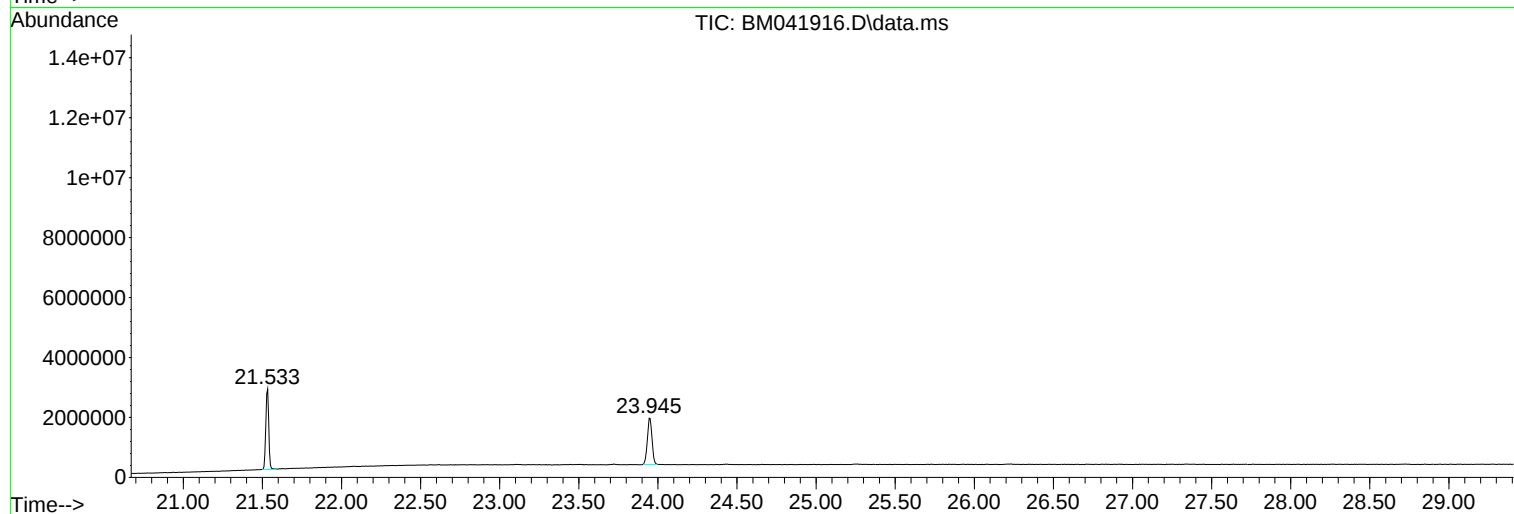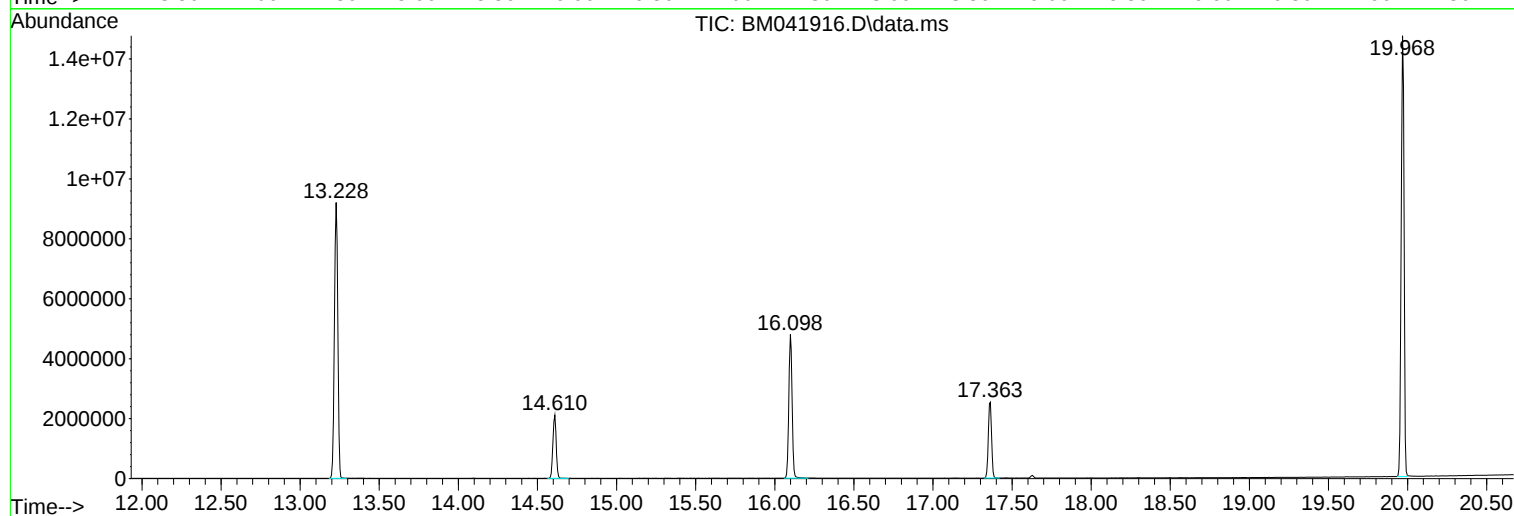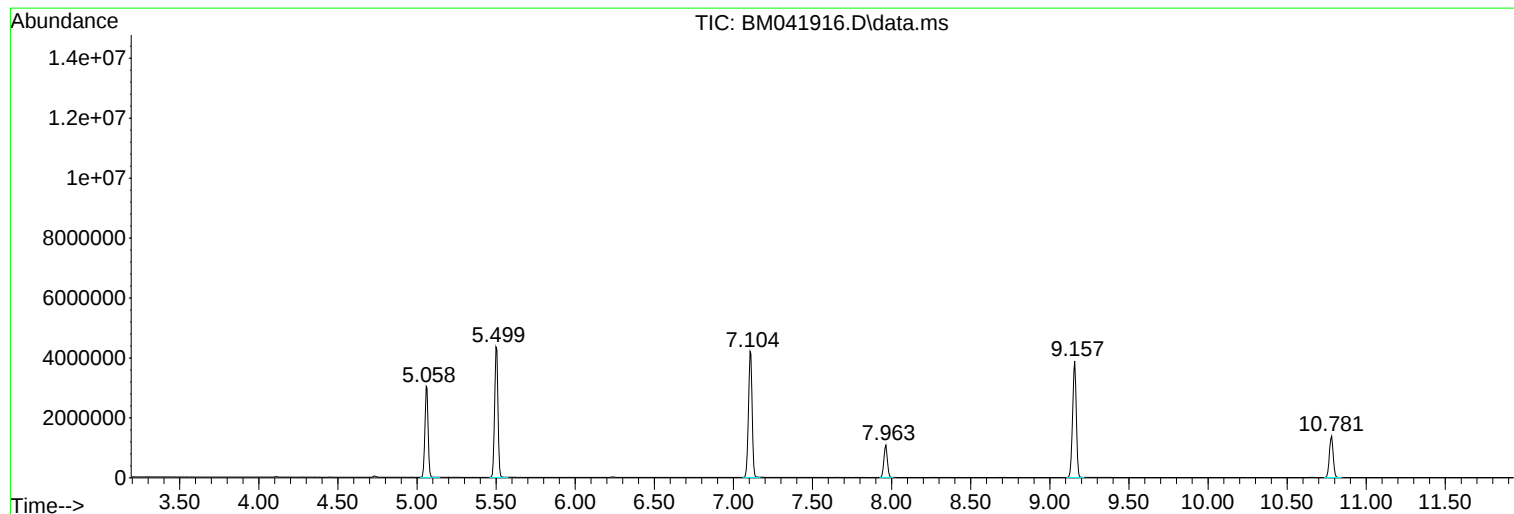

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041916.D
Acq On : 19 Sep 2023 23:15
Operator : MA/JU
Sample : PB155451BL
Misc :
ALS Vial : 16 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB155451BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.058	51.73 ng	4275370	1,4-Dichlorobenzene-d4	7.963	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	9

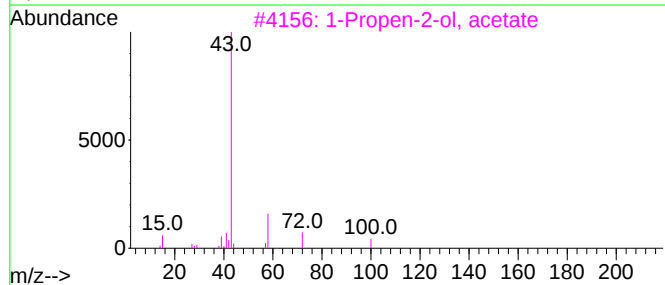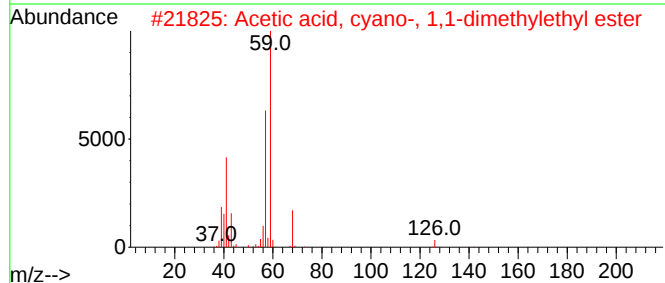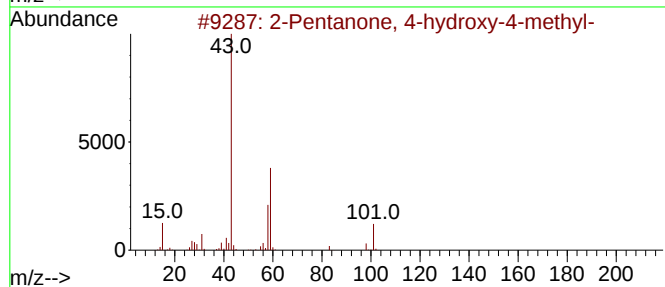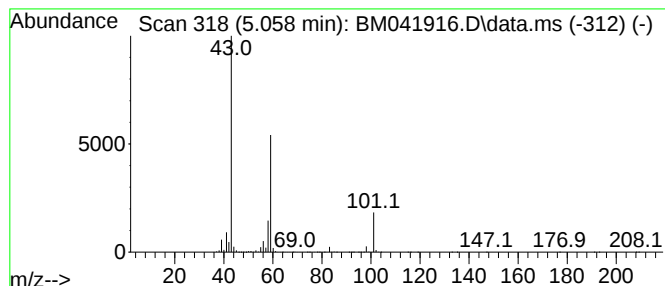

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041916.D
Acq On : 19 Sep 2023 23:15
Operator : MA/JU
Sample : PB155451BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155451BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.058	51.7	ng	4275370	1	7.963	1652920	20.0