
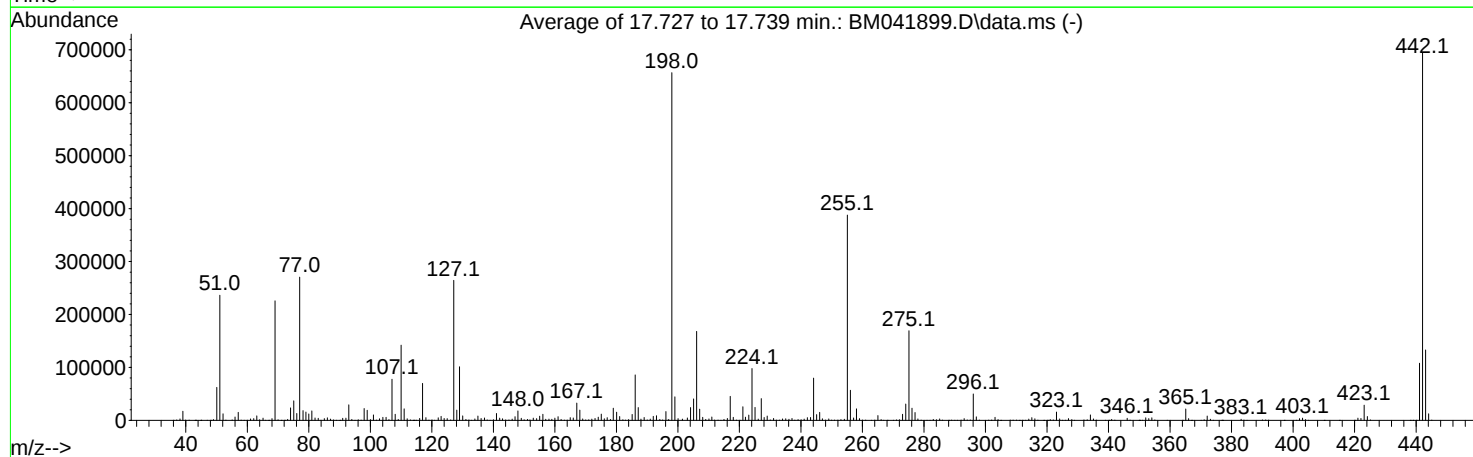


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
 Data File : BM041899.D
 Acq On : 19 Sep 2023 08:02
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 19 04:49:34 2023

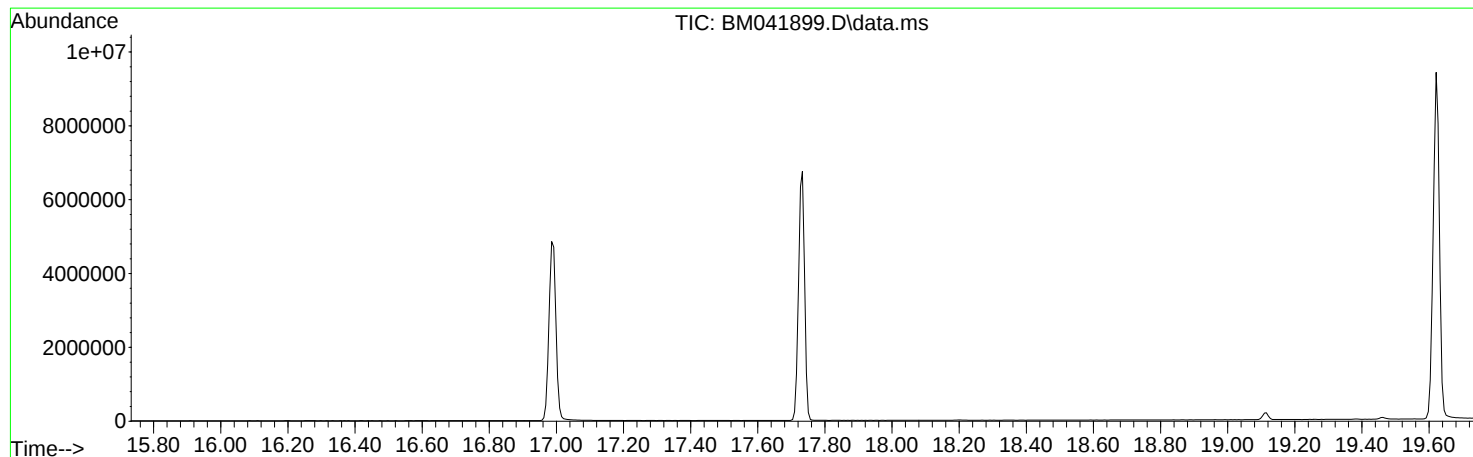




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	236498	PASS
68	69	0.00	2	1.4	3240	PASS
69	198	0.00	100	34.4	225856	PASS
70	69	0.00	2	0.5	1105	PASS
127	198	10	80	40.3	264427	PASS
197	198	0.00	2	0.2	1557	PASS
198	198	100	100	100.0	656811	PASS
199	198	5	9	6.7	44291	PASS
275	198	10	60	25.8	169141	PASS
365	198	1	100	3.3	21563	PASS
441	198	0.01	100	16.4	107907	PASS
442	442	50	100	100.0	694848	PASS
443	442	15	24	19.1	132925	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
Data File : BM041899.D
Acq On : 19 Sep 2023 08:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 19 11:27:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

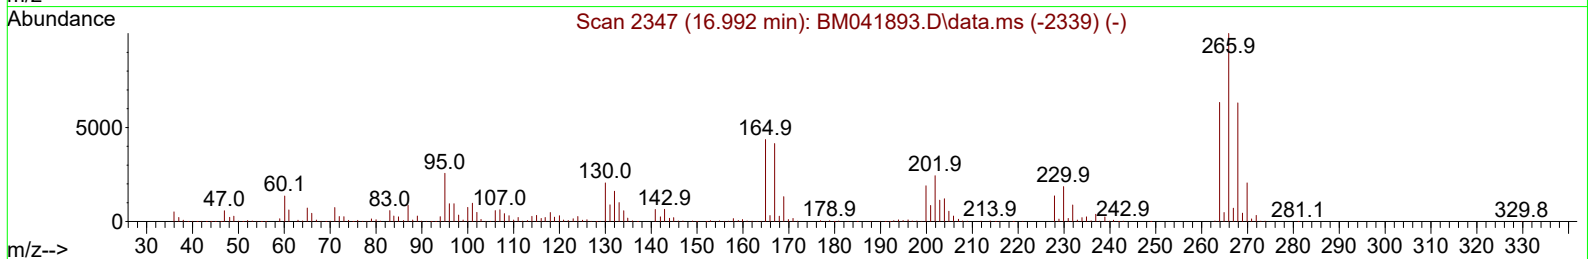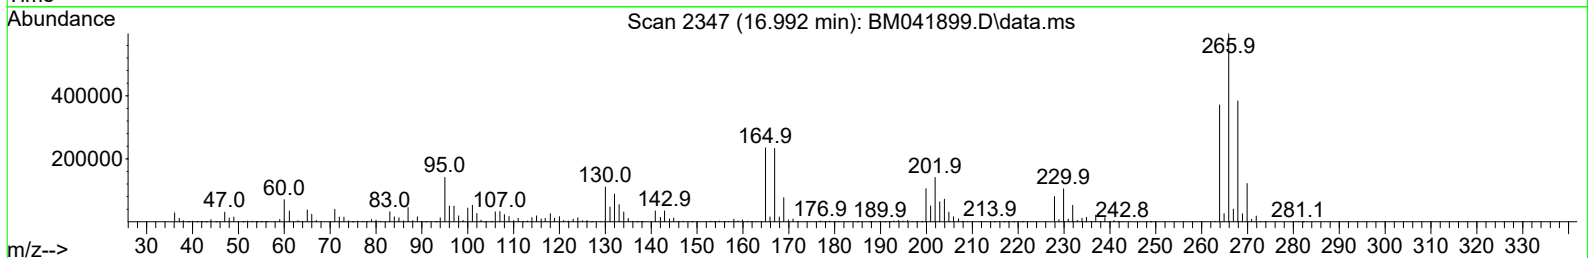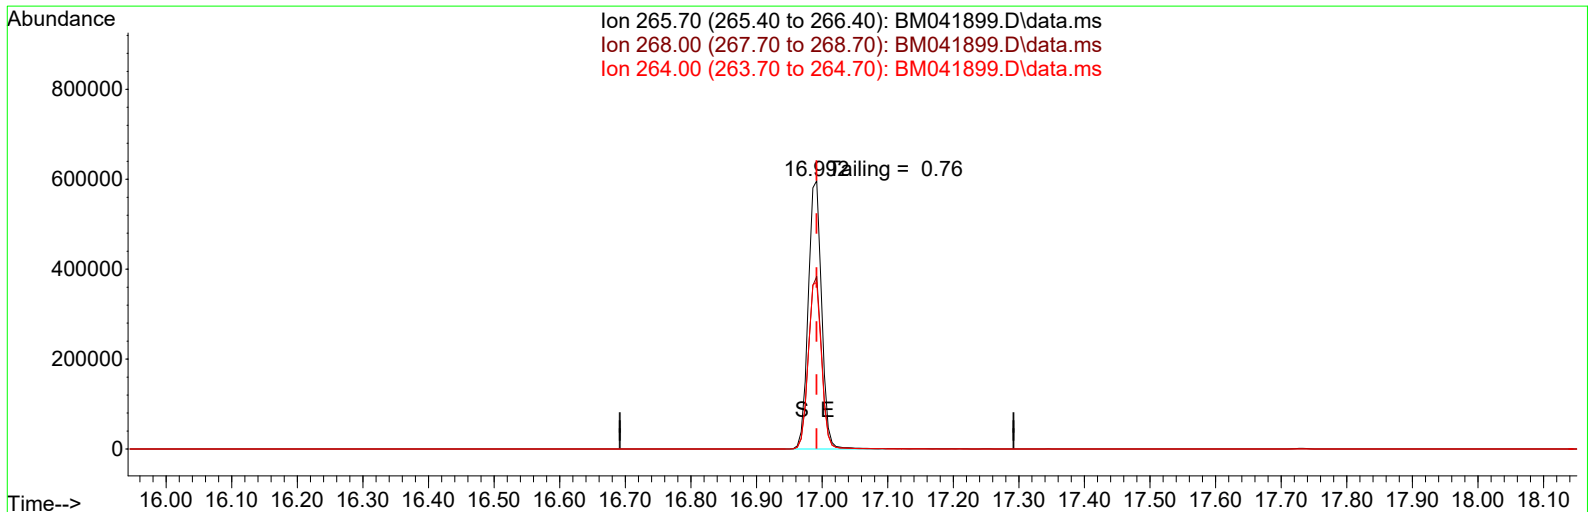

TIC: BM041899.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.000) 0.00 ng




response 850128

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.27
264.00	63.30	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM091923\
 Data File : BM041899.D
 Acq On : 19 Sep 2023 08:02
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Sep 19 11:27:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 19 04:49:34 2023
 Response via : Initial Calibration

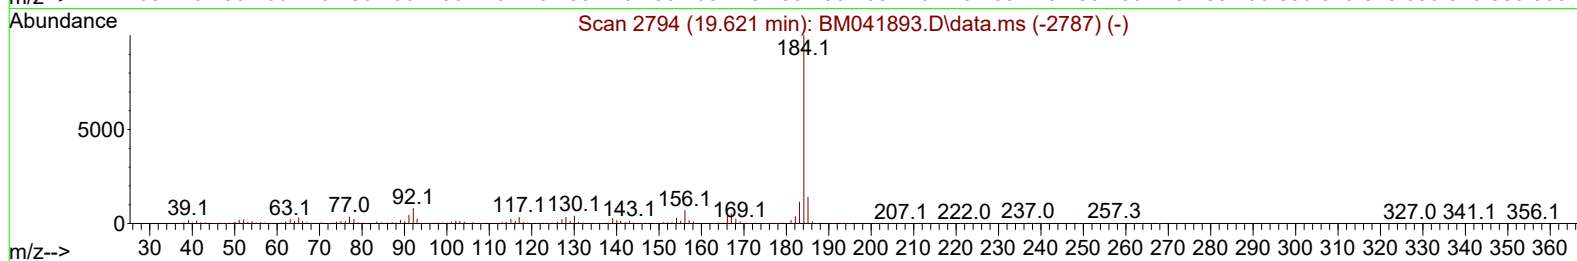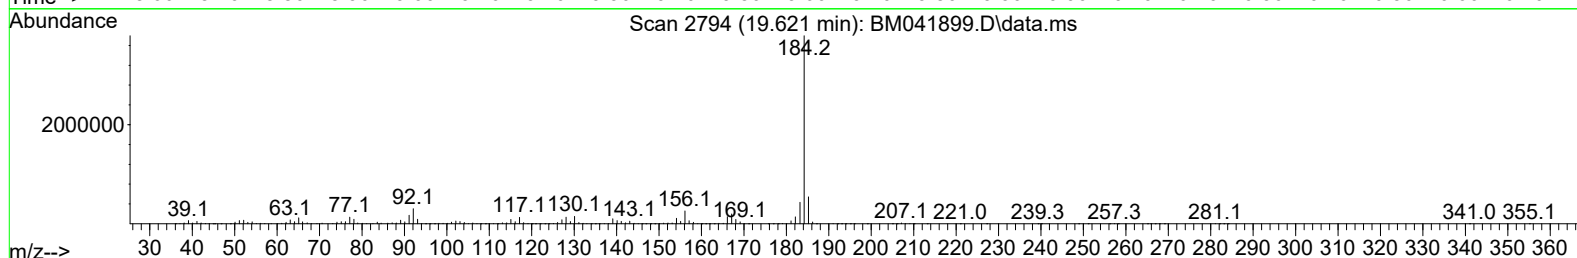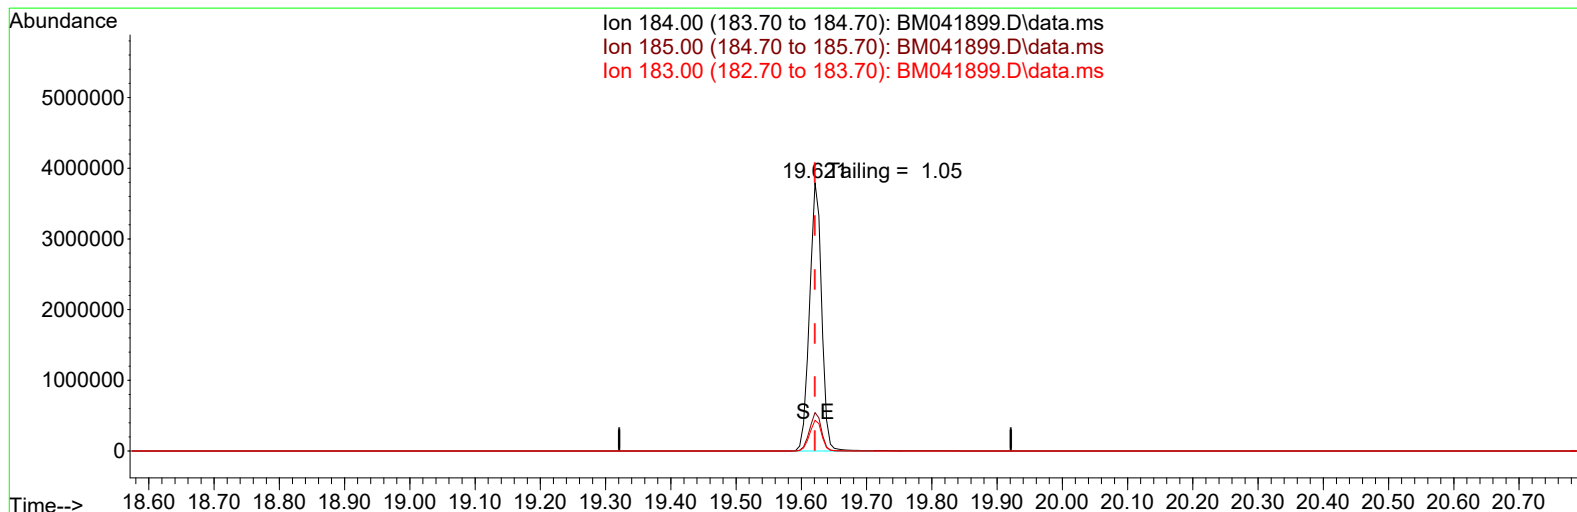

TIC: BM041899.D\data.ms

(77) Benzidine

19.621min (-0.000) 949277.61 ng

response 4921656

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.35
183.00	11.40	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2023	BNA_M	<u>BM041899.D</u>
Compound Name	Response	Retention Time
DDT	2369490	20.815
DDD	32811	20.421
DDE	949	19.862
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33760	2403250	1.40

Instrument :
BNA_M
ClientSampleId :
DFTPP