
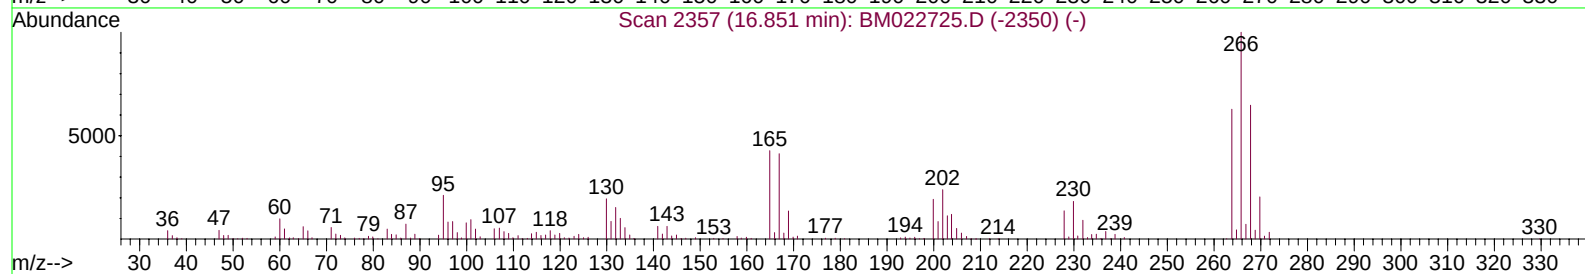
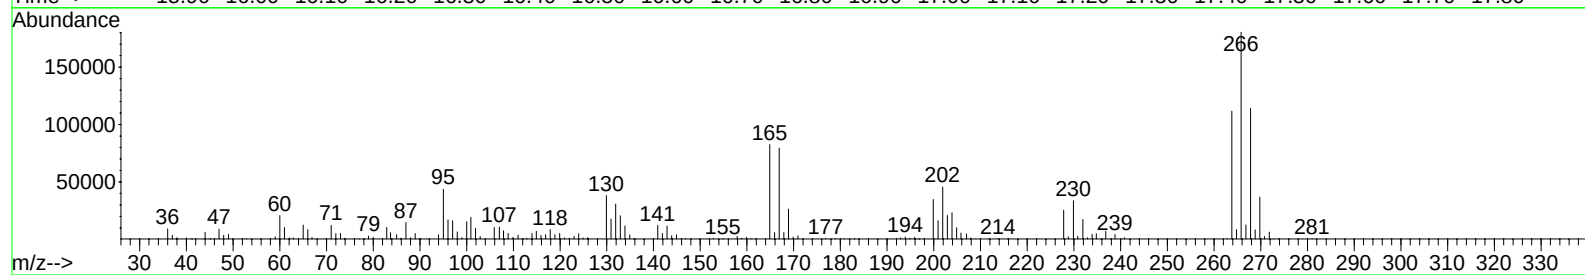


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM092019\
 Data File : BM022722.D
 Acq On : 20 Sep 2019 11:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 18:43:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM092019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 16:34:01 2019
 Response via : Initial Calibration

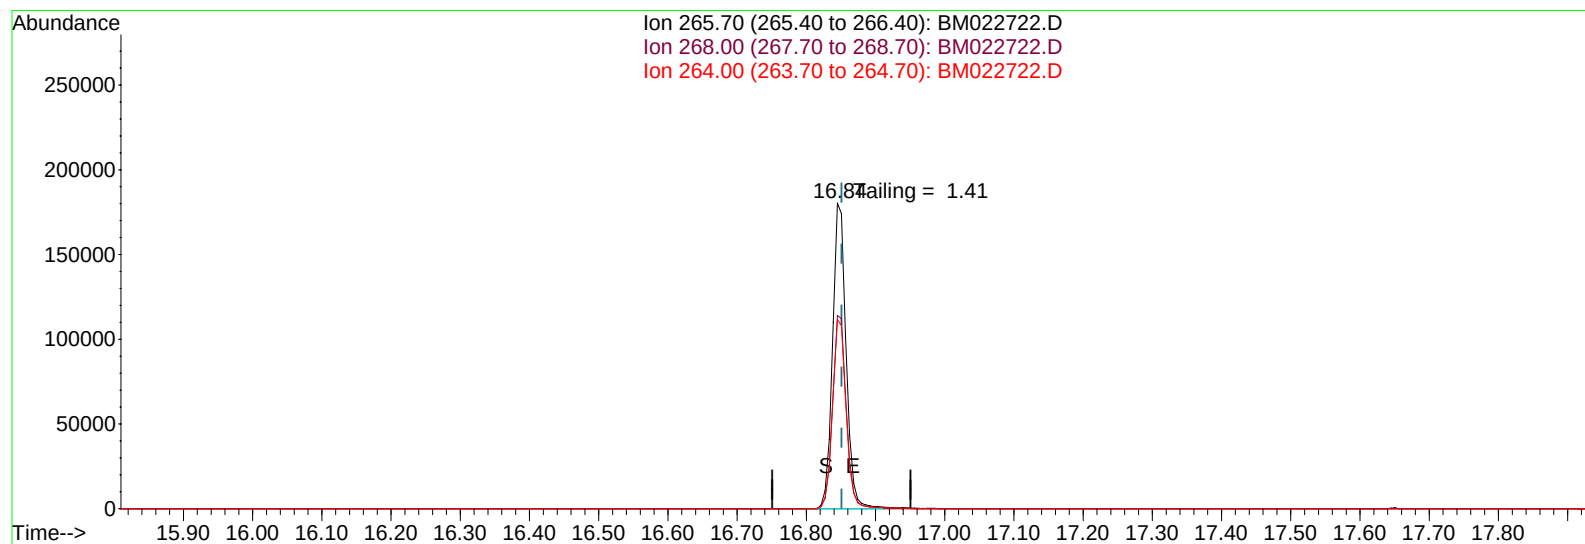

TIC: BM022722.D

(70) Pentachlorophenol (C)




16.845min (-0.006) 23035.23ng

response 246345

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	63.23
264.00	62.80	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM092019\
Data File : BM022722.D
Acq On : 20 Sep 2019 11:31
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 18:43:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM092019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:34:01 2019
Response via : Initial Calibration

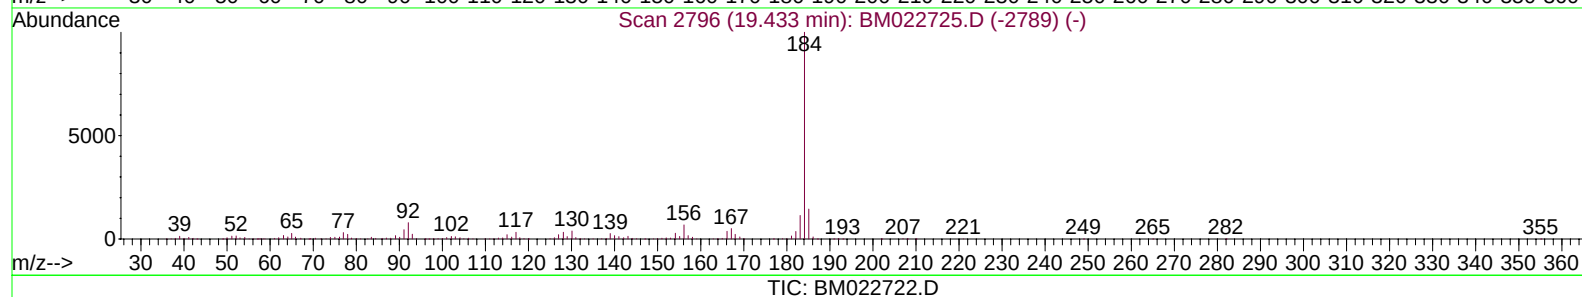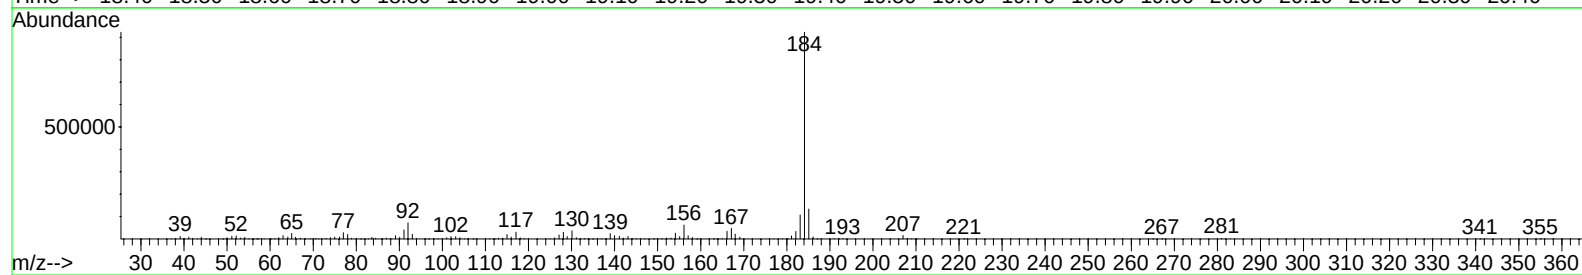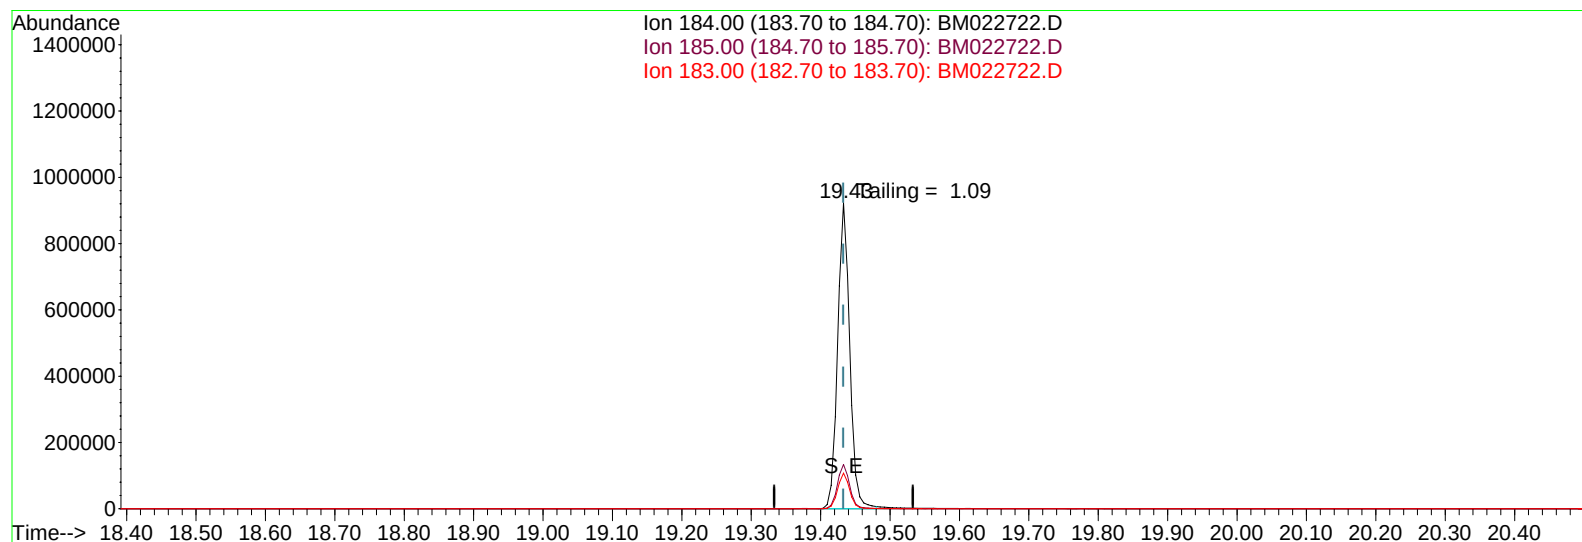

(77) Benzidine

19.433min (-0.000) 28202.96ng

response 1120325

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.51
183.00	11.40	11.66
0.00	0.00	0.00