


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092019\
 Data File : BM022722.D
 Acq On : 20 Sep 2019 11:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM092019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 20 16:34:01 2019

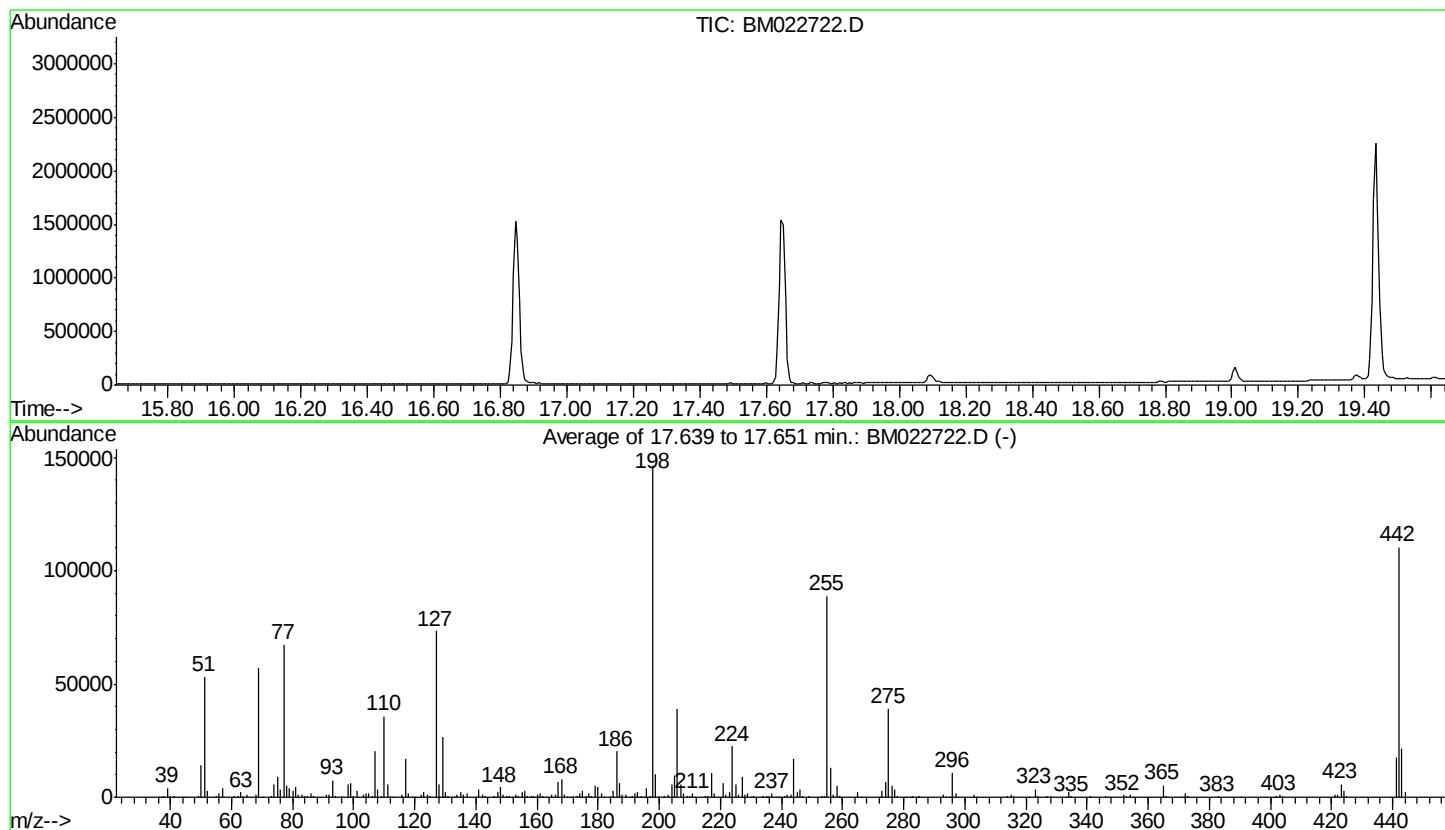

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	53192	PASS
68	69	0.00	2	1.7	978	PASS
69	198	0.00	100	39.0	57082	PASS
70	69	0.00	2	0.2	100	PASS
127	198	10	80	50.1	73325	PASS
197	198	0.00	2	0.4	632	PASS
198	198	100	100	100.0	146424	PASS
199	198	5	9	7.0	10223	PASS
275	198	10	60	26.7	39152	PASS
365	198	1	100	3.7	5383	PASS
441	198	0.01	100	11.8	17333	PASS
442	198	50	100	75.4	110389	PASS
443	442	15	24	19.5	21578	PASS