


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092019\
 Data File : BM022731.D
 Acq On : 20 Sep 2019 18:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM092019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 20 16:34:01 2019

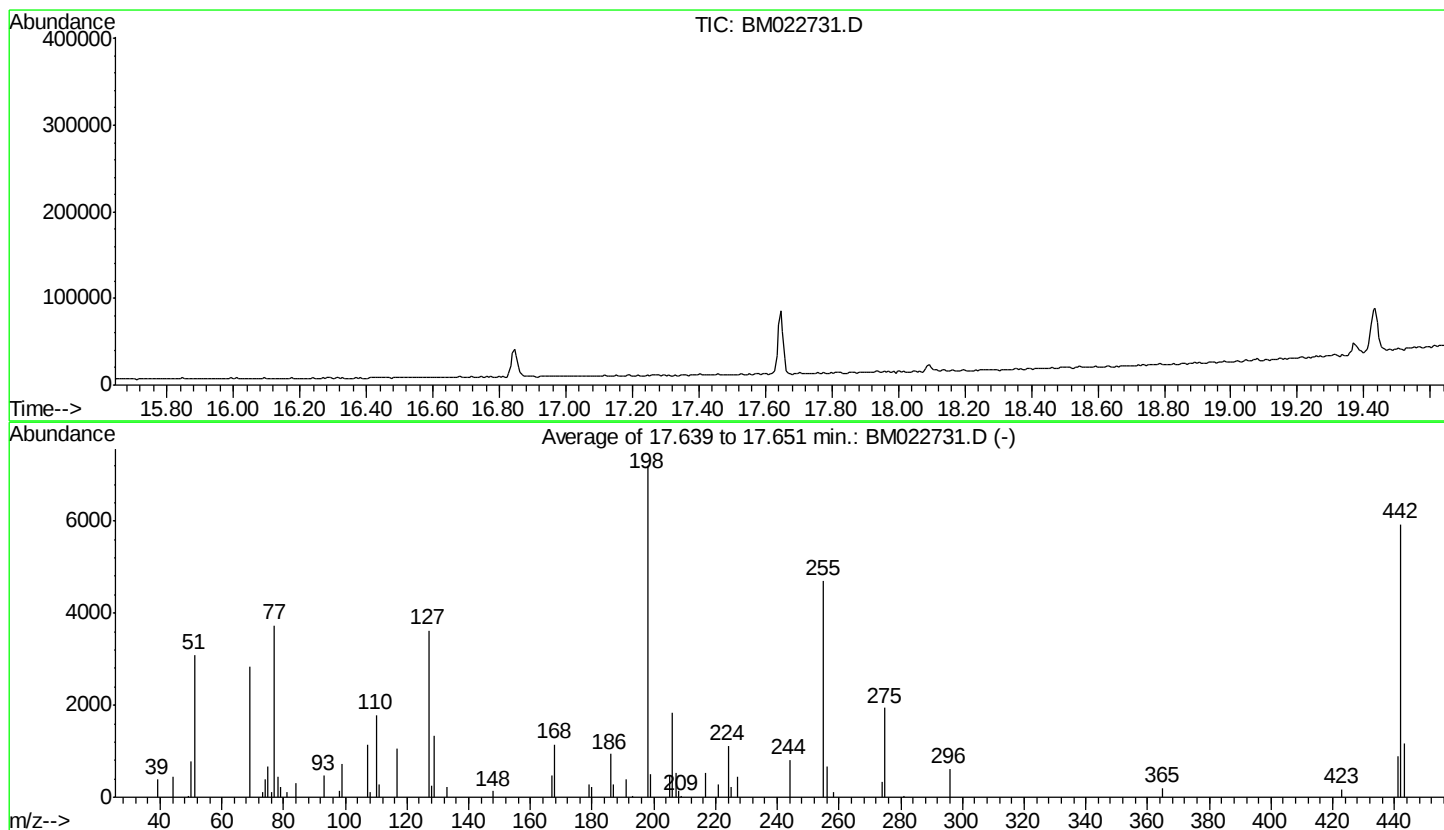

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	3092	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.5	2845	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	3628	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	7207	PASS
199	198	5	9	6.8	488	PASS
275	198	10	60	26.9	1937	PASS
365	198	1	100	2.8	203	PASS
441	198	0.01	100	12.3	889	PASS
442	198	50	100	82.4	5940	PASS
443	442	15	24	19.9	1180	PASS