

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
 Data File : BM041932.D
 Acq On : 20 Sep 2023 10:35
 Operator : MA/JU
 Sample : PB155666BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB155666BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	386	393	404	rBV	6397093	9496075	49.64%	10.653%
2	7.110	658	667	684	rBV	6165511	10121857	52.91%	11.355%
3	7.957	803	811	819	rBV	1159568	1814581	9.49%	2.036%
4	9.151	1004	1014	1022	rBV	3840178	6324550	33.06%	7.095%
5	10.775	1283	1290	1303	rBV	1545070	2570068	13.44%	2.883%
6	13.227	1699	1707	1722	rBV	9021751	13637937	71.29%	15.299%
7	14.604	1935	1941	1952	rBV	2381349	3456283	18.07%	3.877%
8	16.098	2188	2195	2214	rBV	7301017	10585205	55.34%	11.875%
9	17.357	2402	2409	2421	rBV	2894344	4070187	21.28%	4.566%
10	19.968	2847	2853	2858	rBV	15185120	19129069	100.00%	21.459%
11	21.527	3113	3118	3125	rBV	3124404	4111920	21.50%	4.613%
12	23.944	3522	3529	3539	rVB	1914179	3823660	19.99%	4.289%




Sum of corrected areas: 89141392

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041932.D
Acq On : 20 Sep 2023 10:35
Operator : MA/JU
Sample : PB155666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

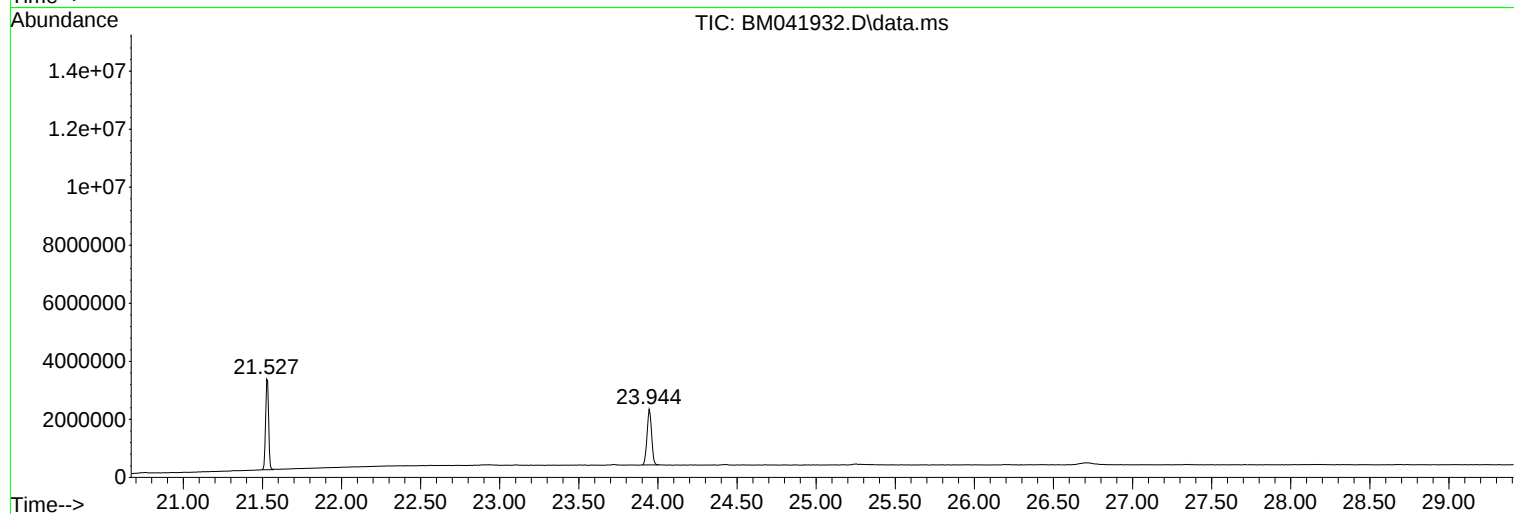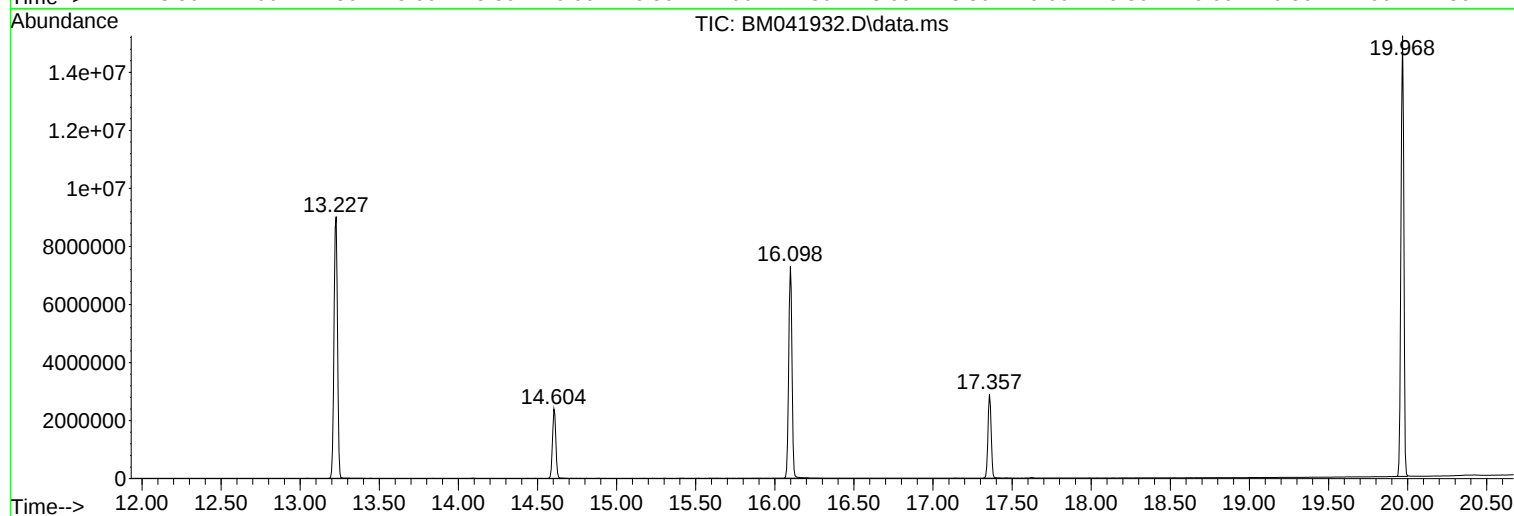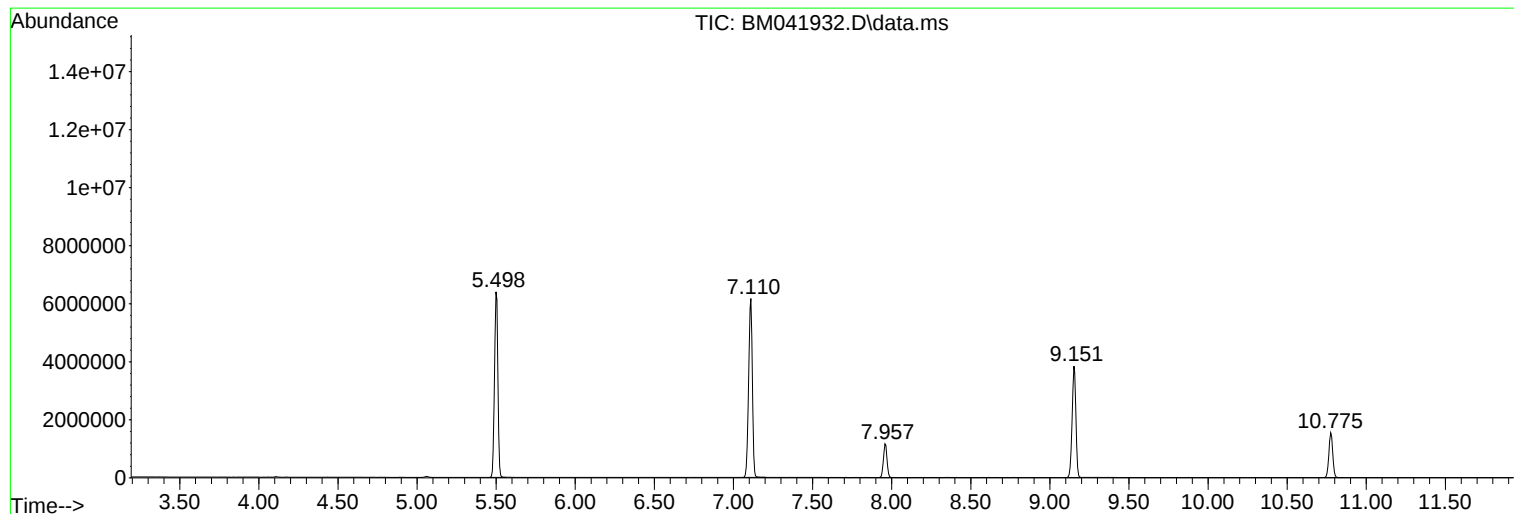

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041932.D
Acq On : 20 Sep 2023 10:35
Operator : MA/JU
Sample : PB155666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041932.D
Acq On : 20 Sep 2023 10:35
Operator : MA/JU
Sample : PB155666BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB155666BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------