

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
 Data File : BM041939.D
 Acq On : 20 Sep 2023 15:35
 Operator : MA/JU
 Sample : 04343-01RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SAMPLE-1-14TH-STREETRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	307	318	330	rBV	1368481	1893778	9.06%	2.150%
2	5.499	384	393	402	rBV	2556464	3660889	17.51%	4.156%
3	7.104	658	666	679	rBV	1651521	2663192	12.74%	3.023%
4	7.957	801	811	823	rBV	1282613	2133875	10.21%	2.422%
5	9.157	1005	1015	1026	rBV	4536099	7731178	36.98%	8.776%
6	10.775	1282	1290	1298	rBV	1816514	3043776	14.56%	3.455%
7	13.227	1699	1707	1714	rBV	11157300	16832989	80.52%	19.108%
8	14.604	1932	1941	1948	rBV	2706391	4026872	19.26%	4.571%
9	16.098	2188	2195	2210	rBV	6154385	8996937	43.04%	10.213%
10	16.721	2296	2301	2307	rVB4	155013	285422	1.37%	0.324%
11	17.357	2403	2409	2415	rBV	3259456	4655796	22.27%	5.285%
12	18.204	2548	2553	2563	rBV	1131689	1622785	7.76%	1.842%
13	19.480	2766	2770	2778	rBV	336487	476824	2.28%	0.541%
14	19.968	2847	2853	2858	rBV	16125169	20904817	100.00%	23.730%
15	21.192	3058	3061	3072	rVB	1074086	1358291	6.50%	1.542%
16	21.392	3093	3095	3100	rVB	331060	354008	1.69%	0.402%
17	21.527	3114	3118	3125	rVB	3128801	4093288	19.58%	4.647%
18	23.950	3524	3530	3538	rVB	1648693	3358851	16.07%	3.813%




Sum of corrected areas: 88093568

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041939.D
Acq On : 20 Sep 2023 15:35
Operator : MA/JU
Sample : 04343-01RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SAMPLE-1-14TH-STREETRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

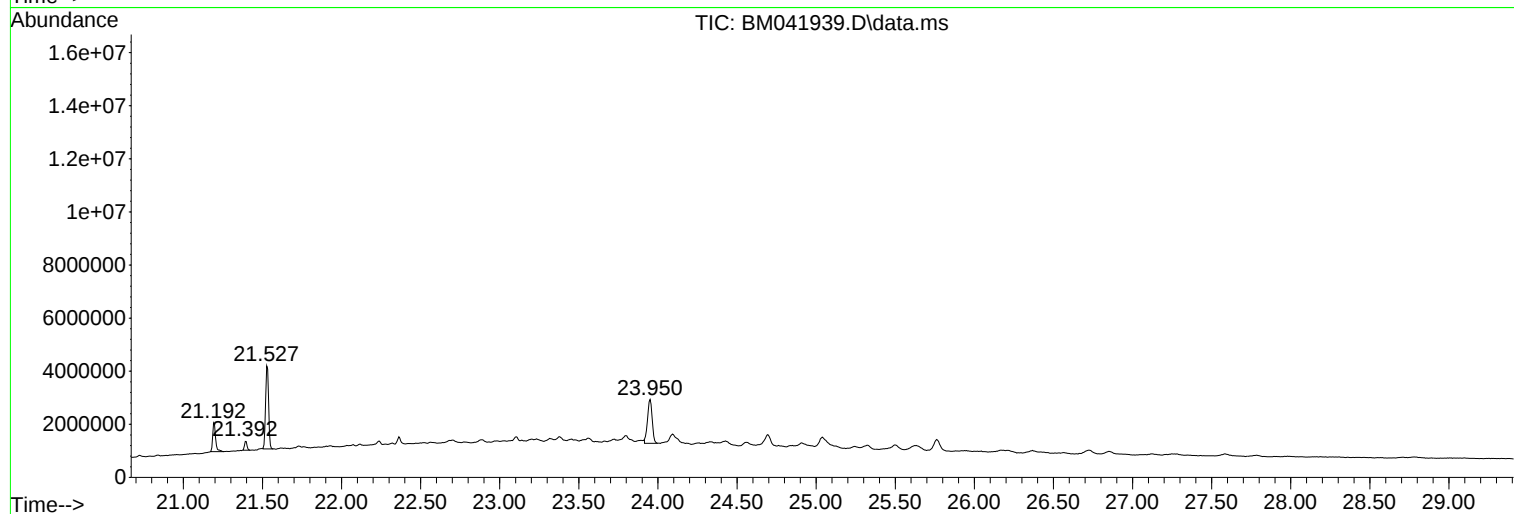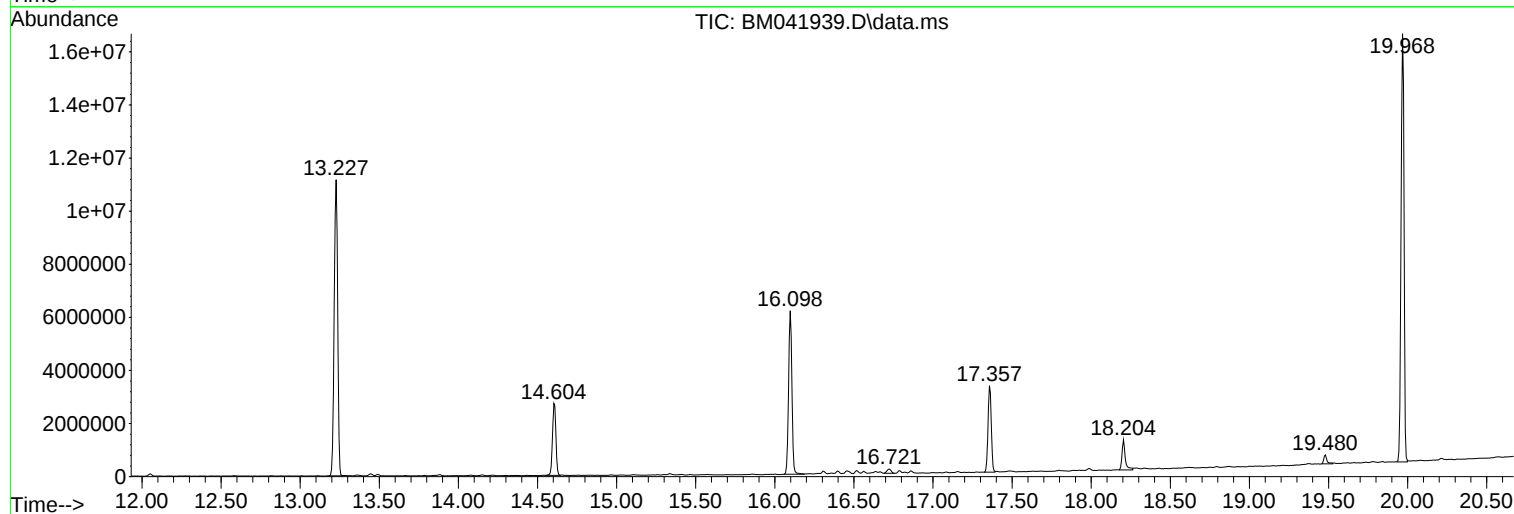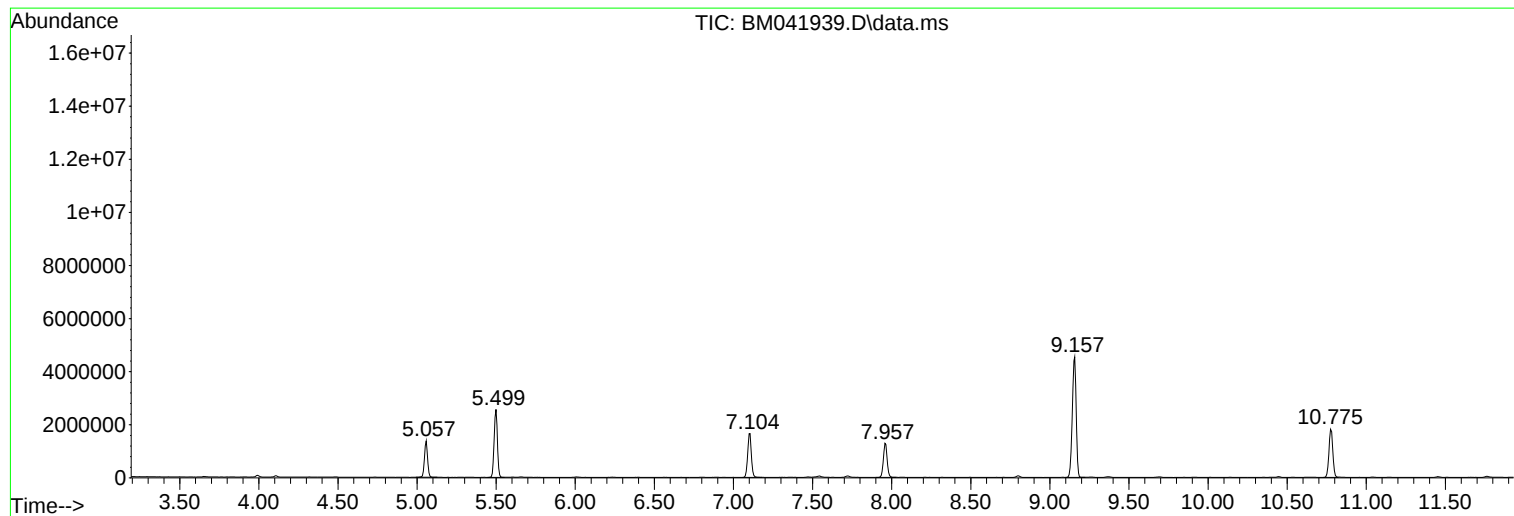

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041939.D
Acq On : 20 Sep 2023 15:35
Operator : MA/JU
Sample : 04343-01RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SAMPLE-1-14TH-STREETRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041939.D
Acq On : 20 Sep 2023 15:35
Operator : MA/JU
Sample : 04343-01RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SAMPLE-1-14TH-STREETRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------