

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
 Data File : BM041946.D
 Acq On : 20 Sep 2023 19:53
 Operator : MA/JU
 Sample : 04453-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CPT102-14

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.652	75	79	88	rVB	115346	156139	1.40%	0.238%
2	5.498	386	393	401	rBV	4564360	6471743	57.99%	9.871%
3	7.104	659	666	683	rBV	4353306	7082691	63.47%	10.803%
4	7.957	804	811	821	rVB	1113279	1762549	15.79%	2.688%
5	9.151	1004	1014	1025	rBV	2664894	4314828	38.66%	6.581%
6	10.775	1283	1290	1298	rBV	1500462	2519258	22.57%	3.843%
7	13.221	1695	1706	1721	rBV	6163740	9357840	83.85%	14.273%
8	14.604	1935	1941	1949	rBV	2318910	3356118	30.07%	5.119%
9	16.098	2188	2195	2210	rBV	5108129	7305337	65.46%	11.143%
10	17.356	2401	2409	2422	rBV	2756065	3819086	34.22%	5.825%
11	18.198	2547	2552	2562	rBV	194367	286664	2.57%	0.437%
12	19.968	2847	2853	2858	rBV	8885854	11159784	100.00%	17.022%
13	20.633	2960	2966	2977	rBV	1507120	1906157	17.08%	2.907%
14	21.192	3058	3061	3069	rVB2	107300	146821	1.32%	0.224%
15	21.527	3113	3118	3124	rBV	2535523	3181084	28.50%	4.852%
16	23.944	3522	3529	3538	rVB	1371917	2736367	24.52%	4.174%




Sum of corrected areas: 65562466

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041946.D
Acq On : 20 Sep 2023 19:53
Operator : MA/JU
Sample : 04453-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CPT102-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

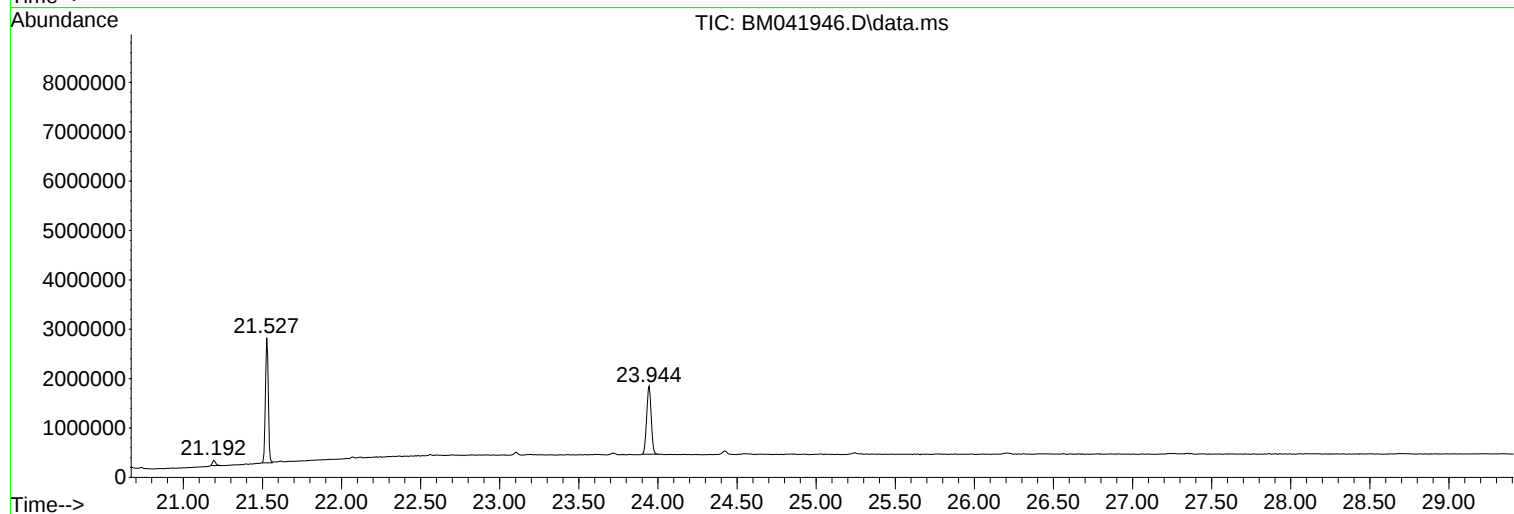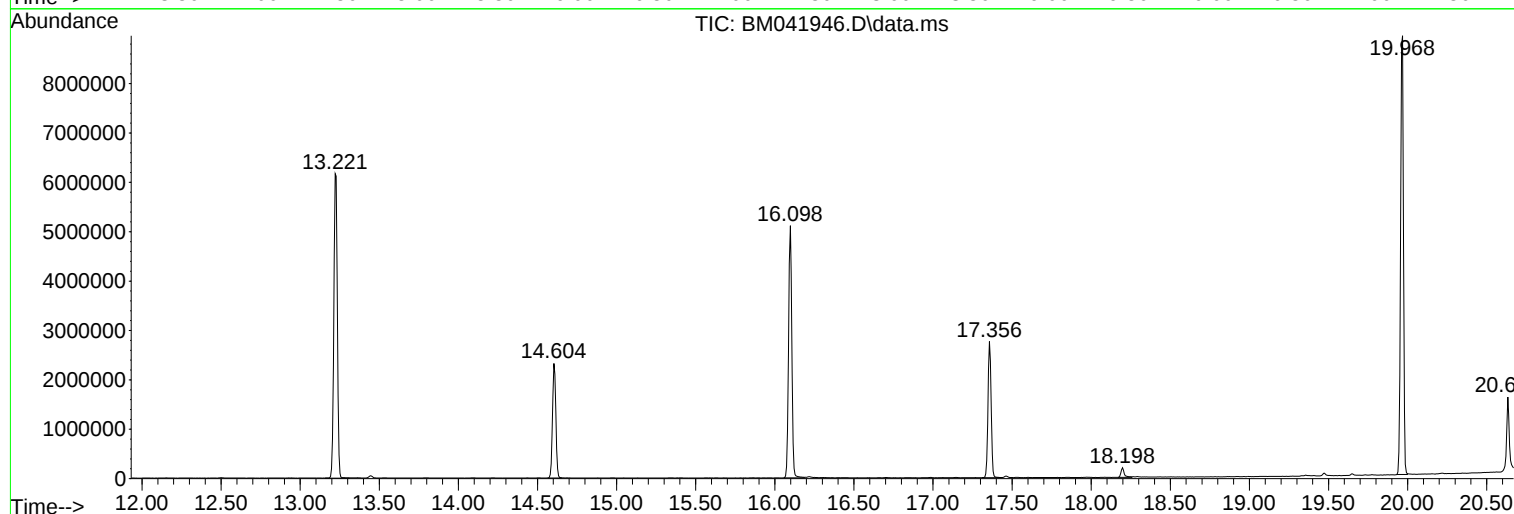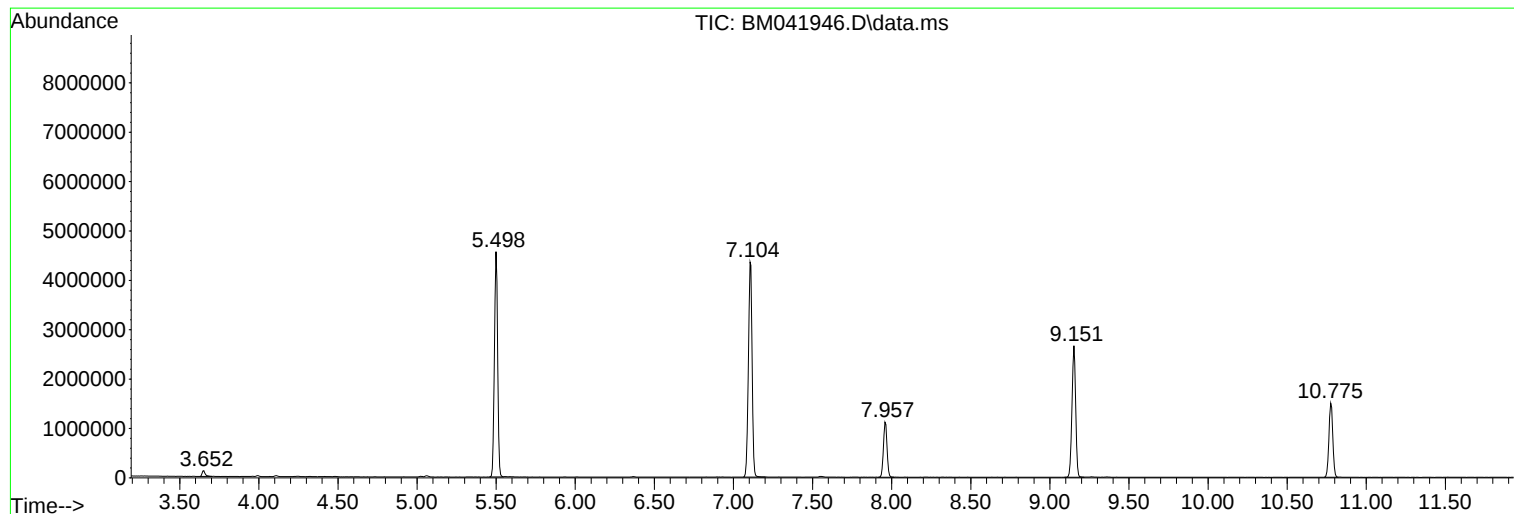

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041946.D
Acq On : 20 Sep 2023 19:53
Operator : MA/JU
Sample : 04453-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CPT102-14










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 9-Octadecenamide, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.633	11.98 ng	1906160	Chrysene-d12	21.527

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	91
2			Octanamide	143	C8H17NO	000629-01-6	64
3			Hexadecanamide	255	C16H33NO	000629-54-9	64
4			7-Nonenamide	155	C9H17NO	090949-53-4	59
5			Octadecanamide	283	C18H37NO	000124-26-5	53

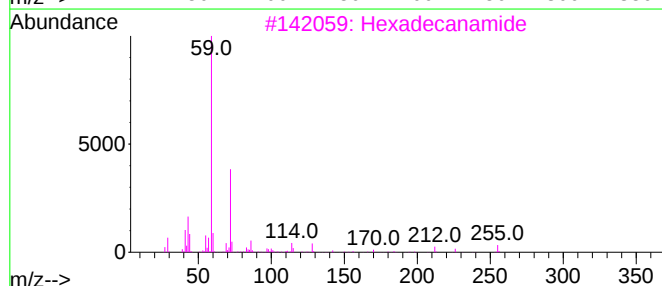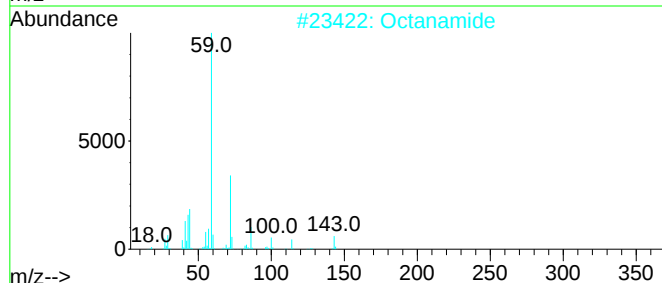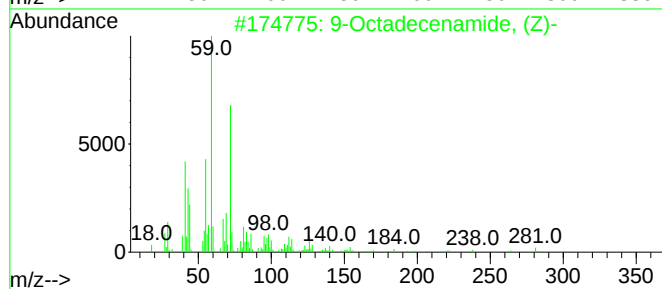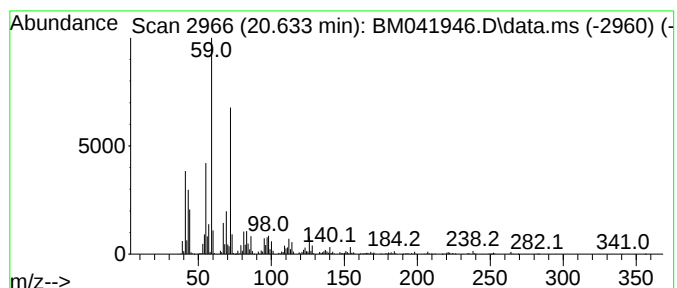

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041946.D
Acq On : 20 Sep 2023 19:53
Operator : MA/JU
Sample : 04453-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CPT102-14

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
9-Octadecenamid...	20.633	12.0	ng	1906160	5	21.527	3181080	20.0