
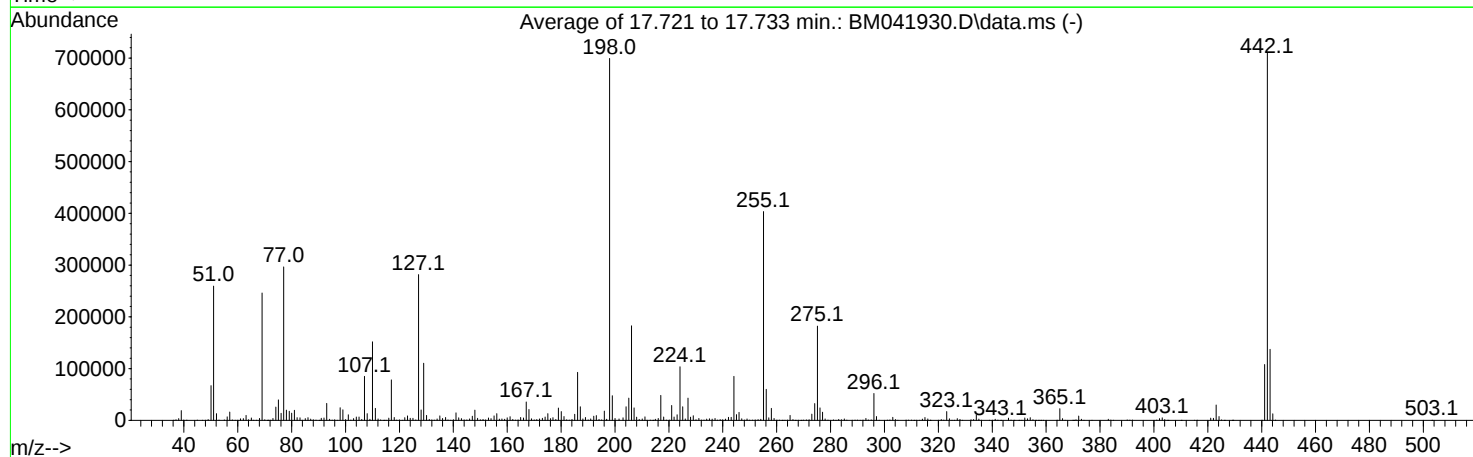


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041930.D
Acq On : 20 Sep 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 19 04:49:34 2023

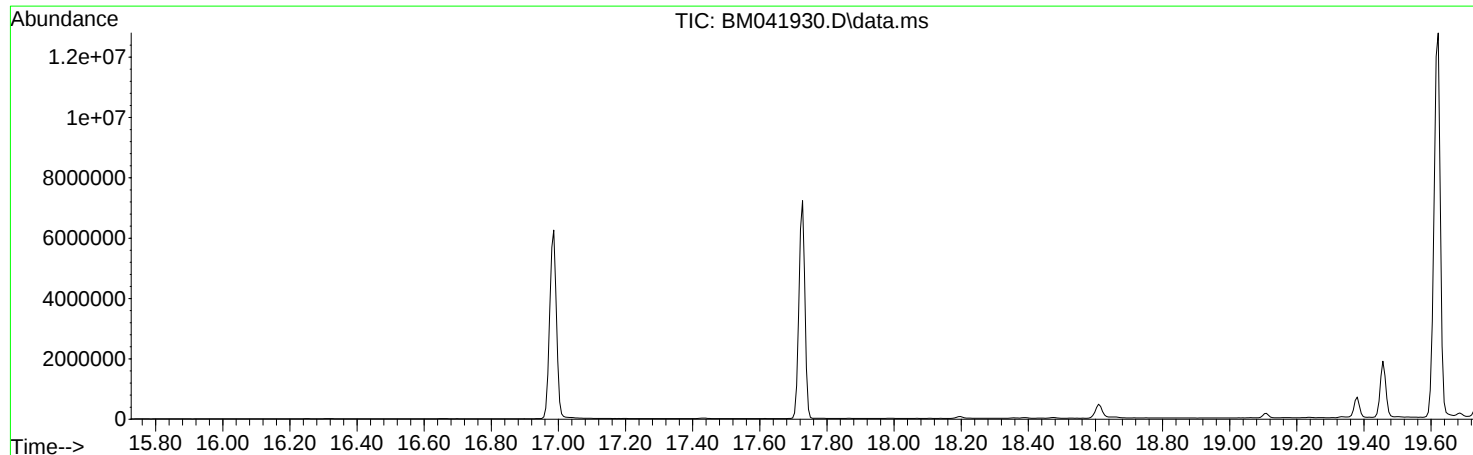




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	259583	PASS
68	69	0.00	2	1.6	3851	PASS
69	198	0.00	100	35.2	246165	PASS
70	69	0.00	2	0.5	1339	PASS
127	198	10	80	40.3	281707	PASS
197	198	0.00	2	0.3	2061	PASS
198	198	100	100	100.0	699349	PASS
199	198	5	9	6.8	47533	PASS
275	198	10	60	26.0	182144	PASS
365	198	1	100	3.2	22501	PASS
441	198	0.01	100	15.4	107803	PASS
442	442	50	100	100.0	710805	PASS
443	442	15	24	19.3	137435	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\  
Data File : BM041930.D  
Acq On    : 20 Sep 2023  09:23  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 20 11:02:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

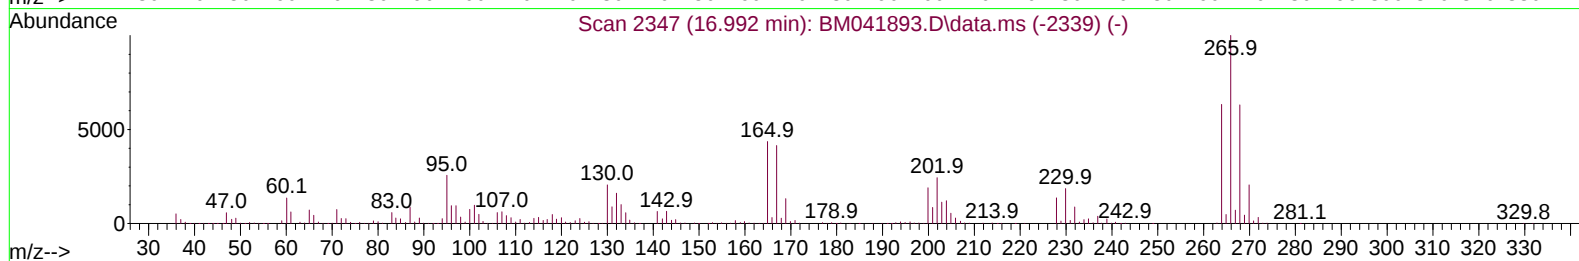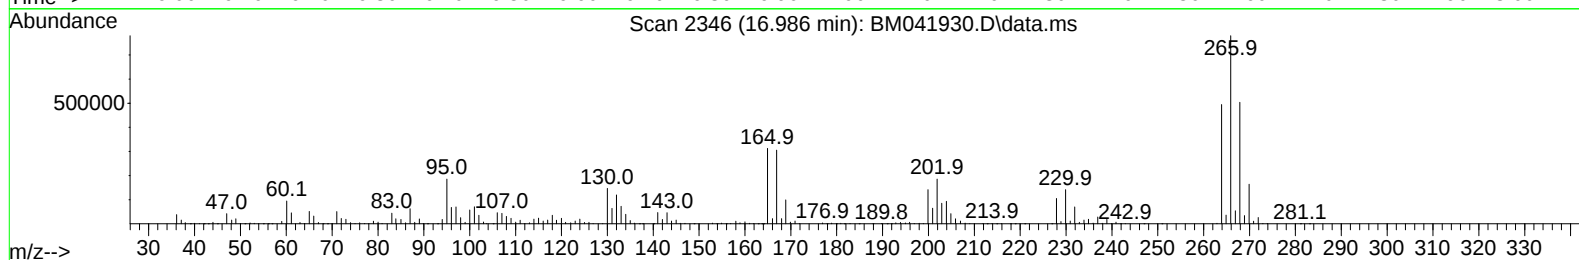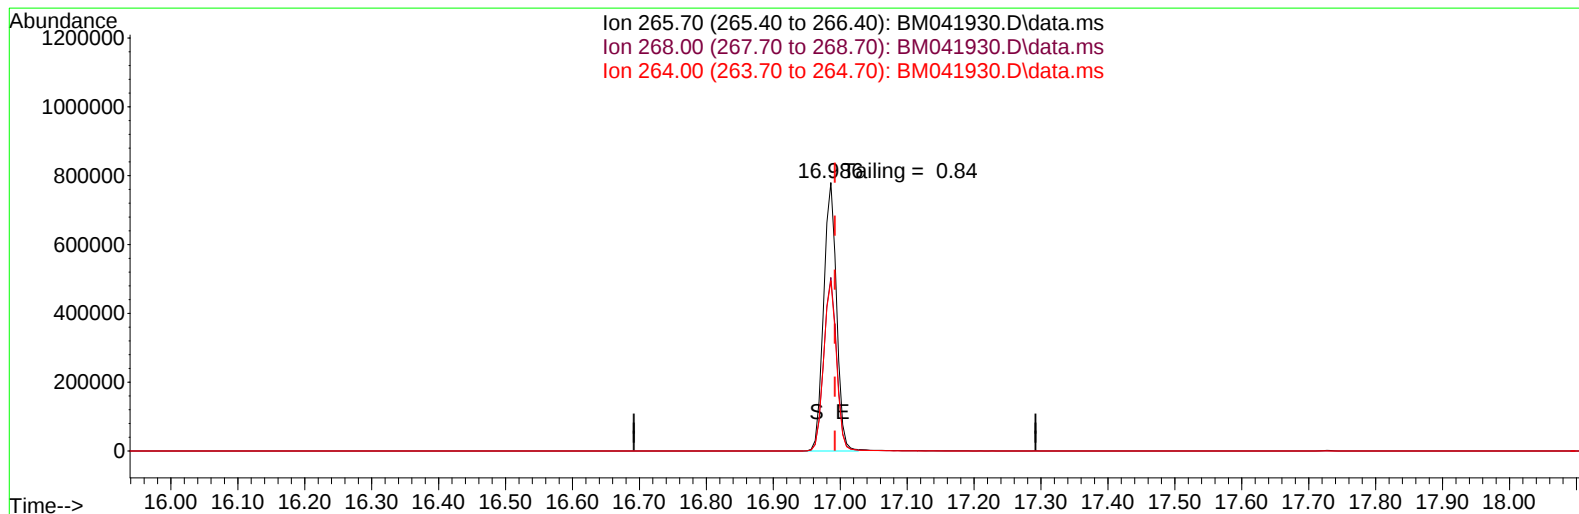

TIC: BM041930.D\data.ms

(70) Pentachlorophenol (C)

16.986min (-0.006) 226714.12 ng




```
response      1054086
```

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.65
264.00	63.30	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092023\
Data File : BM041930.D
Acq On : 20 Sep 2023 09:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 20 11:02:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM091823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 19 04:49:34 2023
Response via : Initial Calibration

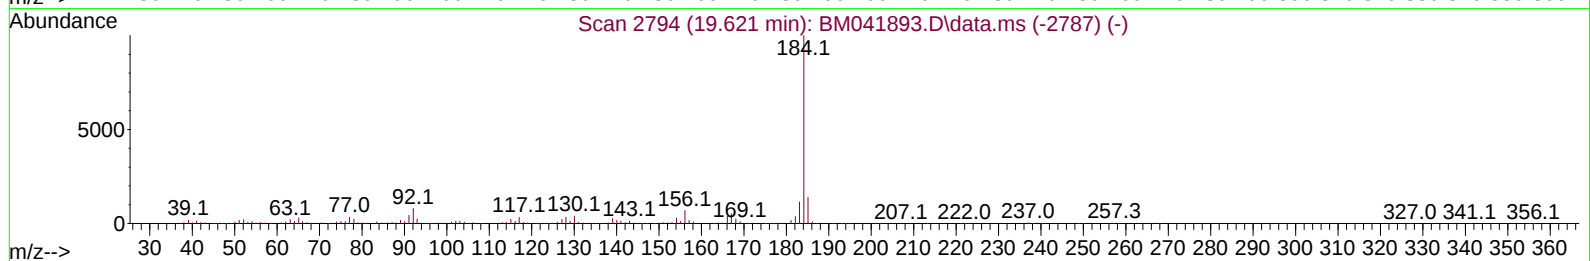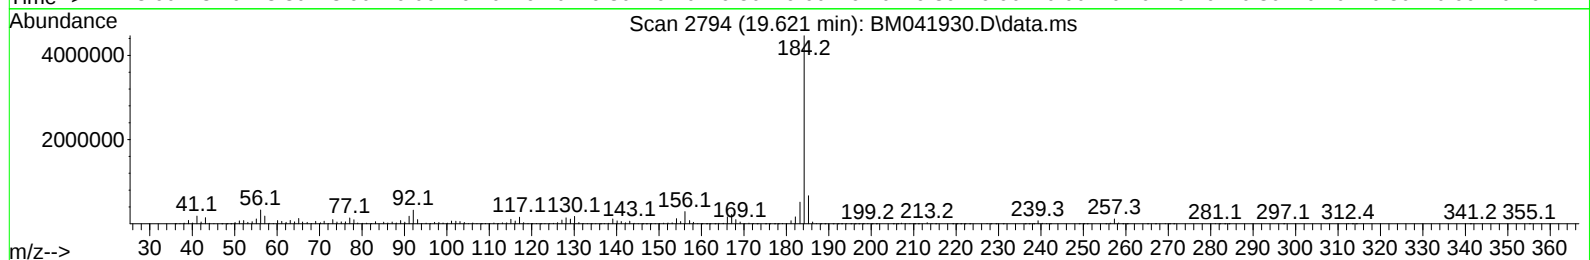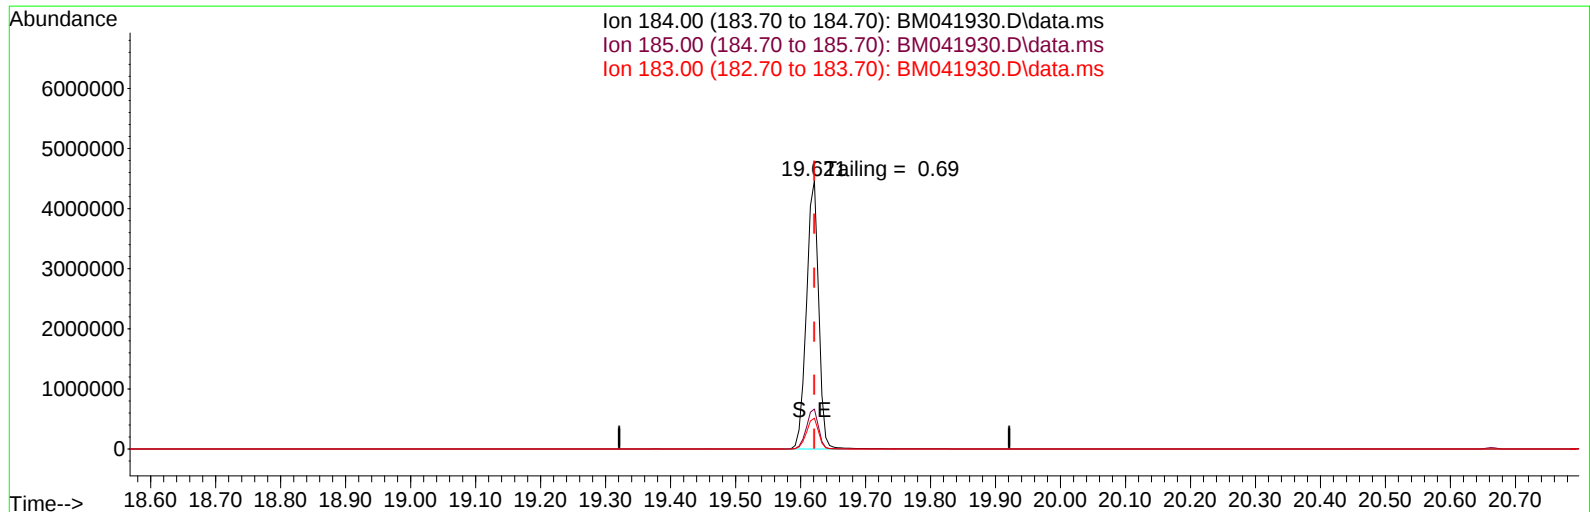

TIC: BM041930.D\data.ms

(77) Benzidine

19.621min (-0.000) 161255.31 ng

response 5832598

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.92
183.00	11.40	11.52
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2023	BNA_M	<u>BM041930.D</u>
Compound Name	Response	Retention Time
DDT	2743132	20.809
DDD	151979	20.374
DDE	4125	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
156104	2899236	5.38

Instrument :
BNA_M
ClientSampleId :
DFTPP