

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
 Data File : BM016827.D
 Acq On : 21 Sep 2018 12:06
 Operator : SJ/JU
 Sample : J5012-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 22 01:09:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 22 01:08:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	279310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1169374	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	630721	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1434960	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1645788	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1766122	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	35323	5.41	ng/uL	0.00
5) Phenol-d5	6.89	99	126602	5.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	346000	23.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	388760	20.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	233536	12.81	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	223391	29.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	216070	30.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	414444	23.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.64	131	30082	1.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1408593	27.81	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	1697312	25.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	39722	4.78	ng/ul	0.00
58) Fluorene-d10	15.35	176	1281395	28.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	160201	27.20	ng/ul	0.00
71) Anthracene-d10	17.20	188	2069349	29.89	ng/ul	0.00
79) Pyrene-d10	19.50	212	2354610	29.48	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	2765572	30.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.82	163	159037	3.213	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
Data File : BM016827.D
Acq On : 21 Sep 2018 12:06
Operator : SJ/JU
Sample : J5012-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 22 01:09:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 22 01:08:22 2018
Response via : Initial Calibration

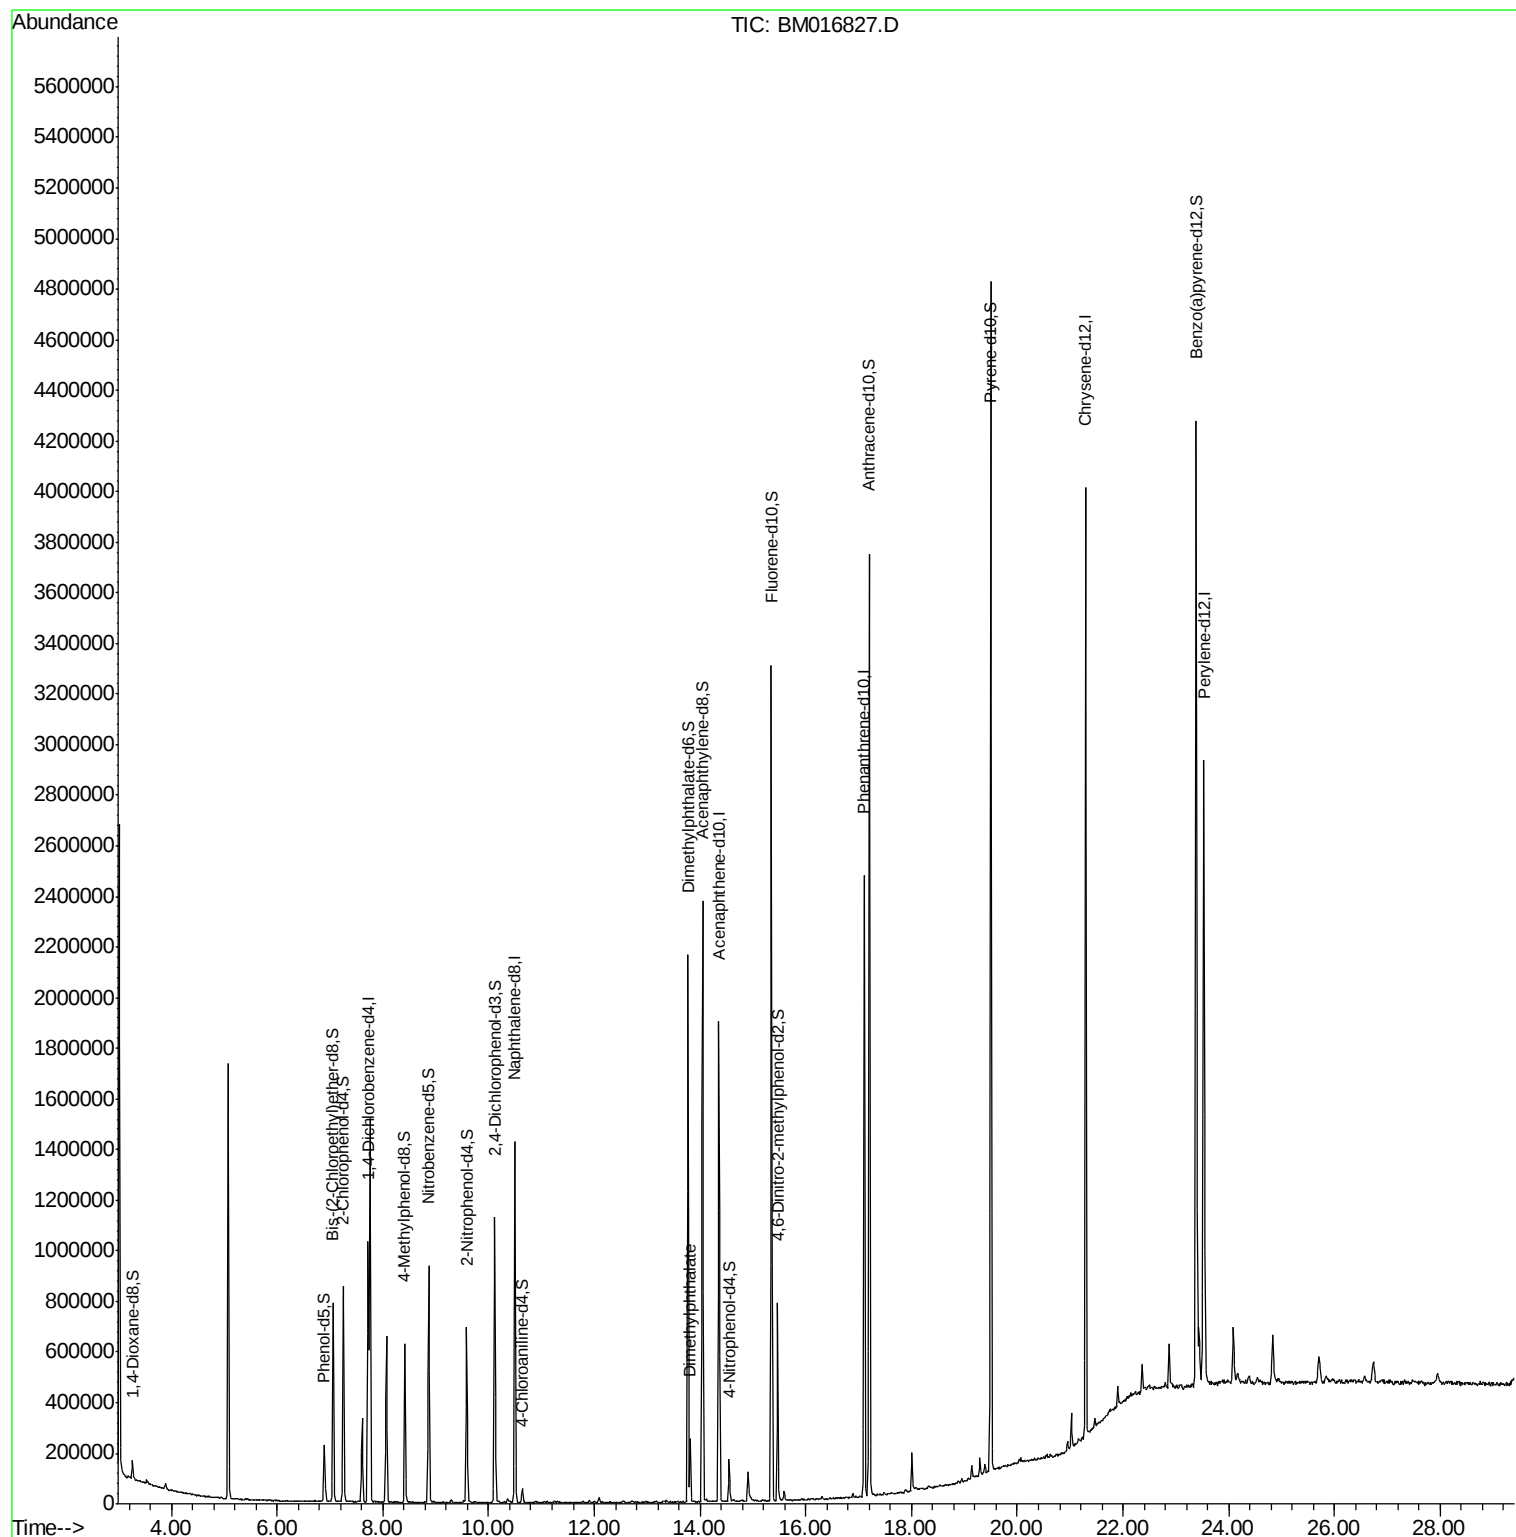

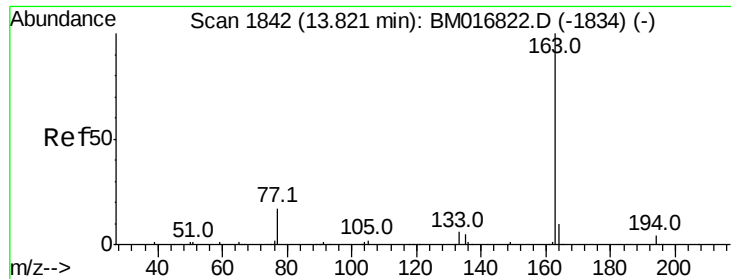

#45

Dimethylphthalate

Concen: 3.213 ng/ul

RT: 13.82 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BM016827.D

Acq: 21 Sep 2018 12:06

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 159037

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 9.7 8.4 12.6

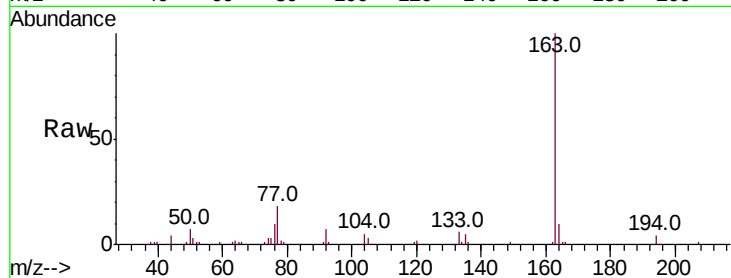

Abundance Ion 163.00 (162.70 to 163.70): E

150000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

