

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
 Data File : BM016830.D
 Acq On : 21 Sep 2018 13:53
 Operator : SJ/JU
 Sample : J5012-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 22 01:09:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 22 01:08:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	276792	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1146090	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	611967	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1369349	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1547001	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1657470	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	37990	5.87	ng/uL	0.00
5) Phenol-d5	6.89	99	168606	7.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	461230	31.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	526173	27.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	308437	17.07	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	305558	40.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	300795	43.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	558525	32.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.64	131	1501	0.07	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1803470	36.70	ng/ul	0.00
47) Acenaphthylene-d8	14.05	160	2264236	35.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	53722	6.66	ng/ul	0.00
58) Fluorene-d10	15.36	176	1638249	38.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	214158	38.10	ng/ul	0.00
71) Anthracene-d10	17.20	188	2613722	39.56	ng/ul	0.00
79) Pyrene-d10	19.50	212	2940584	39.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	3394127	39.26	ng/ul	0.00


Target Compounds				Ovalue	
46) 2,6-Dinitrotoluene	13.77	165	13782	1.869	ng/ul# 41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
Data File : BM016830.D
Acq On : 21 Sep 2018 13:53
Operator : SJ/JU
Sample : J5012-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 22 01:09:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 22 01:08:22 2018
Response via : Initial Calibration

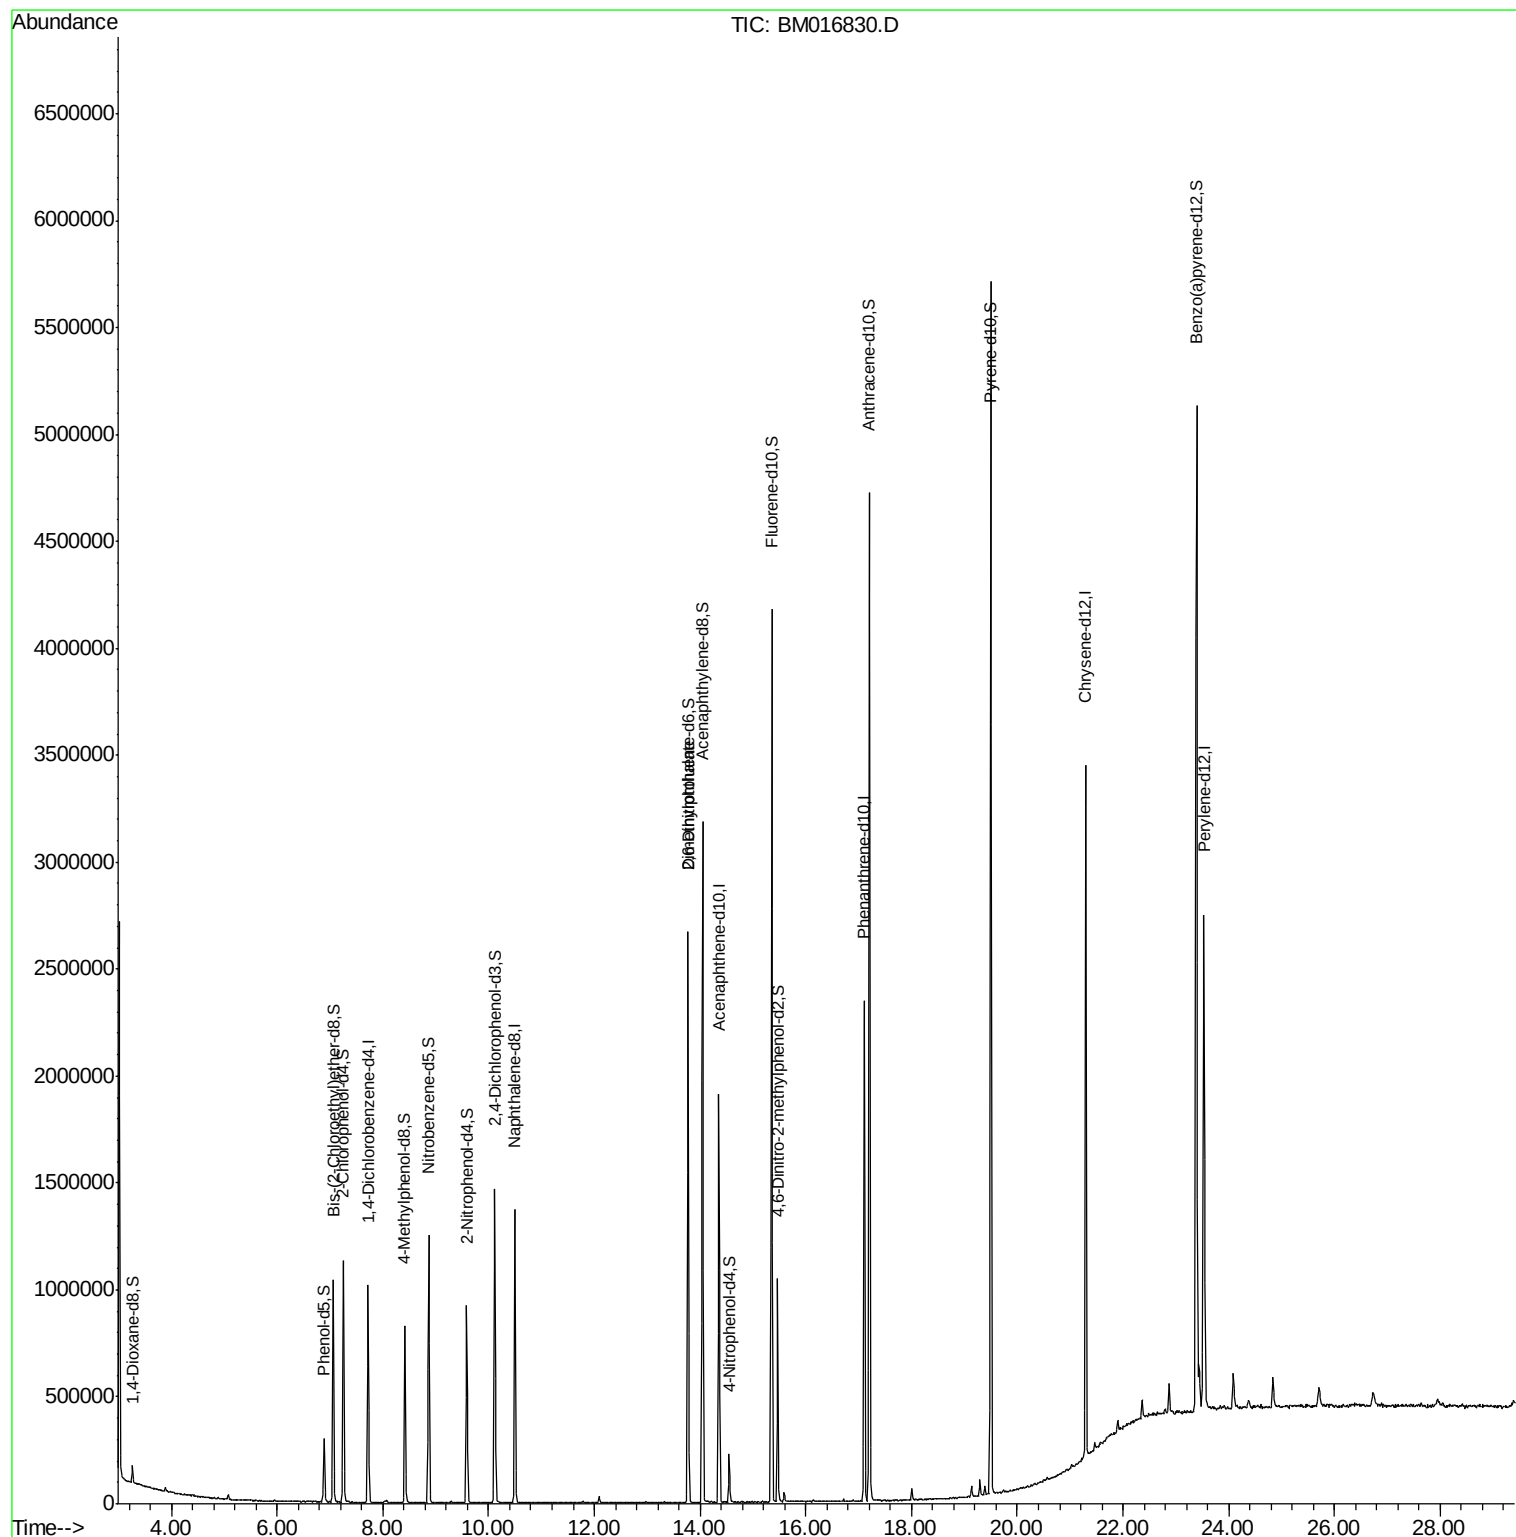

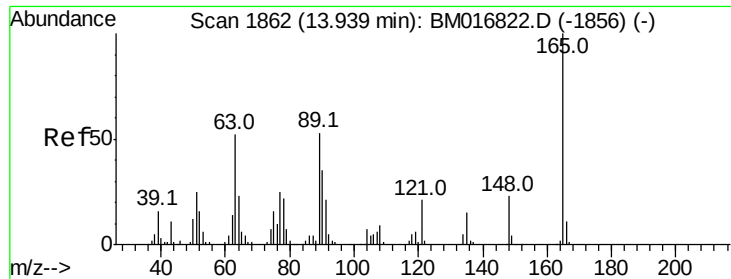

#46

2,6-Dinitrotoluene

Concen: 1.869 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.16 min

Lab File: BM016830.D

Acq: 21 Sep 2018 13:53

Instrument :

BNA_M

ClientSampleId :


Tot Ion:165 Resp: 13782

Ion Ratio Lower Upper

165 100

89 0.0 43.8 65.8#

121 30.3 17.8 26.6#

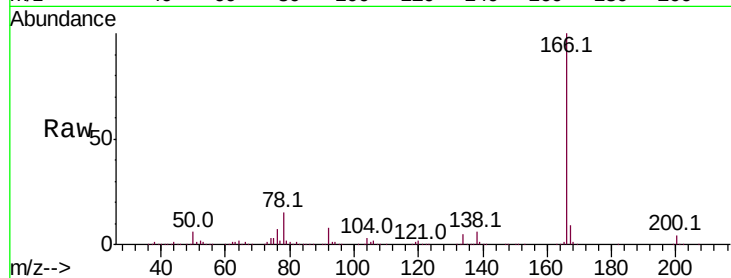

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

