

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
 Data File : BM016851.D
 Acq On : 22 Sep 2018 03:10
 Operator : SJ/JU
 Sample : J5012-18
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Sep 22 05:14:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 22 05:13:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	253985	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1036667	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	560152	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1256801	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1421249	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1565016	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	35156	5.92	ng/uL	0.00
5) Phenol-d5	6.89	99	126840	5.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	385191	29.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	424311	24.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	244190	14.73	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	257075	37.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	255410	41.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	456857	29.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.64	131	12925	0.68	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1507615	33.52	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1928751	33.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	36513	4.95	ng/ul	0.00
58) Fluorene-d10	15.35	176	1385825	35.30	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	169654	32.88	ng/ul	0.00
71) Anthracene-d10	17.20	188	2145977	35.39	ng/ul	0.00
79) Pyrene-d10	19.50	212	2384814	34.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	2820368	34.55	ng/ul	0.00


Target Compounds				Ovalue	
46) 2,6-Dinitrotoluene	13.77	165	11327	1.678	ng/ul# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
Data File : BM016851.D
Acq On : 22 Sep 2018 03:10
Operator : SJ/JU
Sample : J5012-18
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Sep 22 05:14:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 22 05:13:53 2018
Response via : Initial Calibration

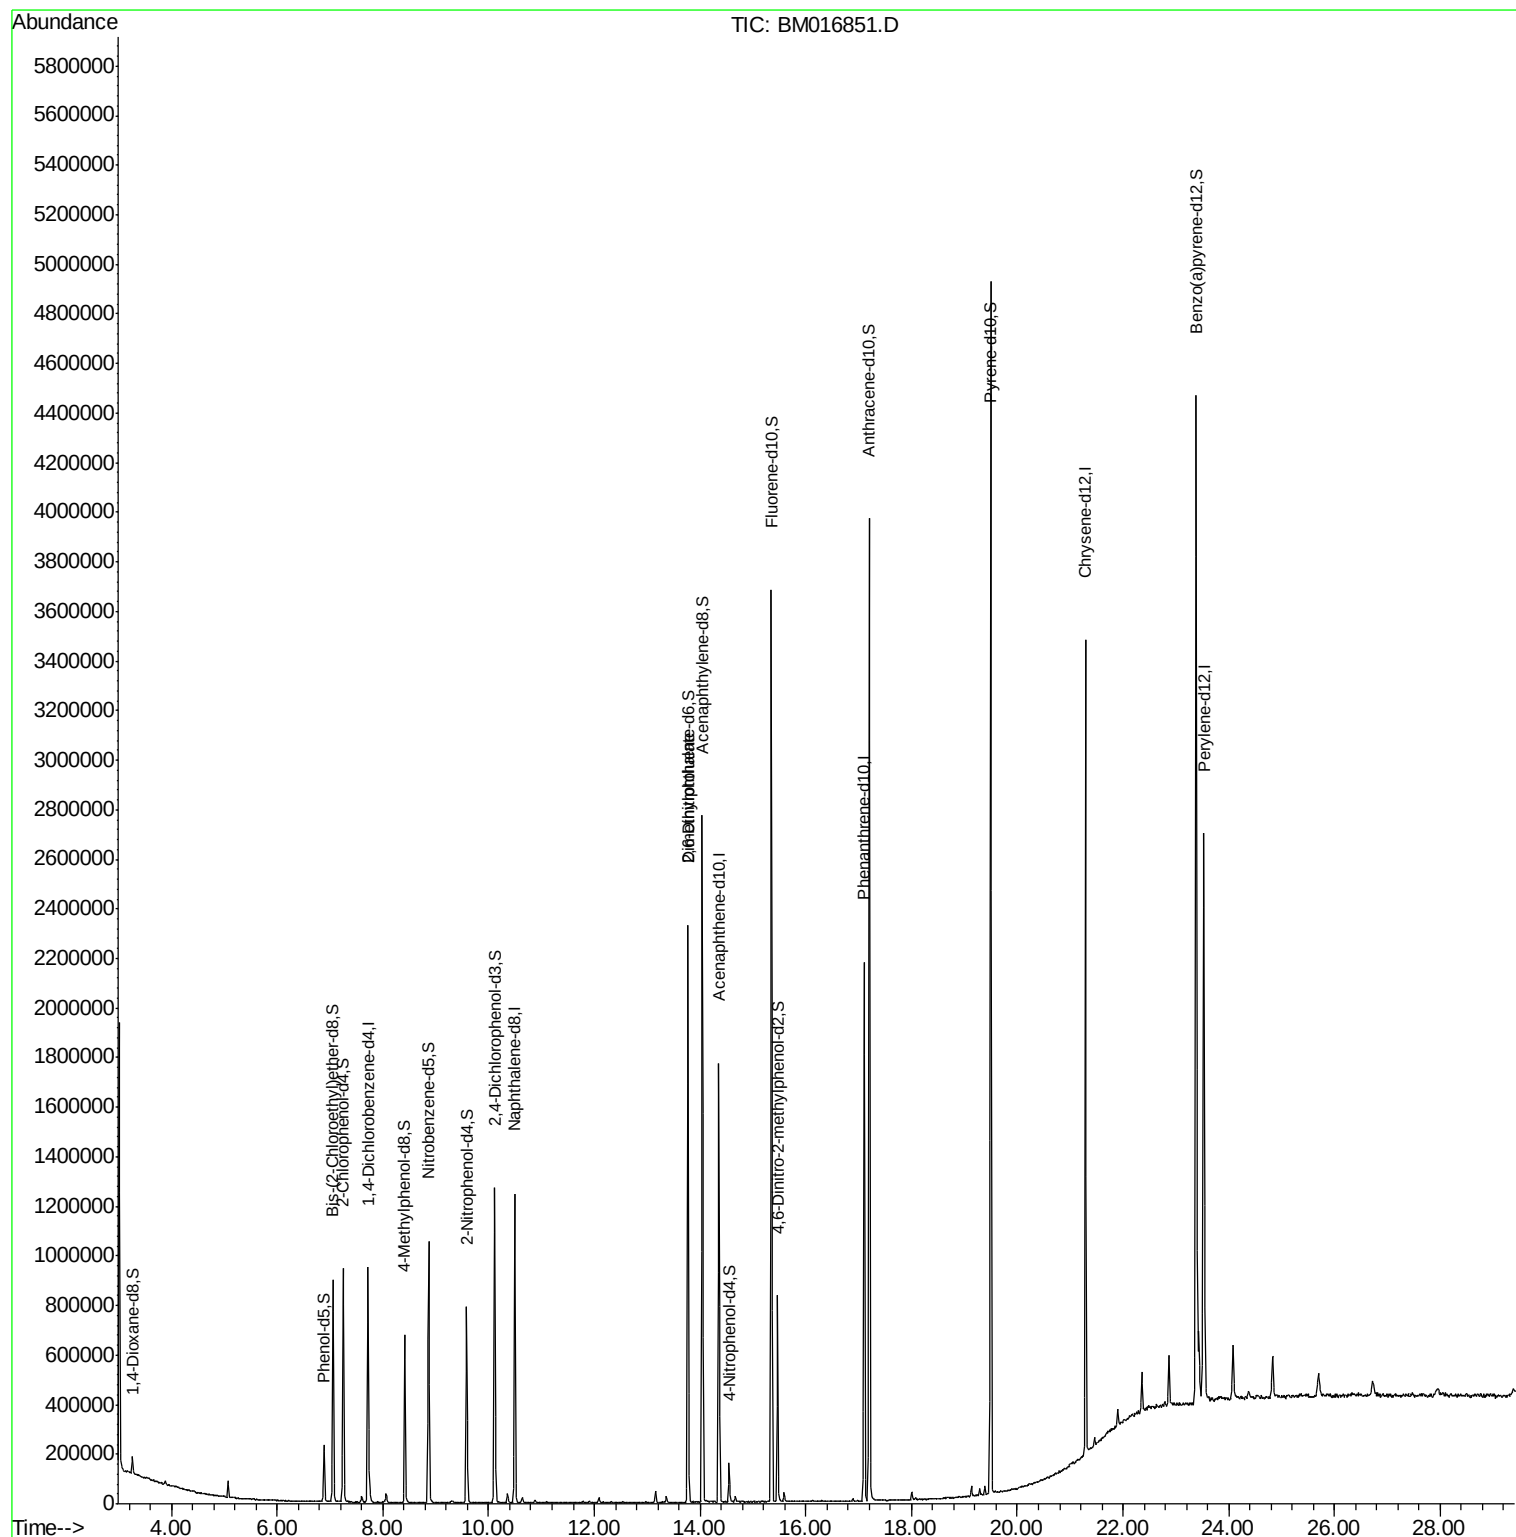

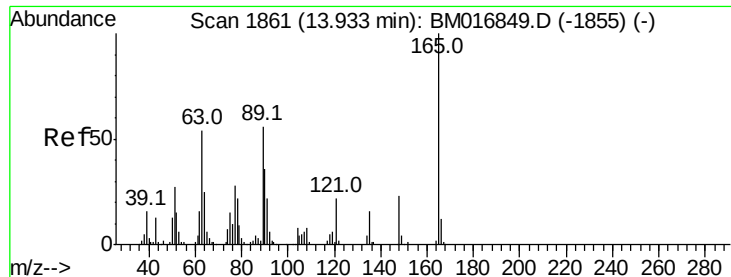

#46

2,6-Dinitrotoluene

Concen: 1.678 ng/ul

RT: 13.77 min Scan# 1834

Delta R.T. -0.16 min

Lab File: BM016851.D

Acq: 22 Sep 2018 03:10

Instrument :

BNA_M

ClientSampleId :



Tot Ion:165 Resp: 11327

Ion Ratio Lower Upper

165 100

89 0.0 43.8 65.8#

121 24.7 17.8 26.6

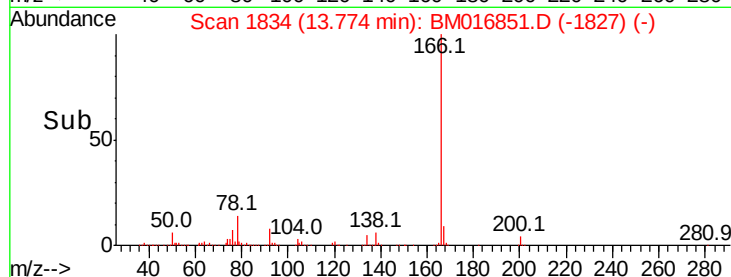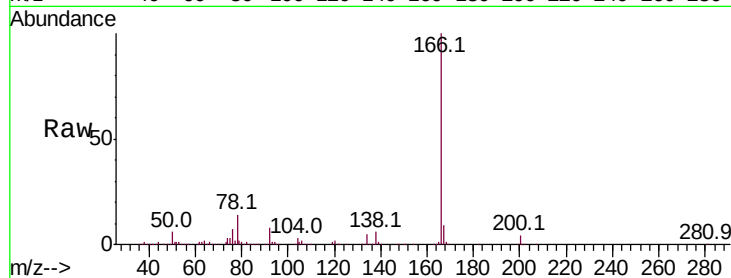

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

