

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
 Data File : BM016854.D
 Acq On : 22 Sep 2018 04:58
 Operator : SJ/JU
 Sample : J5012-20
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C08R1

Quant Time: Sep 22 05:35:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 22 05:13:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	260573	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	1061868	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.36	164	574554	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.10	188	1288845	20.00	ng/ul	0.00
78) Chrysene-d12	21.29	240	1520321	20.00	ng/ul	0.00
86) Perylene-d12	23.53	264	1671285	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	34550	5.67	ng/uL	0.00
5) Phenol-d5	6.89	99	127697	5.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	387381	28.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	431666	24.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	238548	14.03	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	261132	37.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	258817	40.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	472448	29.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.63	131	23502	1.21	ng/ul	0.00
44) Dimethylphthalate-d6	13.77	166	1555944	33.73	ng/ul	0.00
47) Acenaphthylene-d8	14.04	160	1938900	32.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.55	143	38775	5.12	ng/ul	0.00
58) Fluorene-d10	15.35	176	1392381	34.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.47	200	187231	35.39	ng/ul	0.00
71) Anthracene-d10	17.20	188	2217592	35.66	ng/ul	0.00
79) Pyrene-d10	19.50	212	2554405	34.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.39	264	3125167	35.85	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.82	163	176056	3.905	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092118\
Data File : BM016854.D
Acq On : 22 Sep 2018 04:58
Operator : SJ/JU
Sample : J5012-20
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C08R1

Quant Time: Sep 22 05:35:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM091018MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 22 05:13:53 2018
Response via : Initial Calibration

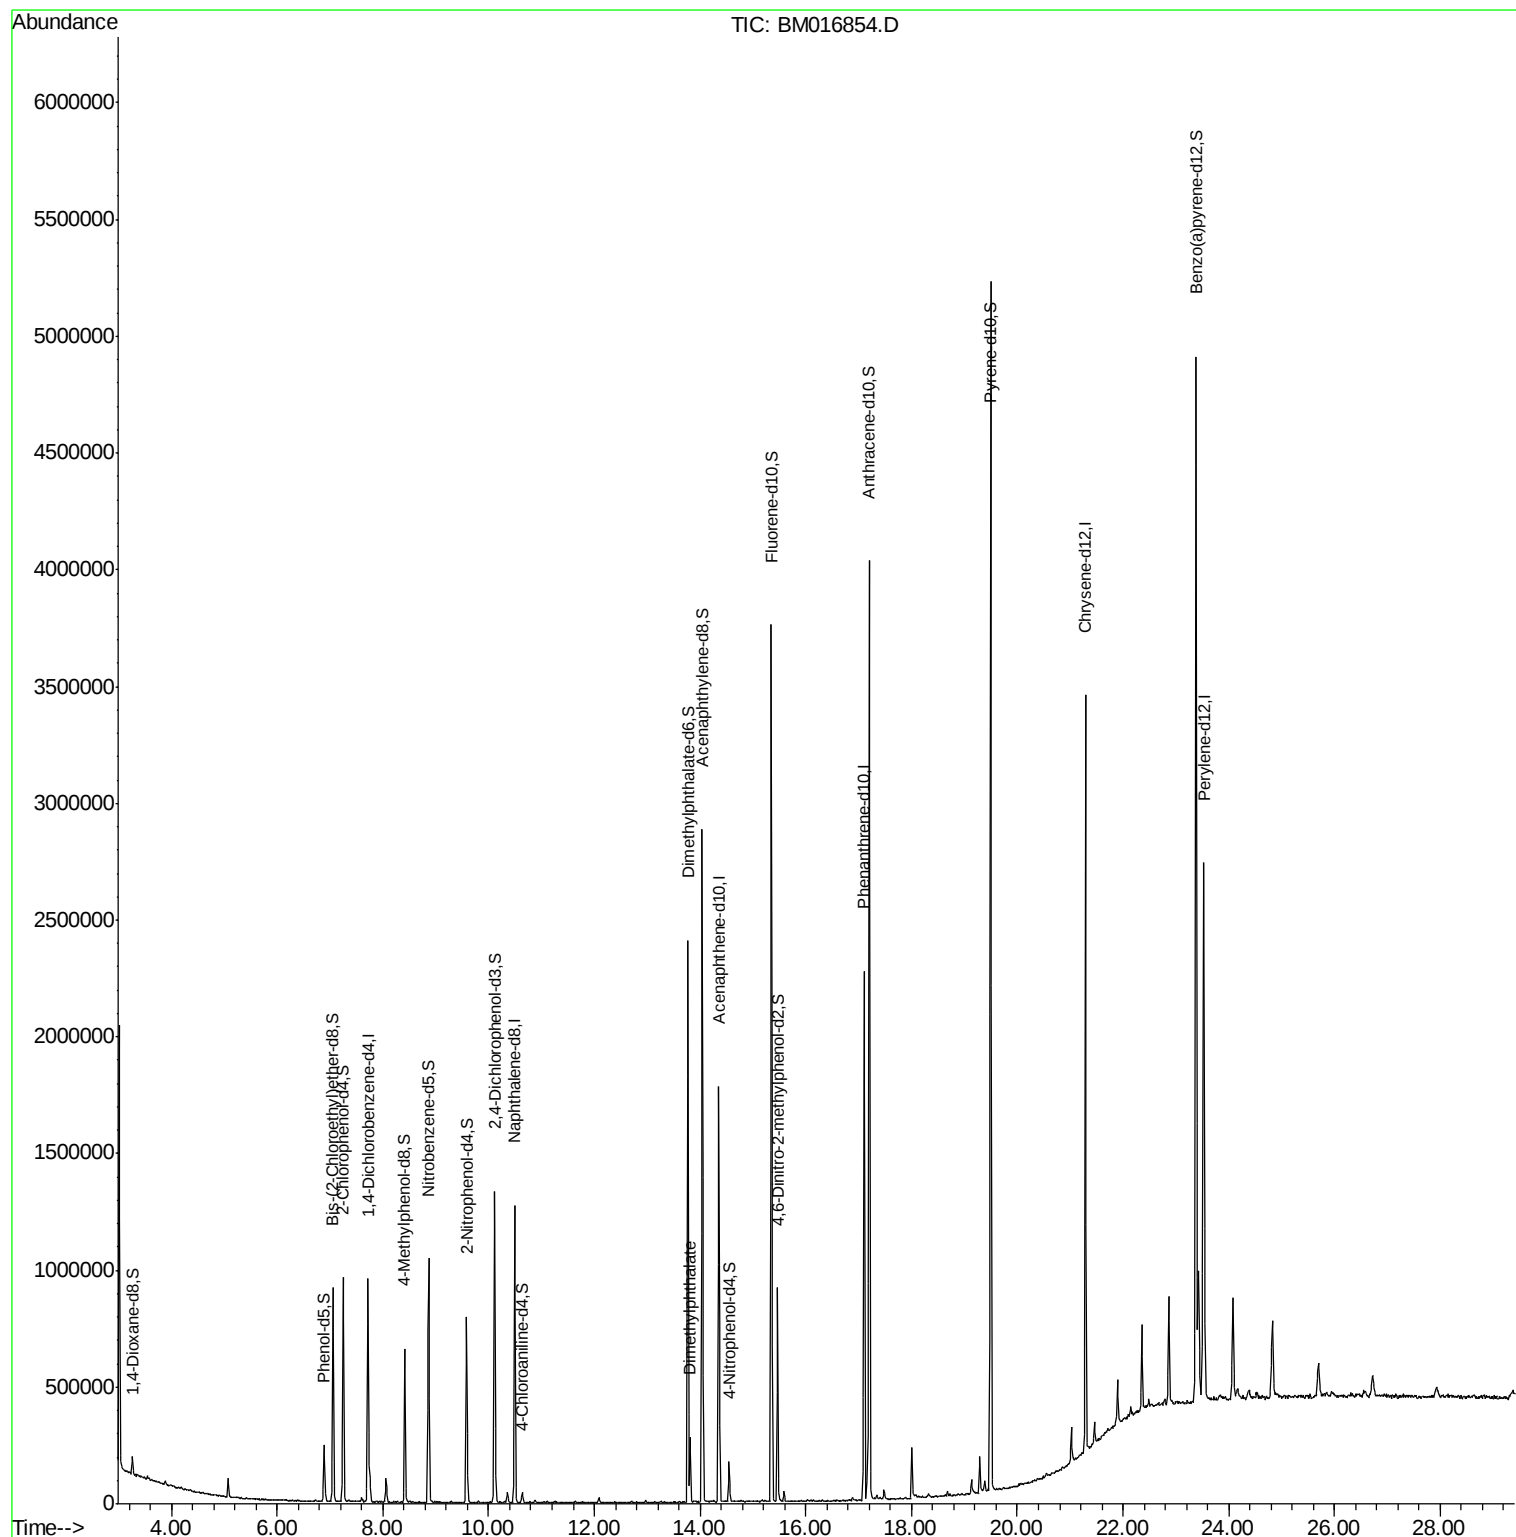

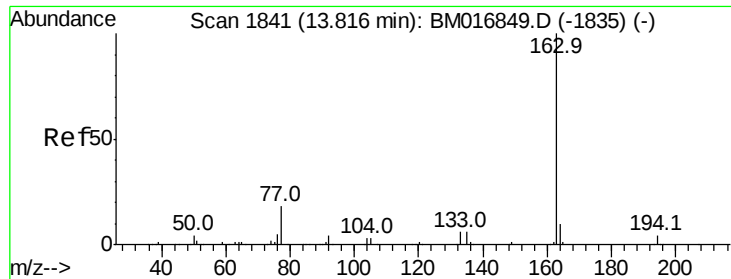

#45

Dimethylphthalate

Concen: 3.905 ng/ul

RT: 13.82 min Scan# 1841

Delta R.T. 0.00 min

Lab File: BM016854.D

Acq: 22 Sep 2018 04:58

Instrument :

BNA_M

ClientSampleId :

C08R1


Tot Ion:163 Resp: 176056

Ion Ratio Lower Upper

163 100

194 4.5 4.0 6.0

164 10.0 8.4 12.6

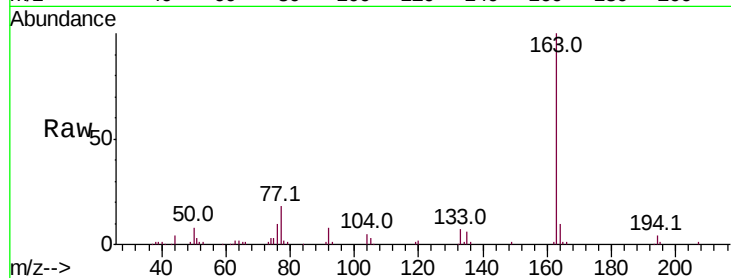

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

