

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092121\
 Data File : BM032121.D
 Acq On : 21 Sep 2021 19:29
 Operator : CG/JU
 Sample : SSTD02027
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027

Quant Time: Sep 22 01:53:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 22 01:45:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.669	152	154456	20.000	ng/u1	0.00
20) Naphthalene-d8	10.469	136	749072	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.322	164	519843	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.045	188	1147768	20.000	ng/u1	0.00
79) Chrysene-d12	21.204	240	1215383	20.000	ng/u1	0.00
88) Perylene-d12	23.380	264	1373910	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.987	96	29687	8.868	ng/uL	0.00
4) Pyridine-d5	3.411	84	233166	24.528	ng/u1	0.00
7) Phenol-d5	6.852	99	273512	21.354	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	170404	22.995	ng/u1	0.00
11) 2-Chlorophenol-d4	7.210	132	196560	19.943	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	225788	20.547	ng/u1	0.00
21) Nitrobenzene-d5	8.822	128	79155	14.549	ng/u1	0.00
24) 2-Nitrophenol-d4	9.551	143	73586	11.428	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	212718	16.466	ng/u1	0.00
31) 4-Chloroaniline-d4	10.598	131	321323	17.633	ng/u1	0.00
46) Dimethylphthalate-d6	13.722	166	709985	18.050	ng/u1	0.00
49) Acenaphthylene-d8	14.010	160	903329	19.391	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	102279	14.365	ng/u1	0.00
60) Fluorene-d10	15.304	176	595778	17.230	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	65144	8.260	ng/u1	0.00
73) Anthracene-d10	17.139	188	958831	17.600	ng/u1	0.00
81) Pyrene-d10	19.427	212	1116681	19.616	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.239	264	1325290	18.354	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.022	88	31565	7.821	ng/uL	99
5) Pyridine	3.434	79	227482	23.277	ng/u1	87
6) Benzaldehyde	6.793	77	192932	33.274	ng/u1	92
8) Phenol	6.875	94	281415	21.835	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.087	93	224024	22.822	ng/u1	93
12) 2-Chlorophenol	7.240	128	205079	20.837	ng/u1	98
13) 2-Methylphenol	8.128	108	218249	21.962	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.210	45	291346	22.838	ng/u1#	90
16) Acetophenone	8.487	105	367562	21.357	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.475	70	202996	24.177	ng/u1#	87
18) 4-Methylphenol	8.457	108	237414	21.514	ng/u1	96
19) Hexachloroethane	8.763	117	84804	20.114	ng/u1	92
22) Nitrobenzene	8.863	77	229073	16.677	ng/u1	94
23) Isophorone	9.387	82	589267	23.309	ng/u1	98
25) 2-Nitrophenol	9.581	139	85141	12.693	ng/u1	93
26) 2,4-Dimethylphenol	9.651	107	276988	20.287	ng/u1	97
27) Bis(2-Chloroethoxy)met...	9.875	93	330865	22.079	ng/u1	100
29) 2,4-Dichlorophenol	10.122	162	208160	16.940	ng/u1	97
30) Naphthalene	10.516	128	715515	19.081	ng/u1	98
32) 4-Chloroaniline	10.622	127	333029	18.320	ng/u1	99
33) Hexachlorobutadiene	10.828	225	132607	16.267	ng/u1	98
34) Caprolactam	11.334	113	87472	21.356	ng/u1	92
35) 4-Chloro-3-methylphenol	11.757	107	262452	20.367	ng/u1	94
36) 2-Methylnaphthalene	12.134	142	509584	17.235	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092121\
 Data File : BM032121.D
 Acq On : 21 Sep 2021 19:29
 Operator : CG/JU
 Sample : SST02027
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST020027


Quant Time: Sep 22 01:53:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 22 01:45:17 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.351	142	519996	17.267	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.516	216	261649	17.534	ng/ul	98
40) Hexachlorocyclopentadiene	12.510	237	152880	19.034	ng/ul	99
41) 2,4,6-Trichlorophenol	12.751	196	169342	16.940	ng/ul	98
42) 2,4,5-Trichlorophenol	12.822	196	176264	16.236	ng/ul	99
43) 1,1'-Biphenyl	13.151	154	699849	19.139	ng/ul	100
44) 2-Chloronaphthalene	13.187	162	533207	18.406	ng/ul	96
45) 2-Nitroaniline	13.386	65	113579	14.231	ng/ul	95
47) Dimethylphthalate	13.769	163	709961	18.381	ng/ul	99
48) 2,6-Dinitrotoluene	13.881	165	92773	12.175	ng/ul	92
50) Acenaphthylene	14.039	152	919028	21.440	ng/ul	99
51) 3-Nitroaniline	14.210	138	108947	15.279	ng/ul#	89
52) Acenaphthene	14.381	153	595119	19.117	ng/ul	99
53) 2,4-Dinitrophenol	14.410	184	39577	7.429	ng/ul	90
55) 4-Nitrophenol	14.528	109	102529	15.598	ng/ul	89
56) Dibenzofuran	14.716	168	842734	18.356	ng/ul	96
57) 2,4-Dinitrotoluene	14.669	165	140984	12.336	ng/ul#	99
58) 2,3,4,6-Tetrachlorophenol	14.951	232	152444	15.642	ng/ul#	97
59) Diethylphthalate	15.133	149	740818	18.766	ng/ul	99
61) Fluorene	15.363	166	682049	17.558	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.357	204	332539	16.715	ng/ul	97
63) 4-Nitroaniline	15.369	138	117655	18.420	ng/ul#	83
66) 4,6-Dinitro-2-methylph...	15.433	198	67653	8.822	ng/ul	96
67) N-Nitrosodiphenylamine	15.563	169	614442	18.641	ng/ul	99
68) 4-Bromophenyl-phenylether	16.239	248	207815	17.668	ng/ul	94
69) Hexachlorobenzene	16.375	284	232973	17.060	ng/ul	96
70) Atrazine	16.504	200	241846	19.474	ng/ul	98
71) Pentachlorophenol	16.710	266	124658	13.959	ng/ul	97
72) Phenanthrene	17.086	178	1122013	17.898	ng/ul	100
74) Anthracene	17.174	178	1153241	17.975	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.122	216	285960	19.146	ng/ul	99
76) Pentachlorobenzene	14.651	250	279730	17.852	ng/ul	98
77) Carbazole	17.439	167	1097492	18.691	ng/ul	98
78) Di-n-butylphthalate	17.998	149	1321230	19.637	ng/ul	99
80) Fluoranthene	19.092	202	1396170	20.183	ng/ul	97
82) Pyrene	19.457	202	1418741	19.372	ng/ul	97
83) Butylbenzylphthalate	20.345	149	567002	19.717	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.121	252	519104	18.972	ng/ul	98
85) Benzo(a)anthracene	21.192	228	1437477	19.014	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.115	149	898561	19.375	ng/ul	99
87) Chrysene	21.239	228	1389158	19.104	ng/ul	99
89) Di-n-octyl phthalate	21.962	149	1579462	16.851	ng/ul	100
90) Benzo(b)fluoranthene	22.727	252	1578001	18.027	ng/ul	99
91) Benzo(k)fluoranthene	22.768	252	1419234	16.747	ng/ul	99
93) Benzo(a)pyrene	23.280	252	1525674	19.301	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.533	276	1795749	17.750	ng/ul	96
95) Dibenzo(a,h)anthracene	25.539	278	1516637	17.825	ng/ul	99
96) Benzo(g,h,i)perylene	26.197	276	1547954	18.478	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :
BNA_M
ClientSampleId :
SSTD020027

Quant Time: Sep 22 01:53:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM092121.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 22 01:45:17 2021
Response via : Initial Calibration




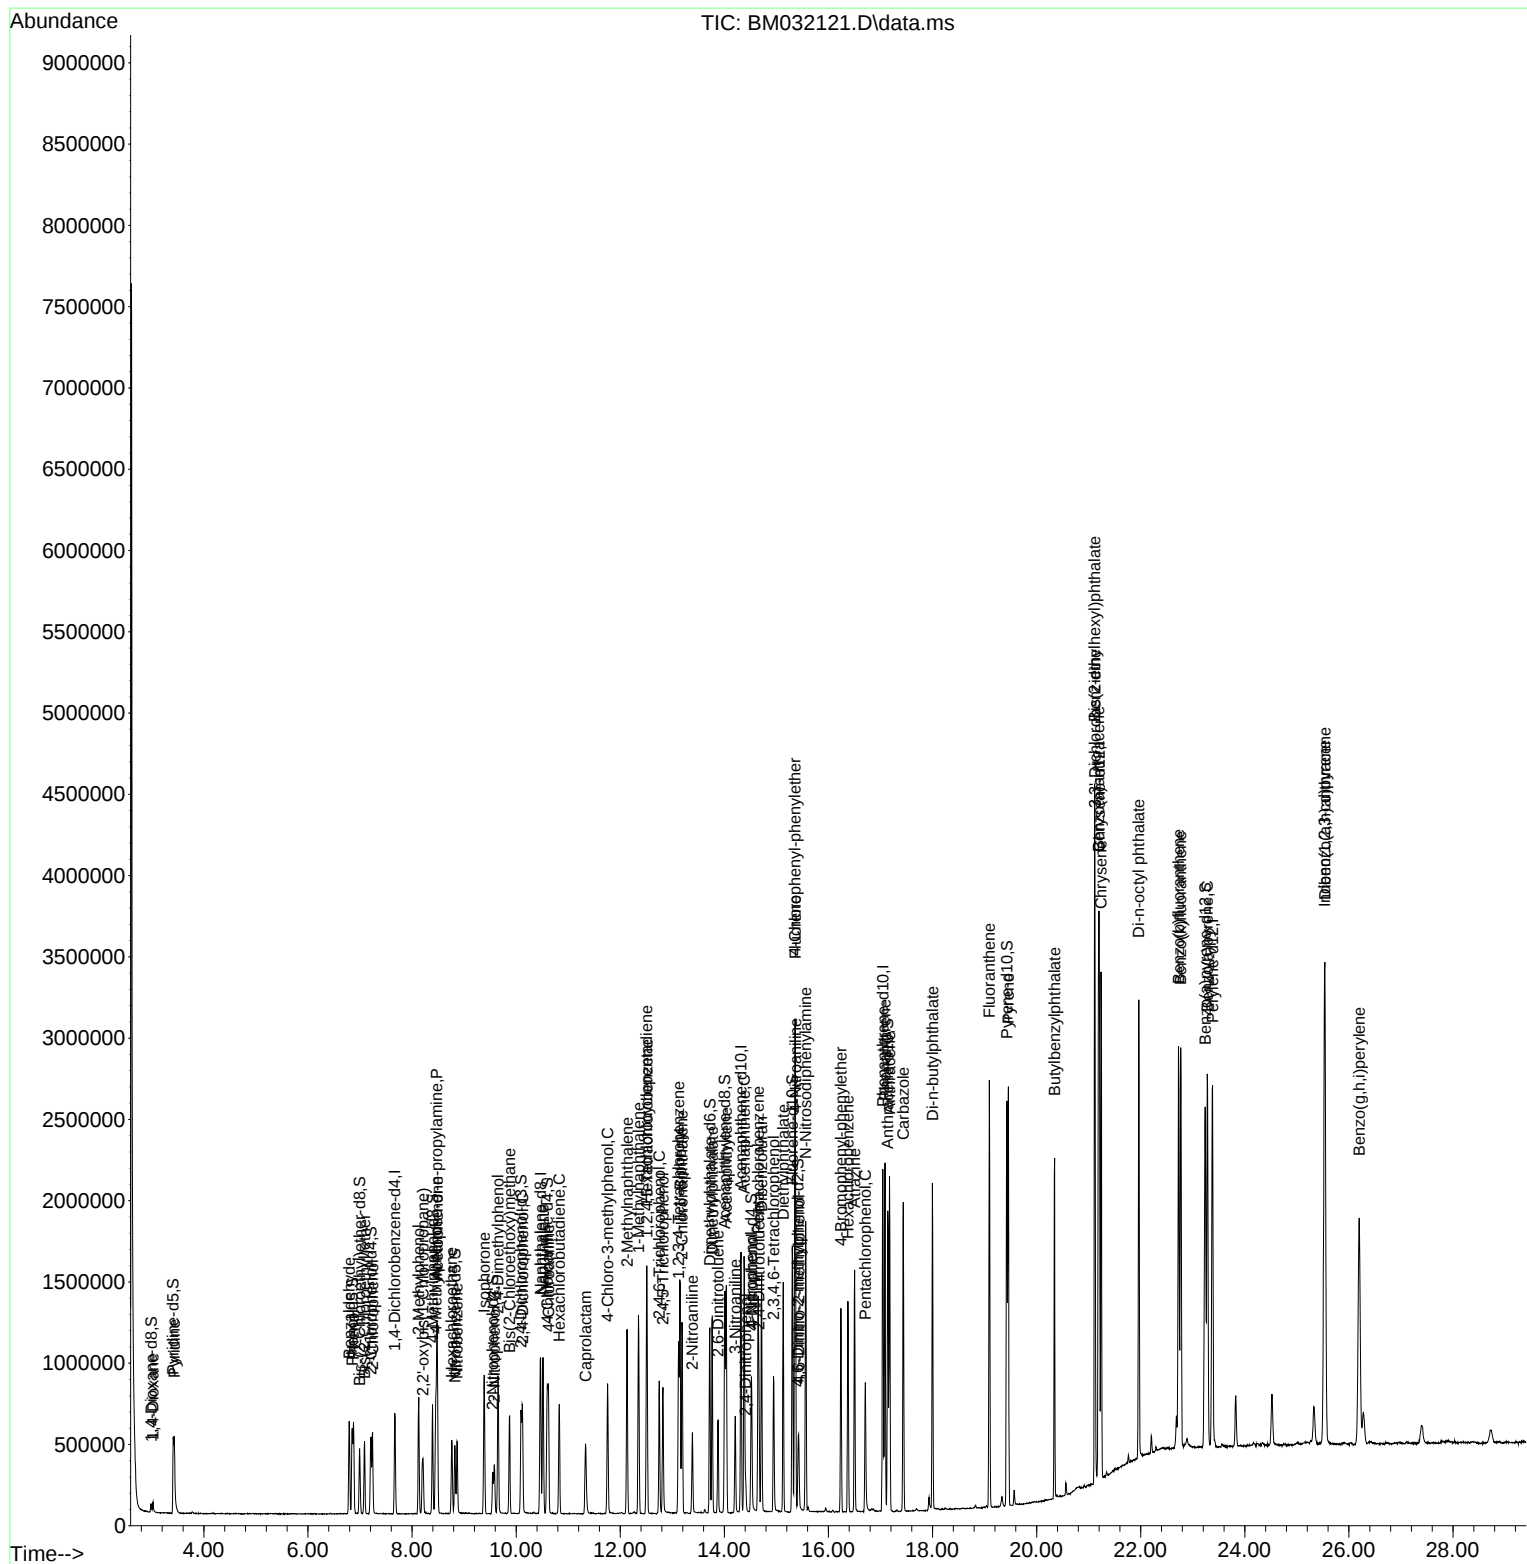




#2
1,4-Dioxane
Concen: 7.821 ng/uL
RT: 3.022 min Scan# 74
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:	88	Resp:	31565
Ion	Ratio	Lower	Upper
88	100		
43	39.2	31.5	47.3
58	79.4	64.1	96.1

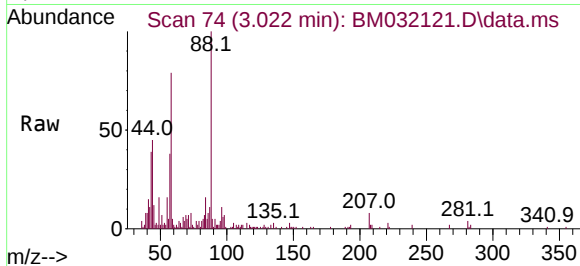

#5
Pyridine
Concen: 23.277 ng/uL
RT: 3.434 min Scan# 144
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:	79	Resp:	227482
Ion	Ratio	Lower	Upper
79	100		
52	73.4	69.9	104.9
51	36.1	33.8	50.6



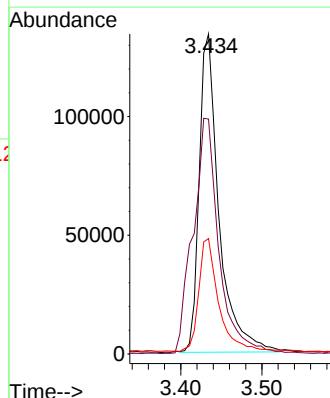
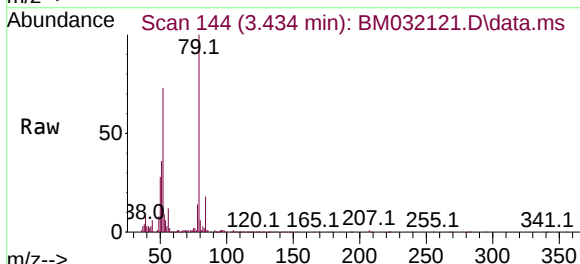




#6
Benzaldehyde
Concen: 33.274 ng/ul
RT: 6.793 min Scan# 715
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion: 77 Resp: 192932
Ion Ratio Lower Upper
77 100
105 92.6 82.2 123.4
106 88.6 75.0 112.4

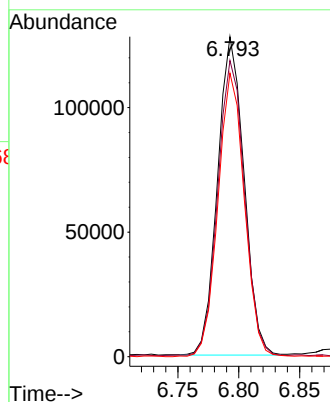

#8
Phenol
Concen: 21.835 ng/ul
RT: 6.875 min Scan# 729
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion: 94 Resp: 281415
Ion Ratio Lower Upper
94 100
65 30.3 24.2 36.4
66 40.2 31.4 47.0









#10
Bis(2-Chloroethyl)ether
Concen: 22.822 ng/ul
RT: 7.087 min Scan# 765
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion: 93 Resp: 224024
Ion Ratio Lower Upper
93 100
63 77.1 68.0 102.0
95 33.5 25.8 38.6



#12
2-Chlorophenol
Concen: 20.837 ng/ul
RT: 7.240 min Scan# 791
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:128 Resp: 205079
Ion Ratio Lower Upper
128 100
64 50.8 39.2 58.8
130 32.5 25.3 37.9









#13
2-Methylphenol
Concen: 21.962 ng/ul
RT: 8.128 min Scan# 942
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:108 Resp: 218249
Ion Ratio Lower Upper
108 100
107 90.2 70.6 105.8

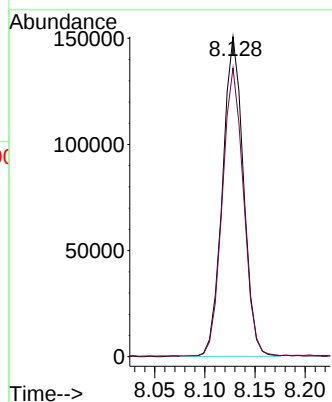

#14
2,2'-oxybis(1-Chloropropane)
Concen: 22.838 ng/ul
RT: 8.210 min Scan# 956
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion: 45 Resp: 291346
Ion Ratio Lower Upper
45 100
77 16.7 10.2 15.4#
79 13.2 7.8 11.8#



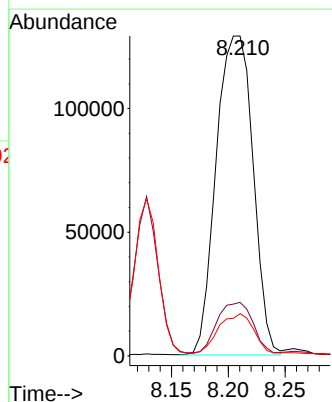



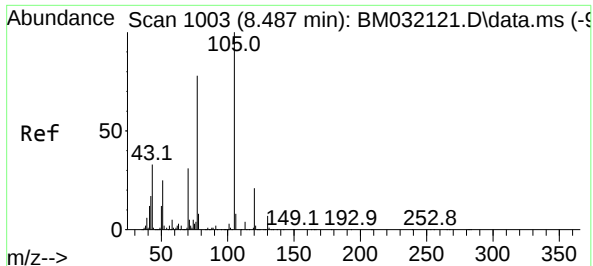

#16
Acetophenone
Concen: 21.357 ng/ul
RT: 8.487 min Scan# 1003
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:105 Resp: 367562
Ion Ratio Lower Upper
105 100
77 79.5 63.7 95.5
51 26.1 25.4 38.0

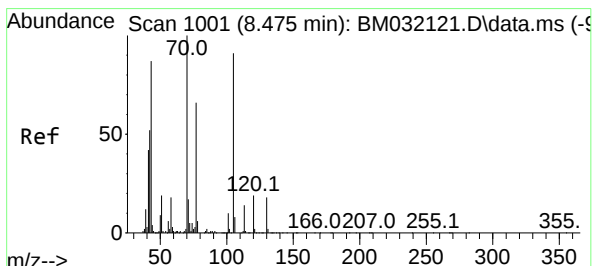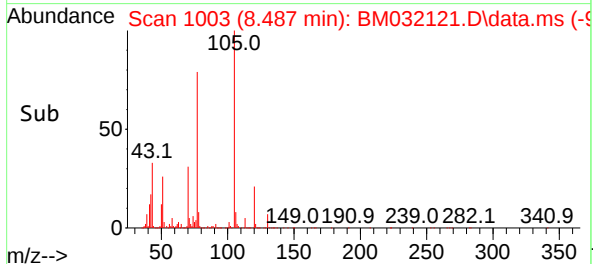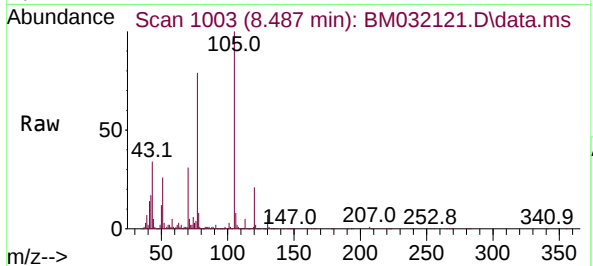

#17
N-Nitroso-di-n-propylamine
Concen: 24.177 ng/ul
RT: 8.475 min Scan# 1001
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion: 70 Resp: 202996
Ion Ratio Lower Upper
70 100
42 52.9 53.4 80.0#
101 9.7 7.4 11.0
130 18.3 16.8 25.2


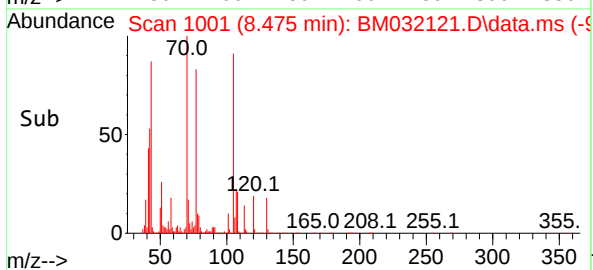

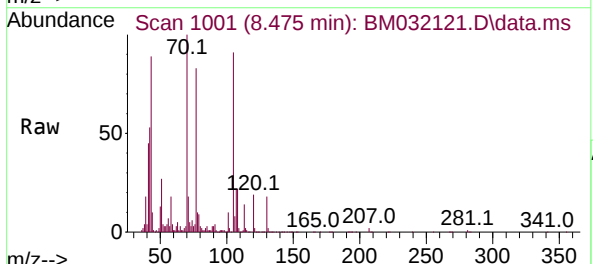




#18
4-Methylphenol
Concen: 21.514 ng/ul
RT: 8.457 min Scan# 998
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:108 Resp: 237414
Ion Ratio Lower Upper
108 100
107 113.1 87.0 130.6



#19
Hexachloroethane
Concen: 20.114 ng/ul
RT: 8.763 min Scan# 1050
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:117 Resp: 84804
Ion Ratio Lower Upper
117 100
201 91.9 80.1 120.1
199 57.9 50.8 76.2

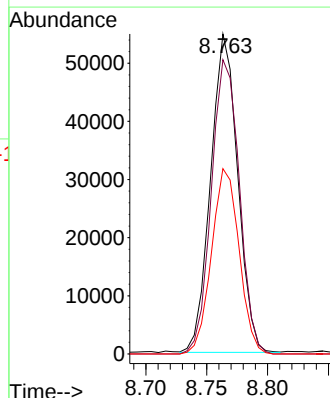



#22

Nitrobenzene

Concen: 16.677 ng/ul

RT: 8.863 min Scan# 1067

Delta R.T. 0.000 min

Lab File: BM032121.D

Acq: 21 Sep 2021 19:29

Tgt Ion: 77 Resp: 229073





Ion	Ratio	Lower	Upper
77	100		
123	39.0	34.8	52.2
65	14.3	10.4	15.6

Instrument :

BNA_M

ClientSampleId :

SSTD020027



#23

Isophorone

Concen: 23.309 ng/ul

RT: 9.387 min Scan# 1156




Delta R.T. 0.000 min


Lab File: BM032121.D

Acq: 21 Sep 2021 19:29

Tgt Ion: 82 Resp: 589267

Ion	Ratio	Lower	Upper
82	100		
95	7.5	5.3	7.9
138	16.3	13.6	20.4









#25
2-Nitrophenol
Concen: 12.693 ng/ul
RT: 9.581 min Scan# 1189
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:	139	Resp:	85141
Ion Ratio	Lower	Upper	
139	100		
65	58.1	43.7	65.5
109	35.6	24.0	36.0



#26
2,4-Dimethylphenol
Concen: 20.287 ng/ul
RT: 9.651 min Scan# 1201
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:	107	Resp:	276988
Ion Ratio	Lower	Upper	
107	100		
121	48.7	41.0	61.6
122	82.6	68.2	102.2









#27
 Bis(2-Chloroethoxy)methane
 Concen: 22.079 ng/ul
 RT: 9.875 min Scan# 1239
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027

Tgt Ion: 93 Resp: 330865




Ion	Ratio	Lower	Upper
93	100		
95	32.4	25.9	38.9
123	10.0	8.5	12.7

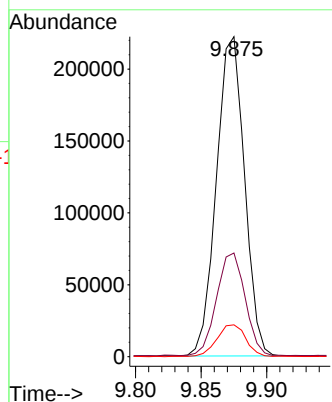


#29
 2,4-Dichlorophenol
 Concen: 16.940 ng/ul
 RT: 10.122 min Scan# 1281
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29

Tgt Ion: 162 Resp: 208160

Ion	Ratio	Lower	Upper
162	100		
164	64.0	51.6	77.4
98	39.6	28.2	42.4









#30
Naphthalene
Concen: 19.081 ng/ul
RT: 10.516 min Scan# 1348
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:128 Resp: 715515
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.4
127 14.3 10.6 15.8

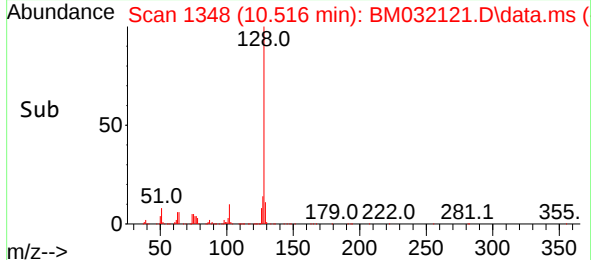

#32
4-Chloroaniline
Concen: 18.320 ng/ul
RT: 10.622 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:127 Resp: 333029
Ion Ratio Lower Upper
127 100
129 32.5 25.6 38.4


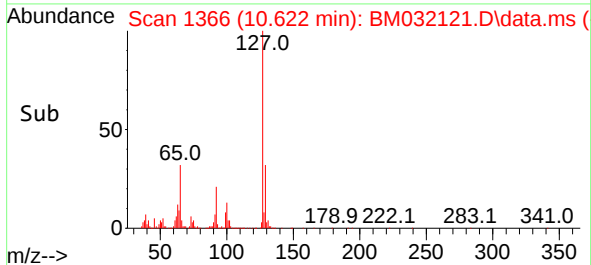






#33
Hexachlorobutadiene
Concen: 16.267 ng/ul
RT: 10.828 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:225 Resp: 132607
Ion Ratio Lower Upper
225 100
223 63.2 50.7 76.1
227 66.1 50.7 76.1

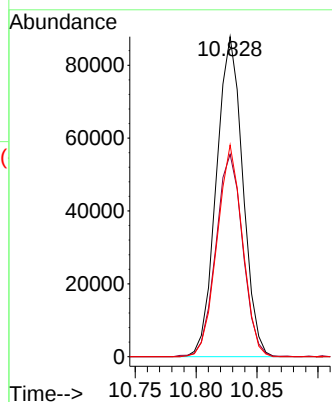

#34
Caprolactam
Concen: 21.356 ng/ul
RT: 11.334 min Scan# 1487
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:113 Resp: 87472
Ion Ratio Lower Upper
113 100
55 182.6 155.2 232.8
56 136.2 101.9 152.9



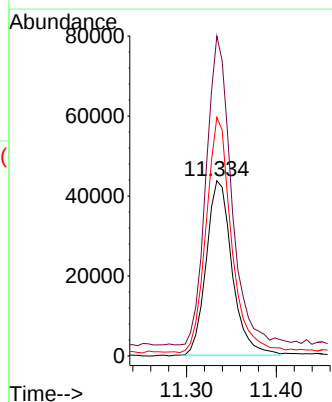





#35
4-Chloro-3-methylphenol
Concen: 20.367 ng/ul
RT: 11.757 min Scan# 1559
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:107 Resp: 262452
Ion Ratio Lower Upper
107 100
144 24.6 22.3 33.5
142 76.5 65.6 98.4

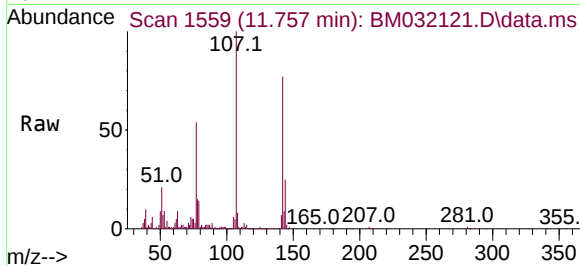

#36
2-Methylnaphthalene
Concen: 17.235 ng/ul
RT: 12.134 min Scan# 1623
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:142 Resp: 509584
Ion Ratio Lower Upper
142 100
141 90.4 70.6 105.8



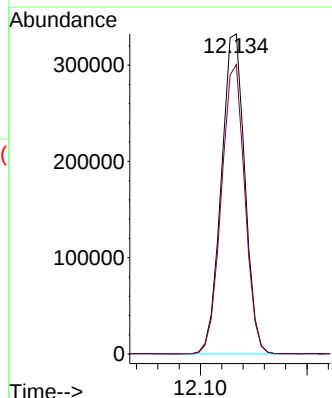
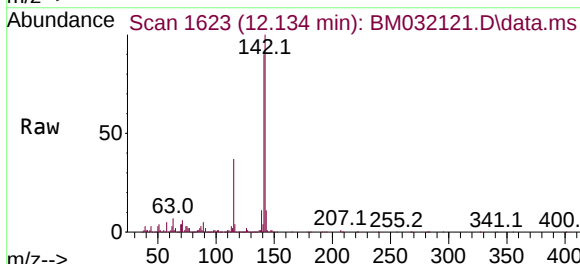




#37
1-Methylnaphthalene
Concen: 17.267 ng/ul
RT: 12.351 min Scan# 1660
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:142 Resp: 519996
Ion Ratio Lower Upper
142 100
141 91.5 72.8 109.2
116 4.1 3.1 4.7



#39
1,2,4,5-Tetrachlorobenzene
Concen: 17.534 ng/ul
RT: 12.516 min Scan# 1688
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:216 Resp: 261649
Ion Ratio Lower Upper
216 100
214 78.2 62.2 93.4
179 22.3 16.6 24.8
108 19.8 13.5 20.3



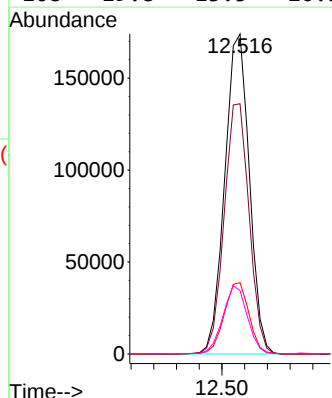





#40
Hexachlorocyclopentadiene
Concen: 19.034 ng/ul
RT: 12.510 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:237 Resp: 152880
Ion Ratio Lower Upper
237 100
235 61.4 49.0 73.4
272 12.1 11.0 16.4

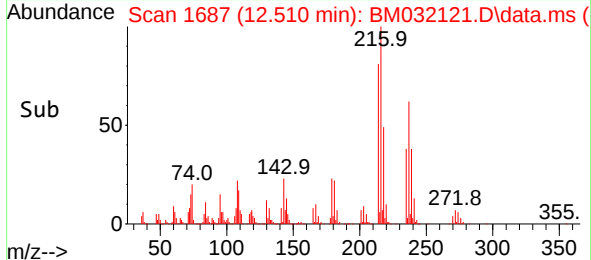

#41
2,4,6-Trichlorophenol
Concen: 16.940 ng/ul
RT: 12.751 min Scan# 1728
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:196 Resp: 169342
Ion Ratio Lower Upper
196 100
198 95.8 78.8 118.2
200 31.6 26.0 39.0


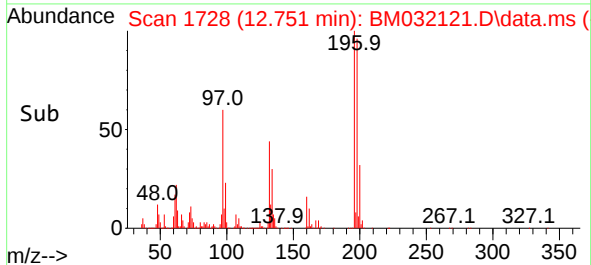






#42
2,4,5-Trichlorophenol
Concen: 16.236 ng/ul
RT: 12.822 min Scan# 1740
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:196 Resp: 176264
Ion Ratio Lower Upper
196 100
198 96.7 76.1 114.1
200 31.3 25.4 38.2



#43
1,1'-Biphenyl
Concen: 19.139 ng/ul
RT: 13.151 min Scan# 1796
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:154 Resp: 699849
Ion Ratio Lower Upper
154 100
153 40.3 32.3 48.5
76 13.3 10.6 15.8









#44
2-Chloronaphthalene
Concen: 18.406 ng/ul
RT: 13.187 min Scan# 1802
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Instrument :
BNA_M
ClientSampleId :
SSTD020027

Tgt Ion:162 Resp: 533207




Ion	Ratio	Lower	Upper
162	100		
164	32.3	26.2	39.4
127	40.4	29.4	44.0




#45
2-Nitroaniline
Concen: 14.231 ng/ul
RT: 13.386 min Scan# 1836
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion: 65 Resp: 113579

Ion	Ratio	Lower	Upper
65	100		
92	71.9	53.9	80.9
138	98.7	83.3	124.9









#47
Dimethylphthalate
Concen: 18.381 ng/ul
RT: 13.769 min Scan# 1901
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:163 Resp: 709961
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 9.9 8.2 12.4

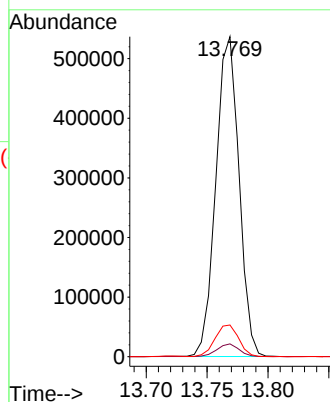

#48
2,6-Dinitrotoluene
Concen: 12.175 ng/ul
RT: 13.881 min Scan# 1920
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:165 Resp: 92773
Ion Ratio Lower Upper
165 100
89 66.4 48.6 72.8
121 26.2 18.1 27.1


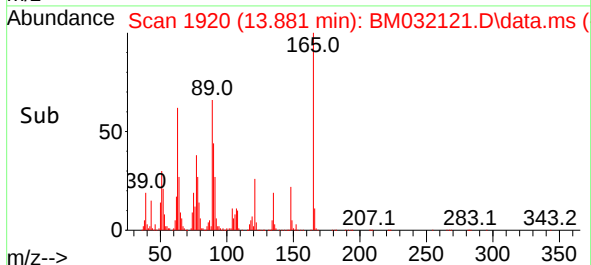






#50
Acenaphthylene
Concen: 21.440 ng/ul
RT: 14.039 min Scan# 1947
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:152 Resp: 919028
Ion Ratio Lower Upper
152 100
151 20.9 16.2 24.2
153 12.8 10.2 15.4



#51
3-Nitroaniline
Concen: 15.279 ng/ul
RT: 14.210 min Scan# 1976
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:138 Resp: 108947
Ion Ratio Lower Upper
138 100
108 30.3 7.4 11.2#
92 129.2 96.5 144.7









#52
Acenaphthene
Concen: 19.117 ng/ul
RT: 14.381 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:153 Resp: 595119
Ion Ratio Lower Upper
153 100
152 46.2 37.4 56.2
154 85.8 69.4 104.0



#53
2,4-Dinitrophenol
Concen: 7.429 ng/ul
RT: 14.410 min Scan# 2010
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:184 Resp: 39577
Ion Ratio Lower Upper
184 100
63 61.3 56.9 85.3
154 67.1 49.0 73.6


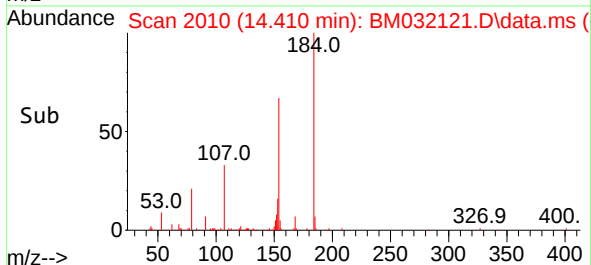
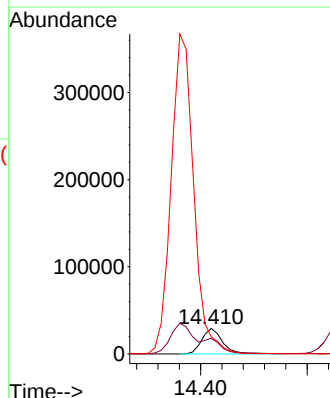





#55
4-Nitrophenol
Concen: 15.598 ng/ul
RT: 14.528 min Scan# 2030
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:109 Resp: 102529
Ion Ratio Lower Upper
109 100
139 113.6 100.3 150.5
65 117.6 104.6 156.8



#56
Dibenzofuran
Concen: 18.356 ng/ul
RT: 14.716 min Scan# 2062
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:168 Resp: 842734
Ion Ratio Lower Upper
168 100
139 39.2 29.5 44.3









#57
2,4-Dinitrotoluene
Concen: 12.336 ng/ul
RT: 14.669 min Scan# 2054
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:165 Resp: 140984
Ion Ratio Lower Upper
165 100
63 46.4 37.6 56.4
182 3.7 1.8 2.8#



#58
2,3,4,6-Tetrachlorophenol
Concen: 15.642 ng/ul
RT: 14.951 min Scan# 2102
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:232 Resp: 152444
Ion Ratio Lower Upper
232 100
131 45.4 35.0 52.6
130 3.1 1.7 2.5#
166 32.0 24.4 36.6









#59
Diethylphthalate
Concen: 18.766 ng/ul
RT: 15.133 min Scan# 2133
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:149 Resp: 740818
Ion Ratio Lower Upper
149 100
177 21.7 17.0 25.4
150 12.2 9.9 14.9



#61
Fluorene
Concen: 17.558 ng/ul
RT: 15.363 min Scan# 2172
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:166 Resp: 682049
Ion Ratio Lower Upper
166 100
165 99.2 78.4 117.6
167 13.2 10.6 15.8









#62
4-Chlorophenyl-phenylether
Concen: 16.715 ng/ul
RT: 15.357 min Scan# 2171
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:204 Resp: 332539
Ion Ratio Lower Upper
204 100
206 33.1 26.0 39.0
141 60.5 45.6 68.4

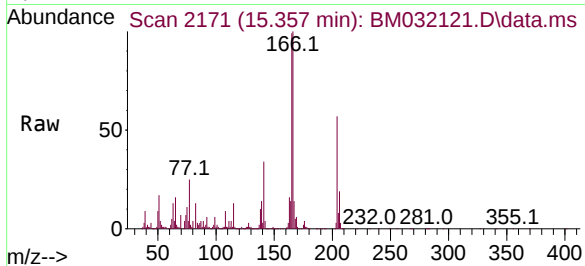

#63
4-Nitroaniline
Concen: 18.420 ng/ul
RT: 15.369 min Scan# 2173
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:138 Resp: 117655
Ion Ratio Lower Upper
138 100
92 58.3 41.5 62.3
108 96.7 61.4 92.2#




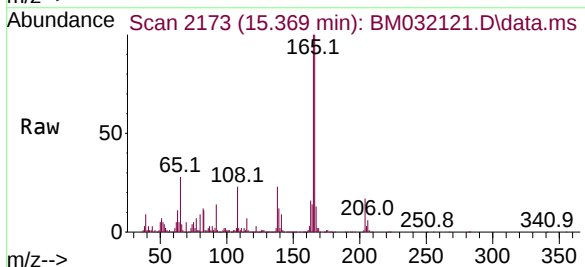




#66
 4,6-Dinitro-2-methylphenol
 Concen: 8.822 ng/ul
 RT: 15.433 min Scan# 2184
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027


Tgt Ion:198 Resp: 67653
 Ion Ratio Lower Upper
 198 100
 182 4.8 3.8 5.6
 77 27.5 20.1 30.1



#67
 N-Nitrosodiphenylamine
 Concen: 18.641 ng/ul
 RT: 15.563 min Scan# 2206
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29

Tgt Ion:169 Resp: 614442
 Ion Ratio Lower Upper
 169 100
 168 66.4 53.8 80.6
 167 36.6 28.6 43.0









#68
4-Bromophenyl-phenylether
Concen: 17.668 ng/ul
RT: 16.239 min Scan# 2321
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:	248	Resp:	207815
Ion Ratio	Lower	Upper	
248	100		
250	96.6	78.6	118.0
141	80.4	56.2	84.2

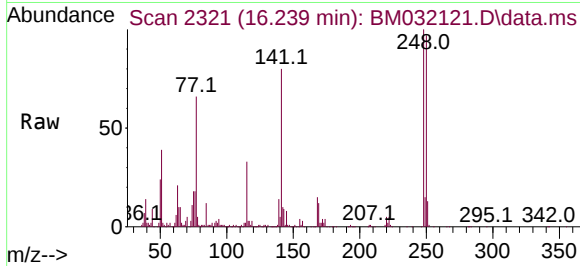

#69
Hexachlorobenzene
Concen: 17.060 ng/ul
RT: 16.375 min Scan# 2344
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:	284	Resp:	232973
Ion Ratio	Lower	Upper	
284	100		
142	39.0	29.0	43.4
249	33.1	25.0	37.4




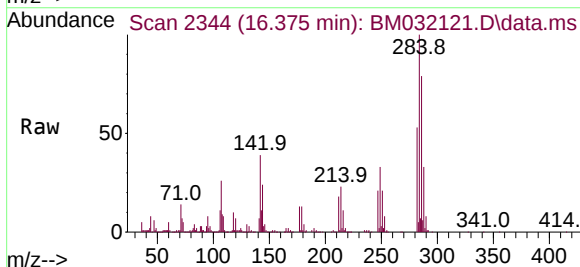




#70
Atrazine
Concen: 19.474 ng/ul
RT: 16.504 min Scan# 2366
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:200 Resp: 241846
Ion Ratio Lower Upper
200 100
173 25.2 18.7 28.1
215 49.0 38.9 58.3



#71
Pentachlorophenol
Concen: 13.959 ng/ul
RT: 16.710 min Scan# 2401
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:266 Resp: 124658
Ion Ratio Lower Upper
266 100
264 63.9 48.2 72.4
268 64.1 51.6 77.4


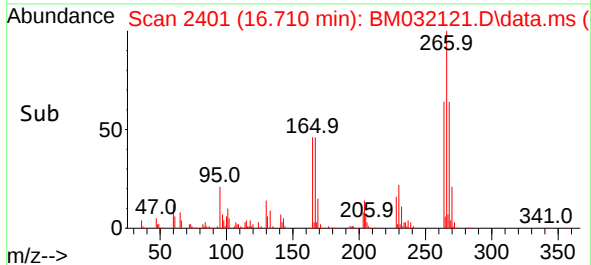






#72
Phenanthrene
Concen: 17.898 ng/ul
RT: 17.086 min Scan# 2465
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:178 Resp: 1122013
Ion Ratio Lower Upper
178 100
179 15.2 12.1 18.1
176 19.2 15.2 22.8



#74
Anthracene
Concen: 17.975 ng/ul
RT: 17.174 min Scan# 2480
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:178 Resp: 1153241
Ion Ratio Lower Upper
178 100
179 14.9 12.1 18.1
176 18.8 15.2 22.8


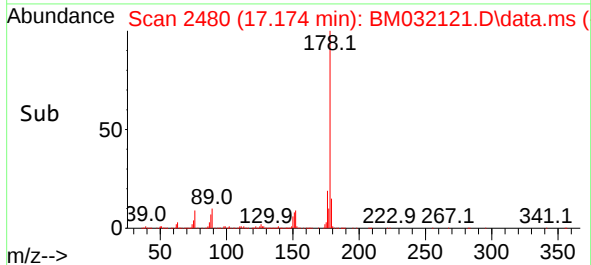






#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.146 ng/uL
RT: 13.122 min Scan# 1791
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:216 Resp: 285960
Ion Ratio Lower Upper
216 100
214 77.3 61.9 92.9
218 47.5 39.5 59.3

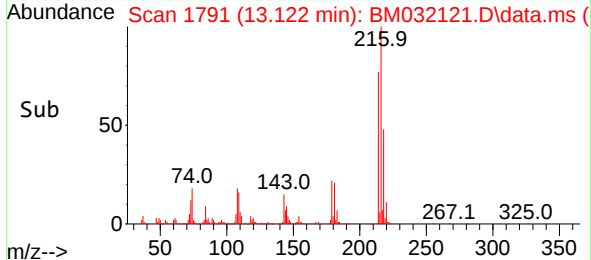

#76
Pentachlorobenzene
Concen: 17.852 ng/uL
RT: 14.651 min Scan# 2051
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:250 Resp: 279730
Ion Ratio Lower Upper
250 100
248 61.0 50.2 75.4
252 63.3 52.2 78.2


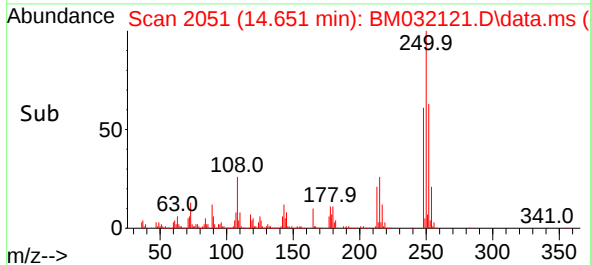






#77
 Carbazole
 Concen: 18.691 ng/ul
 RT: 17.439 min Scan# 2525
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29




Instrument :
 BNA_M
 ClientSampleId :
 SST020027


Tgt Ion:167 Resp: 1097492
 Ion Ratio Lower Upper
 167 100
 166 22.3 17.0 25.6
 139 13.3 9.9 14.9

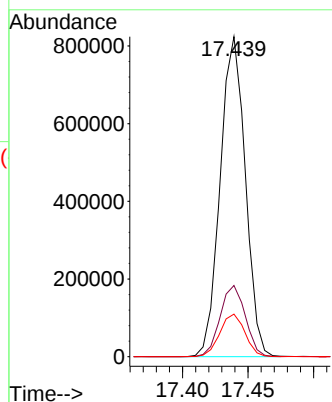

#78
 Di-n-butylphthalate
 Concen: 19.637 ng/ul
 RT: 17.998 min Scan# 2620
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29

Tgt Ion:149 Resp: 1321230
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.3 10.9
 104 5.6 4.1 6.1



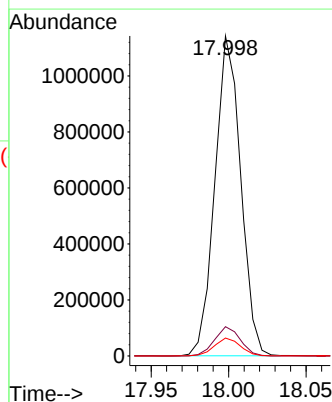





#80
 Fluoranthene
 Concen: 20.183 ng/u1
 RT: 19.092 min Scan# 2806
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020027


Tgt Ion:202 Resp: 1396170
 Ion Ratio Lower Upper
 202 100
 101 12.1 8.8 13.2
 100 9.5 6.8 10.2



#82
 Pyrene
 Concen: 19.372 ng/u1
 RT: 19.457 min Scan# 2868
 Delta R.T. 0.000 min
 Lab File: BM032121.D
 Acq: 21 Sep 2021 19:29

Tgt Ion:202 Resp: 1418741
 Ion Ratio Lower Upper
 202 100
 101 13.7 10.0 15.0
 100 11.8 8.5 12.7


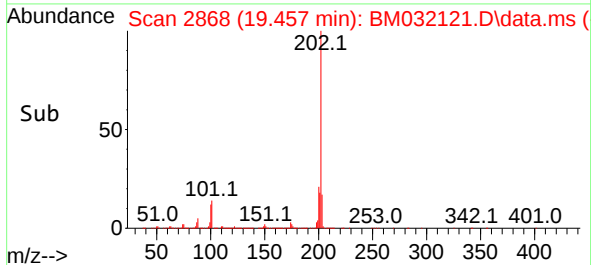






#83
Butylbenzylphthalate
Concen: 19.717 ng/ul
RT: 20.345 min Scan# 3019
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:149 Resp: 567002
Ion Ratio Lower Upper
149 100
91 75.8 57.4 86.2
206 21.0 15.9 23.9



#84
3,3'-Dichlorobenzidine
Concen: 18.972 ng/ul
RT: 21.121 min Scan# 3151
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:252 Resp: 519104
Ion Ratio Lower Upper
252 100
254 64.0 49.9 74.9
126 12.2 8.9 13.3









#85
Benzo(a)anthracene
Concen: 19.014 ng/ul
RT: 21.192 min Scan# 3163
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:228 Resp: 1437477
Ion Ratio Lower Upper
228 100
229 19.5 16.0 24.0
226 27.1 22.2 33.2

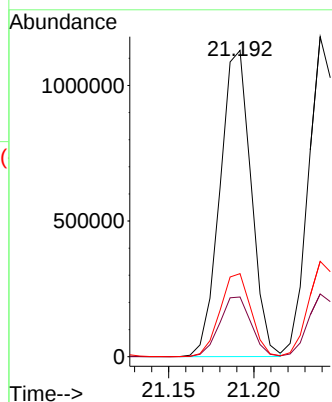

#86
Bis(2-ethylhexyl)phthalate
Concen: 19.375 ng/ul
RT: 21.115 min Scan# 3150
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:149 Resp: 898561
Ion Ratio Lower Upper
149 100
167 26.5 20.7 31.1
279 4.0 3.0 4.4









#87
Chrysene
Concen: 19.104 ng/ul
RT: 21.239 min Scan# 3171
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:228 Resp: 1389158
Ion Ratio Lower Upper
228 100
226 29.8 23.6 35.4
229 19.6 15.9 23.9



#89
Di-n-octyl phthalate
Concen: 16.851 ng/ul
RT: 21.962 min Scan# 3294
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:149 Resp: 1579462




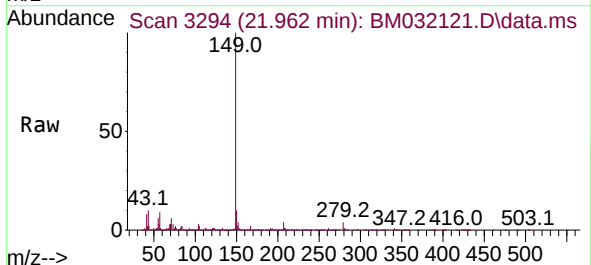




#90
Benzo(b)fluoranthene
Concen: 18.027 ng/ul
RT: 22.727 min Scan# 3424
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:252 Resp: 1578001
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 10.7 7.7 11.5



#91
Benzo(k)fluoranthene
Concen: 16.747 ng/ul
RT: 22.768 min Scan# 3431
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:252 Resp: 1419234
Ion Ratio Lower Upper
252 100
253 22.0 17.4 26.2
125 10.9 7.9 11.9









#93
Benzo(a)pyrene
Concen: 19.301 ng/ul
RT: 23.280 min Scan# 3518
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29




Instrument :
BNA_M
ClientSampleId :
SSTD020027


Tgt Ion:252 Resp: 1525674
Ion Ratio Lower Upper
252 100
253 21.8 17.5 26.3
125 11.8 8.6 13.0



#94
Indeno(1,2,3-cd)pyrene
Concen: 17.750 ng/ul
RT: 25.533 min Scan# 3901
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:276 Resp: 1795749
Ion Ratio Lower Upper
276 100
138 26.8 19.5 29.3
277 25.8 19.6 29.4









#95
Dibenzo(a,h)anthracene
Concen: 17.825 ng/ul
RT: 25.539 min Scan# 3902
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Instrument :
BNA_M
ClientSampleId :
SSTD020027

Tgt Ion:278 Resp: 1516637
Ion Ratio Lower Upper
278 100
139 16.6 12.8 19.2
279 24.2 19.1 28.7



#96
Benzo(g,h,i)perylene
Concen: 18.478 ng/ul
RT: 26.197 min Scan# 4014
Delta R.T. 0.000 min
Lab File: BM032121.D
Acq: 21 Sep 2021 19:29

Tgt Ion:276 Resp: 1547954
Ion Ratio Lower Upper
276 100
138 22.0 16.5 24.7
277 24.2 18.5 27.7

