

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041963.D
 Acq On : 21 Sep 2023 18:45
 Operator : MA/JU
 Sample : 04344-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHK8

Quant Time: Sep 22 03:26:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6615	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	16460	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	8193	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	14133	0.400	ng/ul	0.00
17) Chrysene-d12	21.527	240	5235	0.400	ng/ul	# 0.00
23) Perylene-d12	23.939	264	5749	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	38992	5.030	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	6548	0.290	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	9218	0.477	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.410	88	5132	0.637	ng/ul#	86
20) Pyrene	19.747	202	2805	0.068	ng/ul#	1
26) Benzo(a)pyrene	23.784	252	3779	0.137	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041963.D
Acq On : 21 Sep 2023 18:45
Operator : MA/JU
Sample : 04344-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHK8

Quant Time: Sep 22 03:26:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:25:00 2023
Response via : Initial Calibration




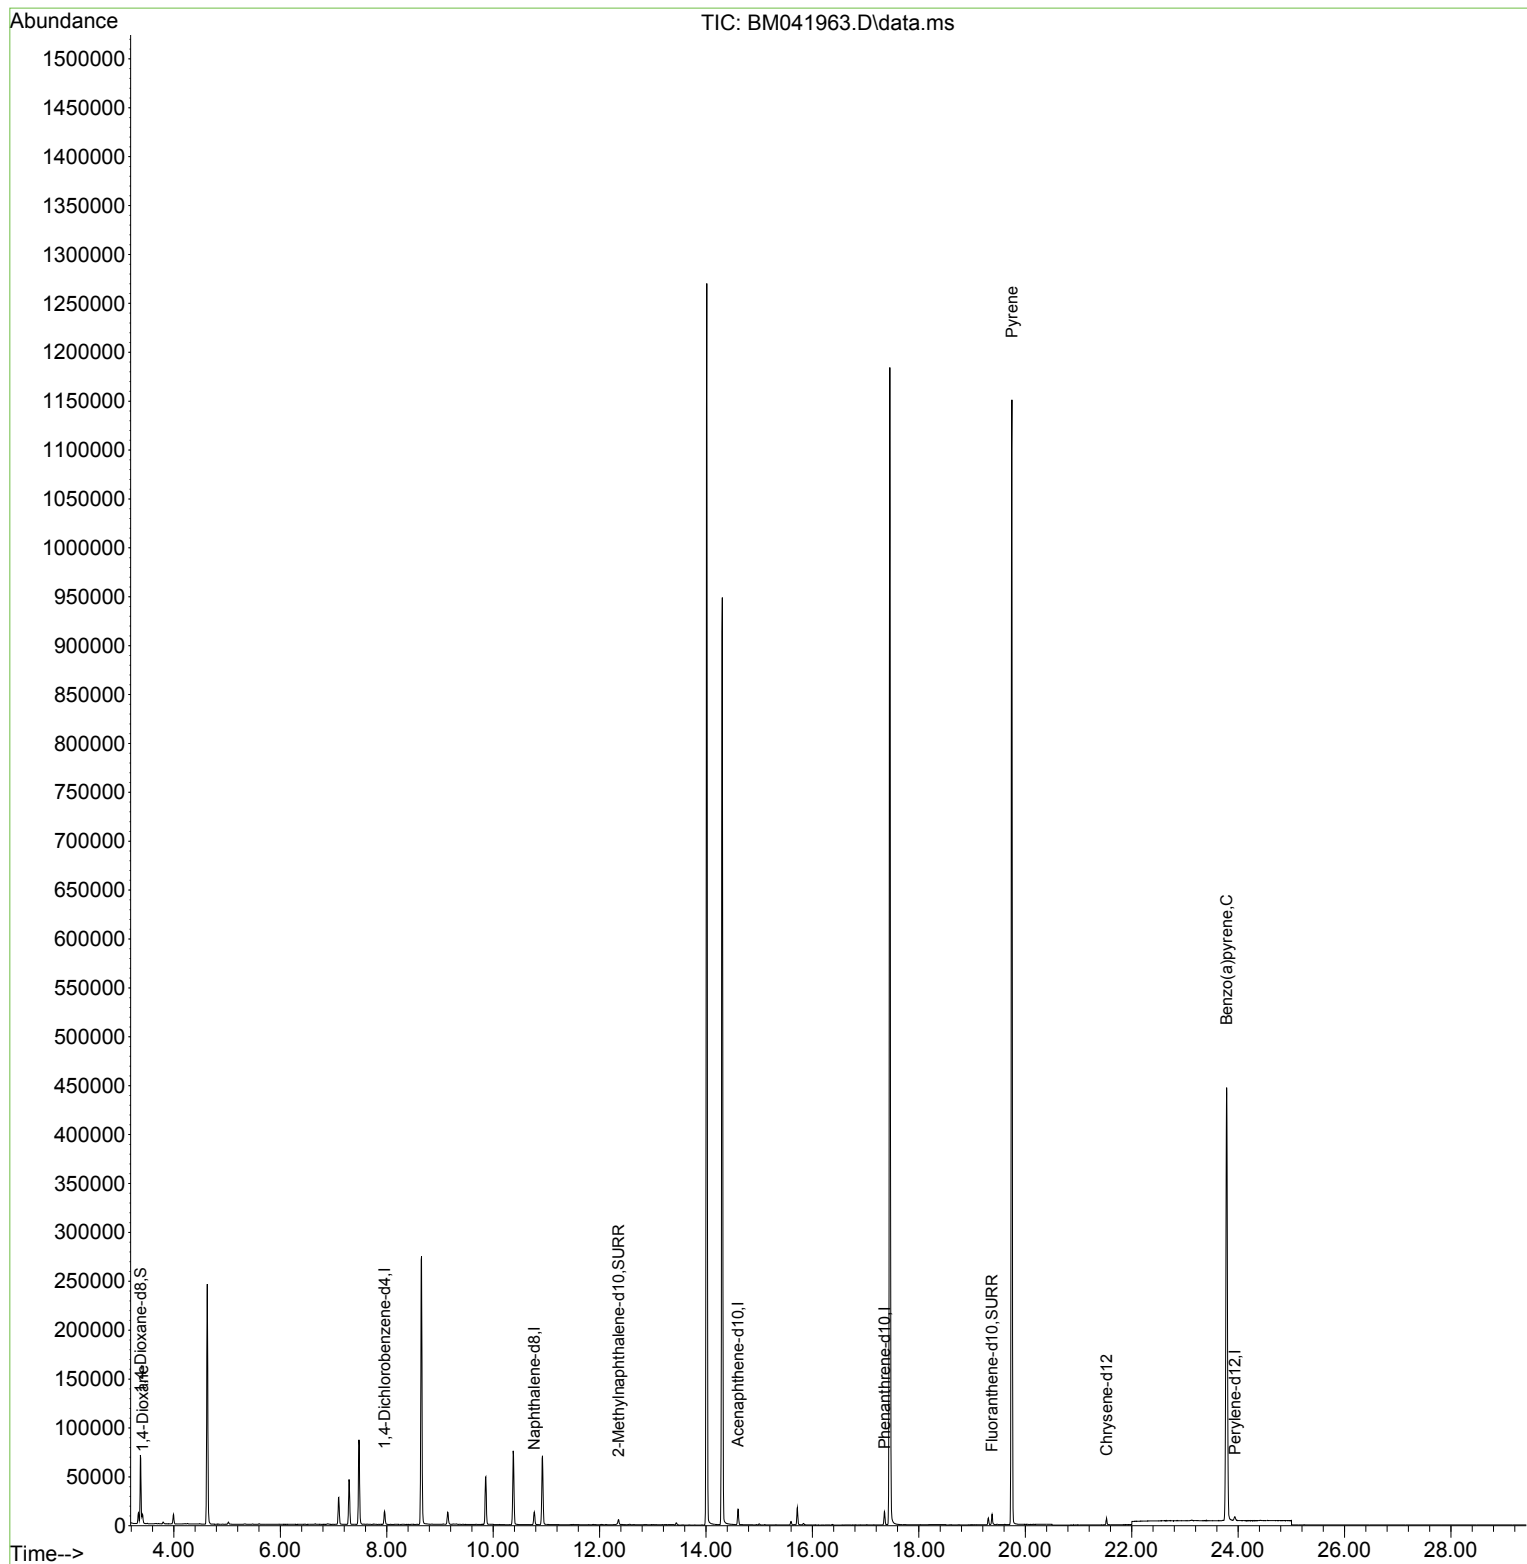


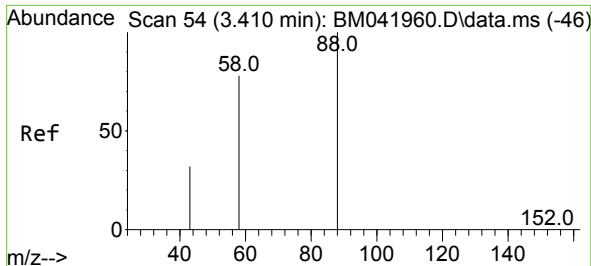

#2
1,4-Dioxane
Concen: 0.637 ng/ul
RT: 3.410 min Scan# 54
Delta R.T. 0.000 min
Lab File: BM041963.D
Acq: 21 Sep 2023 18:45




Instrument :
BNA_M
ClientSampleId :
BBHK8


Tgt Ion: 88 Resp: 5132
Ion Ratio Lower Upper
88 100
43 44.3 51.0 76.4#
58 74.1 56.2 84.4

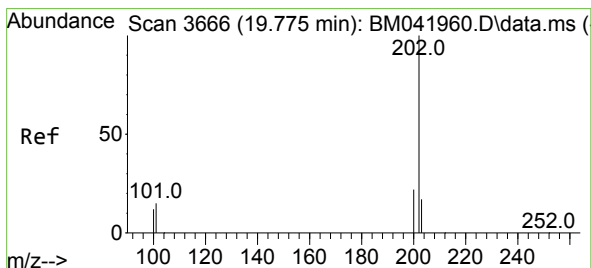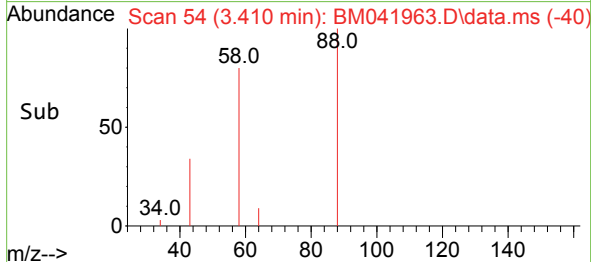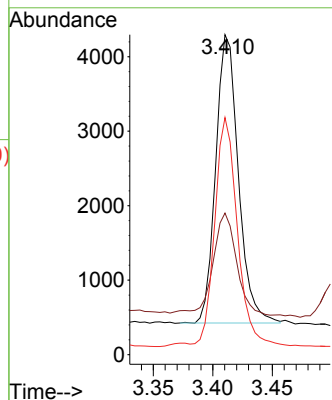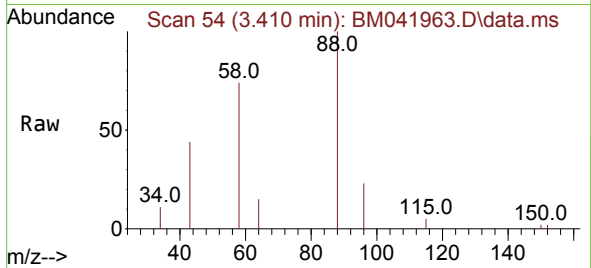

#20
Pyrene
Concen: 0.068 ng/ul
RT: 19.747 min Scan# 3660
Delta R.T. -0.028 min
Lab File: BM041963.D
Acq: 21 Sep 2023 18:45


Tgt Ion: 202 Resp: 2805
Ion Ratio Lower Upper
202 100
101 160.4 11.8 17.6#
100 1146.9 9.3 13.9#

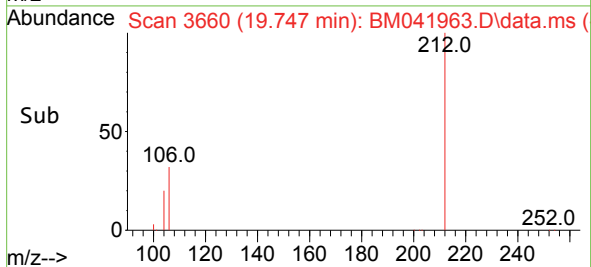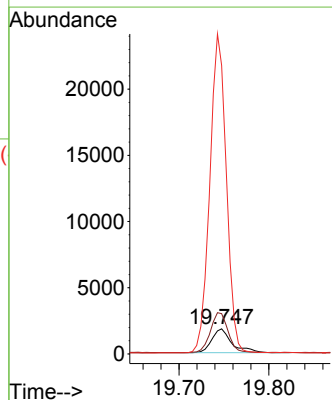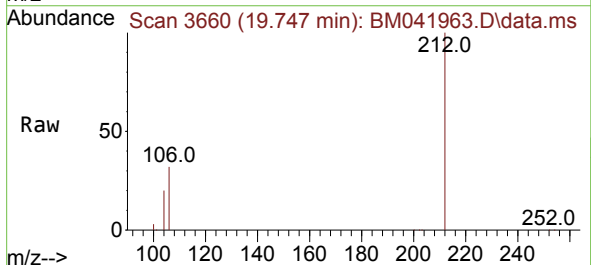

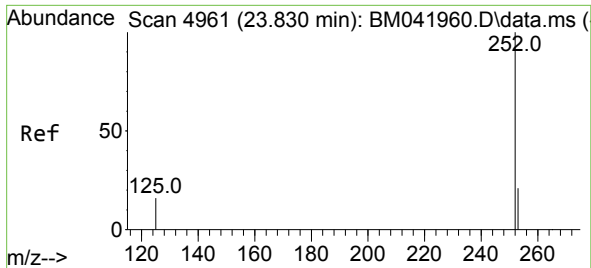

#26
Benzo(a)pyrene
Concen: 0.137 ng/ul
RT: 23.784 min Scan# 4945
Delta R.T. -0.047 min
Lab File: BM041963.D
Acq: 21 Sep 2023 18:45

Instrument :
BNA_M
ClientSampleId :
BBHK8

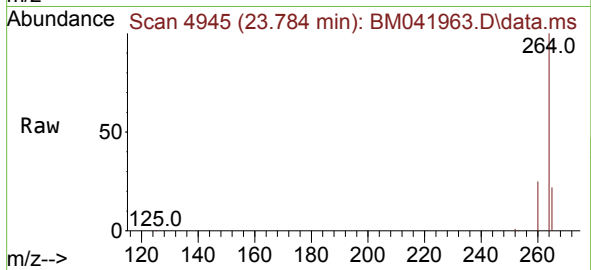

Tgt Ion:252 Resp: 3779
Ion Ratio Lower Upper
252 100
253 51.3 23.0 34.4#
125 50.9 19.9 29.9#

