

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041965.D
 Acq On : 21 Sep 2023 19:59
 Operator : MA/JU
 Sample : 04344-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHL6

Quant Time: Sep 22 03:26:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	7084	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	17946	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	9108	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	16154	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.527	240	5798	0.400	ng/ul	# 0.00
23) Perylene-d12	23.936	264	5991	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	38632	4.654	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	7217	0.293	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	10677	0.499	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.747	202	3105	0.068	ng/ul#	1
26) Benzo(a)pyrene	23.781	252	3917	0.137	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041965.D
Acq On : 21 Sep 2023 19:59
Operator : MA/JU
Sample : 04344-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHL6

Quant Time: Sep 22 03:26:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:25:00 2023
Response via : Initial Calibration




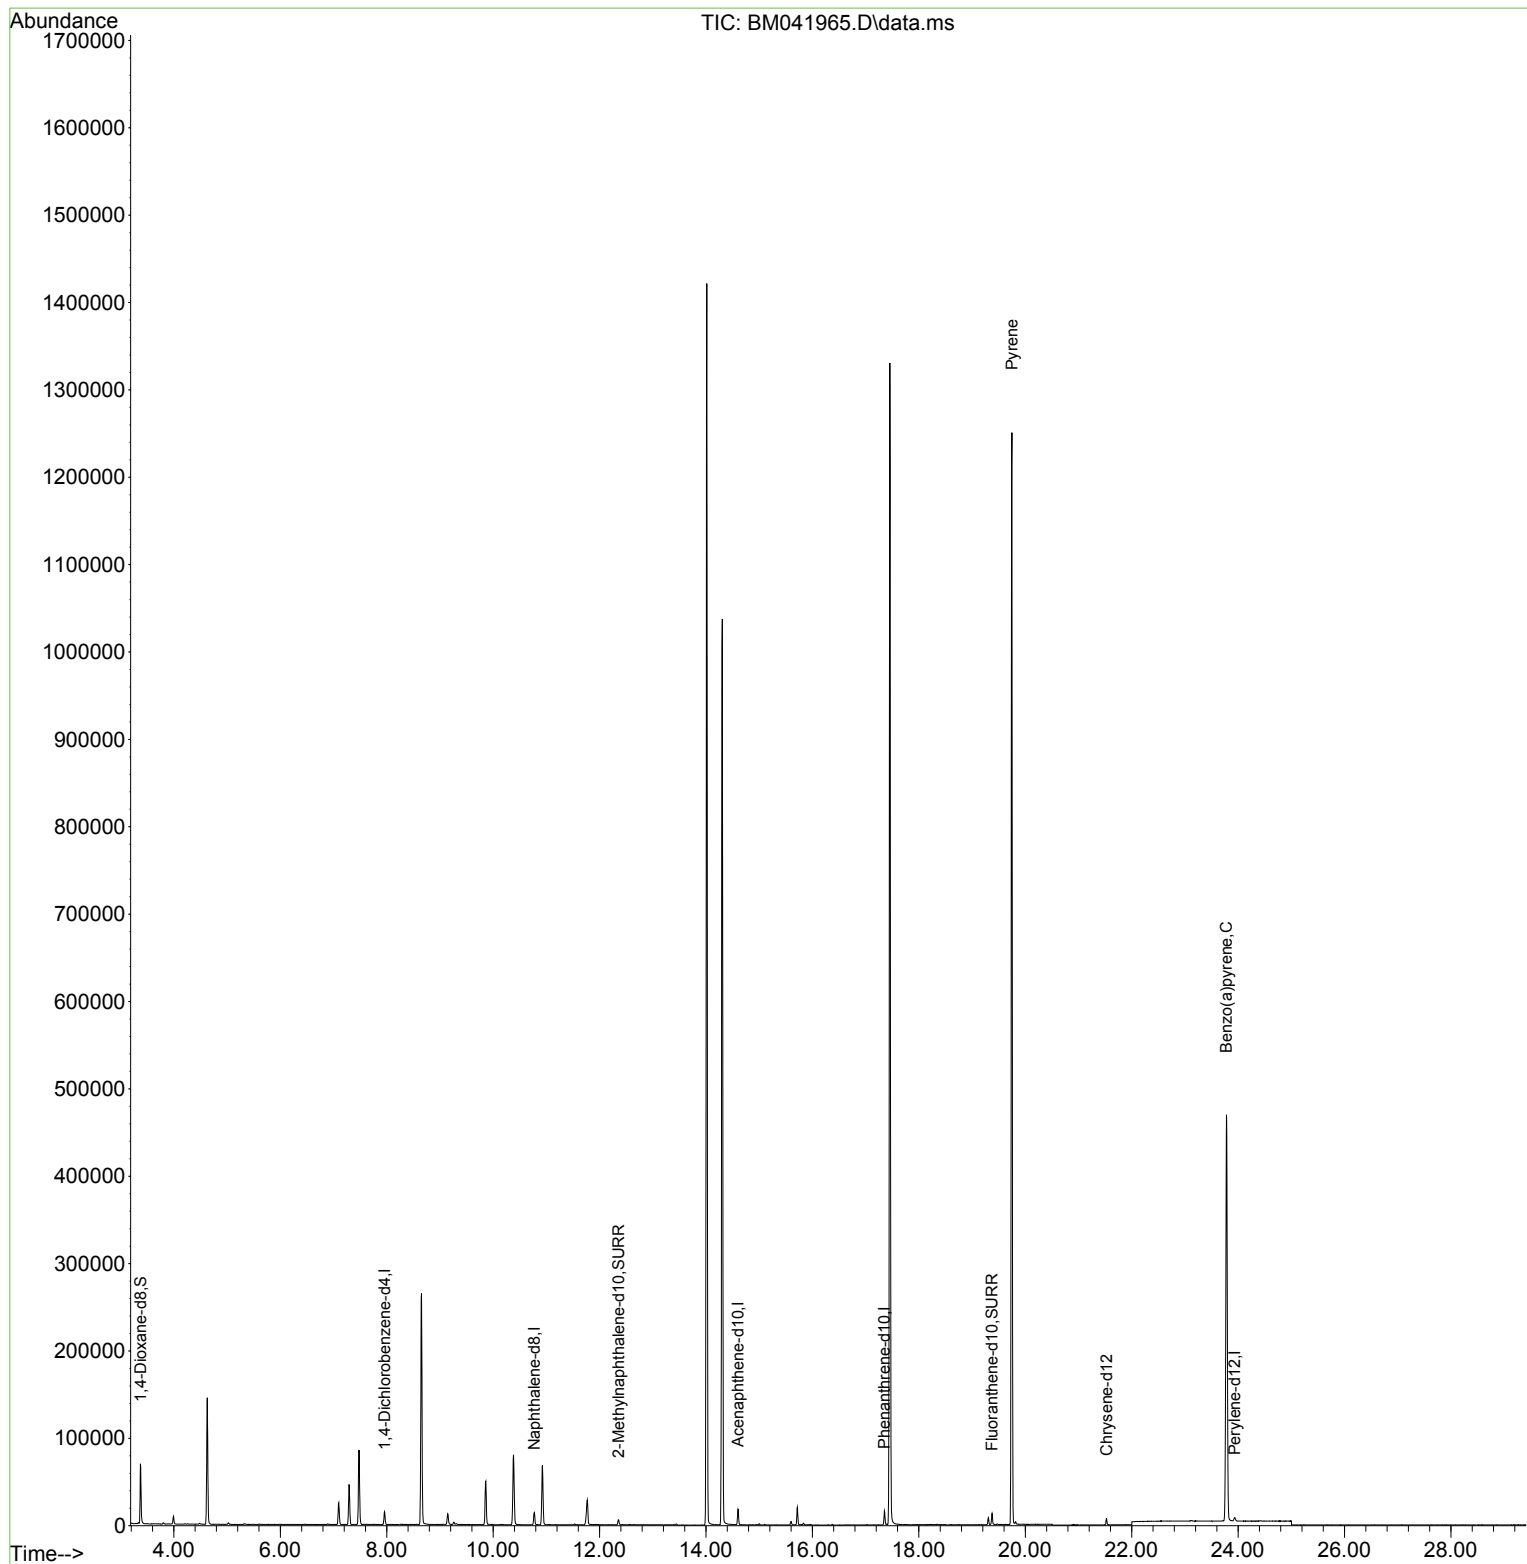


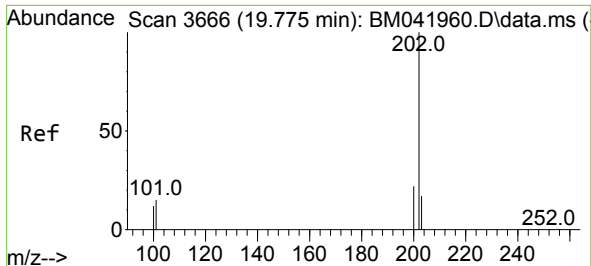

#20
Pyrene
Concen: 0.068 ng/ul
RT: 19.747 min Scan# 3105
Delta R.T. -0.028 min
Lab File: BM041965.D
Acq: 21 Sep 2023 19:59

Instrument :
BNA_M
ClientSampleId :
BBHL6

Tgt Ion:202 Resp: 3105
Ion Ratio Lower Upper
202 100
101 162.5 11.8 17.6#
100 1170.8 9.3 13.9#

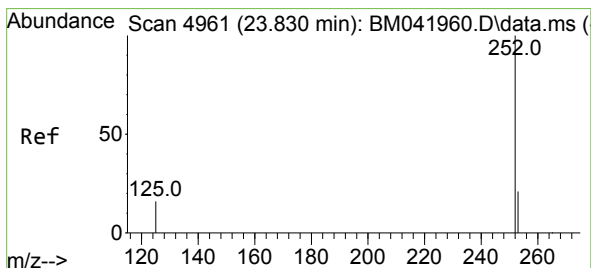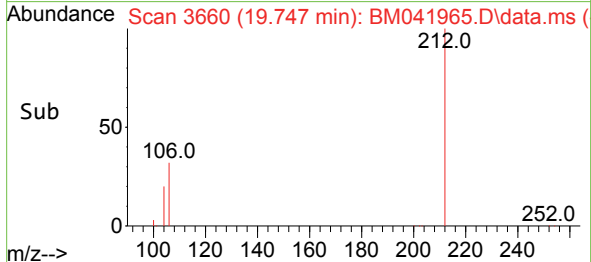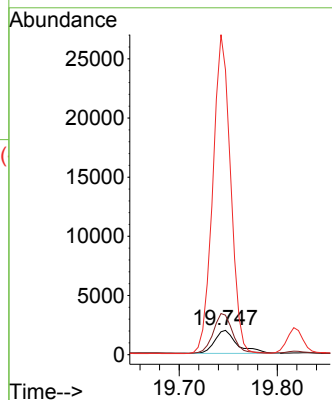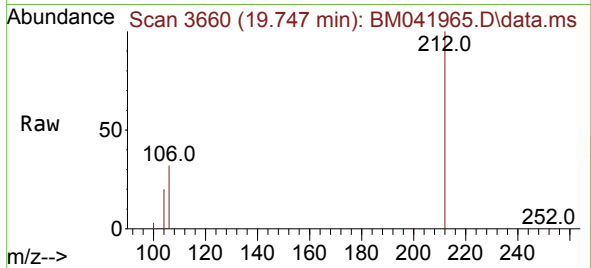

#26
Benzo(a)pyrene
Concen: 0.137 ng/ul
RT: 23.781 min Scan# 4944
Delta R.T. -0.050 min
Lab File: BM041965.D
Acq: 21 Sep 2023 19:59

Tgt Ion:252 Resp: 3917
Ion Ratio Lower Upper
252 100
253 52.2 23.0 34.4#
125 51.0 19.9 29.9#

