

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041954.D
 Acq On : 21 Sep 2023 13:15
 Operator : MA/JU
 Sample : 04378-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJG5

Quant Time: Sep 21 13:55:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 03:49:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	5068	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.774	136	12131	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.606	164	5964	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	11746	0.400	ng/ul	#-0.02
17) Chrysene-d12	21.530	240	6004	0.400	ng/ul	#-0.01
23) Perylene-d12	23.941	264	6717	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	25881	4.358	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	5632	0.339	ng/ul	-0.01
18) Fluoranthene-d10	19.380	212	10658	0.481	ng/ul	0.00
Target Compounds				Qvalue		
2) 1,4-Dioxane	3.410	88	409	0.066	ng/ul#	58
19) Fluoranthene	19.408	202	1879	0.042	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041954.D
Acq On : 21 Sep 2023 13:15
Operator : MA/JU
Sample : 04378-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJG5

Quant Time: Sep 21 13:55:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 03:49:33 2023
Response via : Initial Calibration




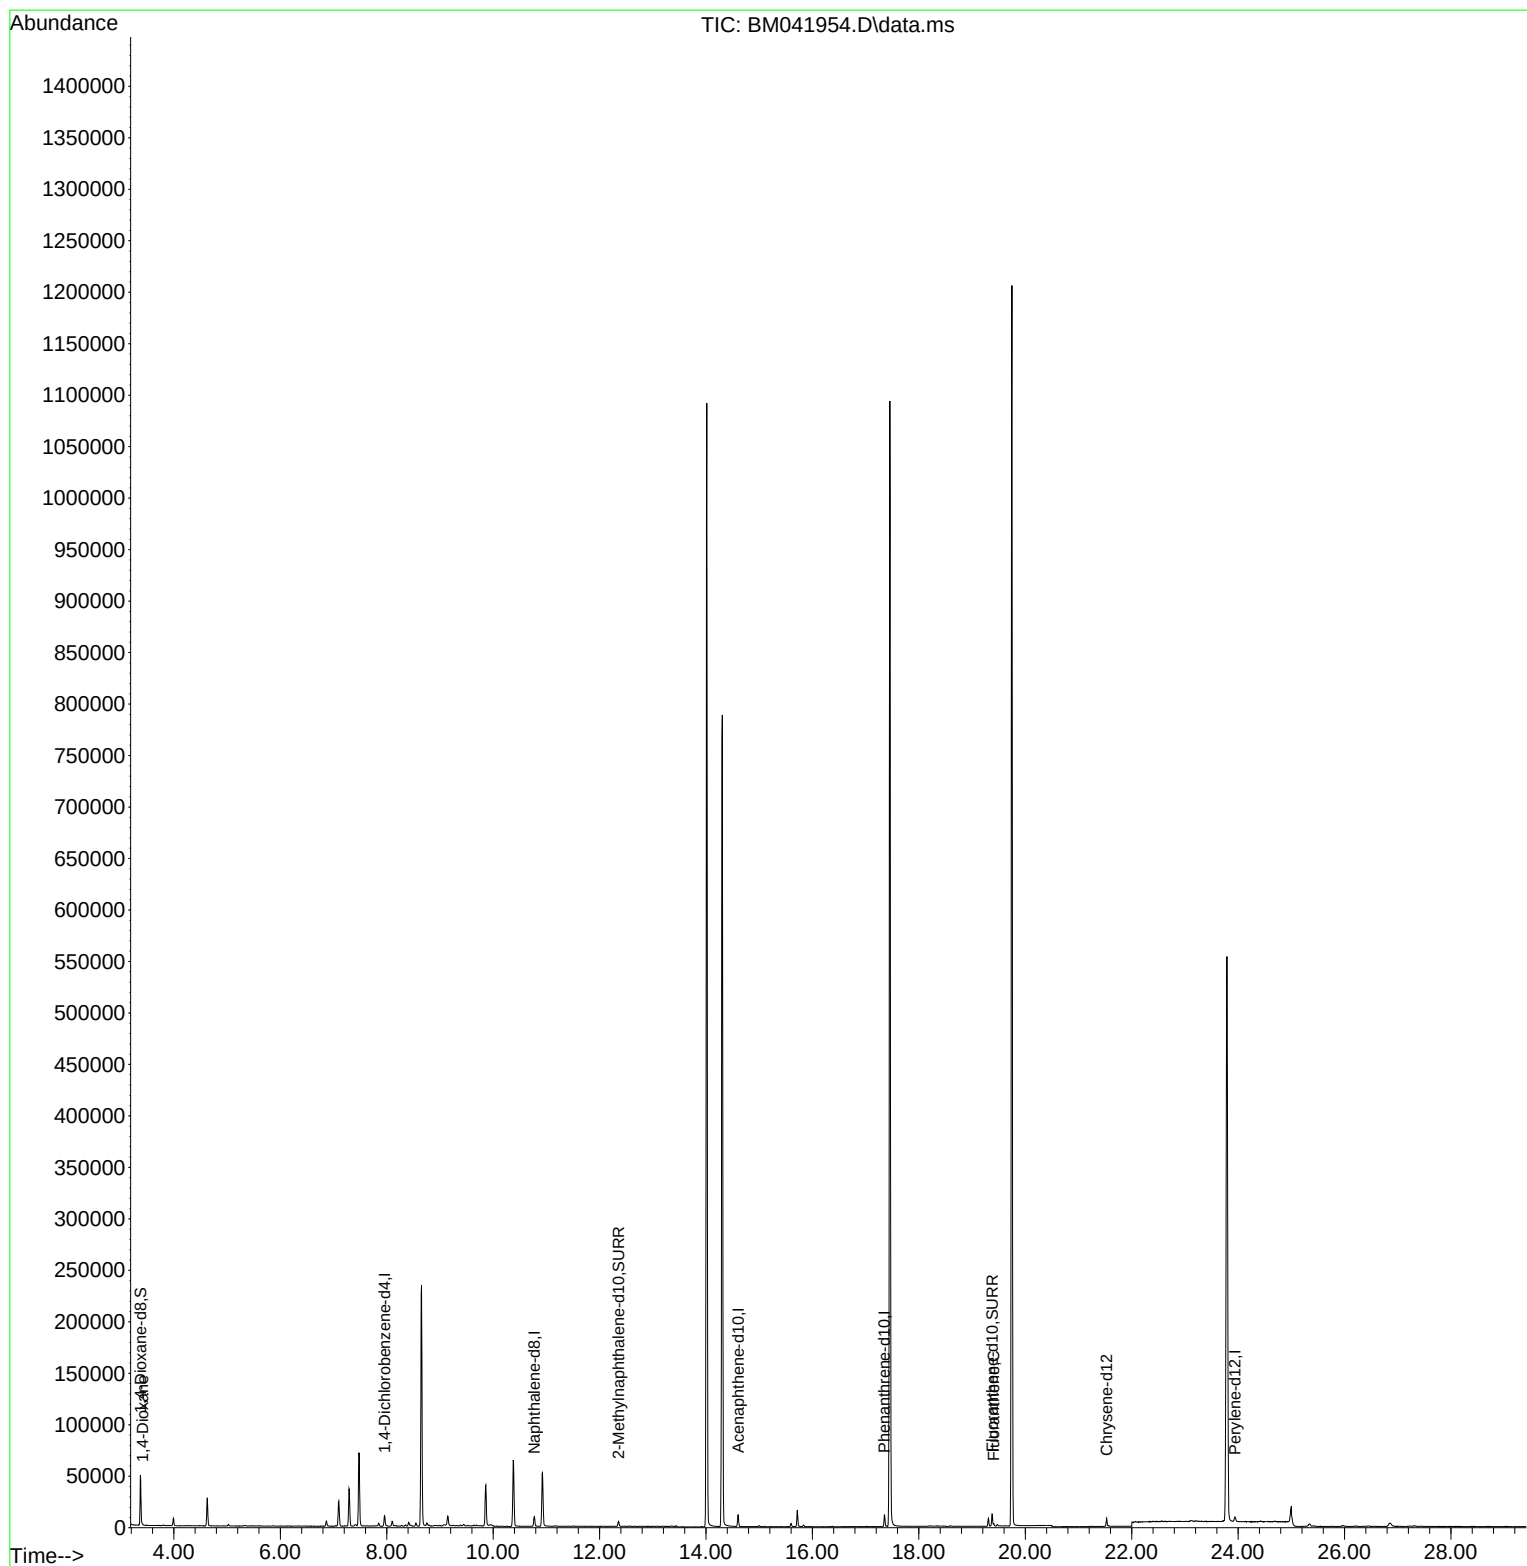


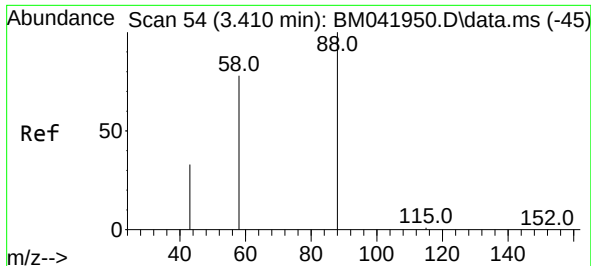

#2
1,4-Dioxane
Concen: 0.066 ng/ul
RT: 3.410 min Scan# 54
Delta R.T. -0.008 min
Lab File: BM041954.D
Acq: 21 Sep 2023 13:15

Instrument :
BNA_M
ClientSampleId :
BBJG5

Tgt Ion: 88 Resp: 409
Ion Ratio Lower Upper
88 100
43 104.5 51.0 76.4#
58 43.4 56.2 84.4#

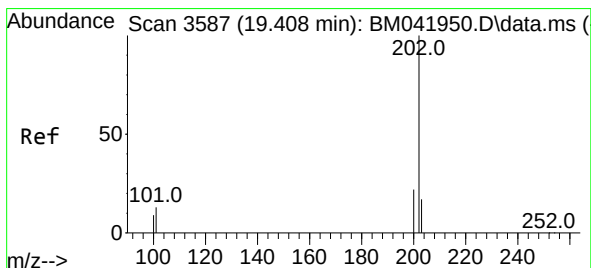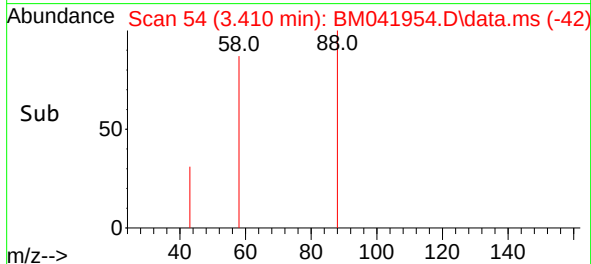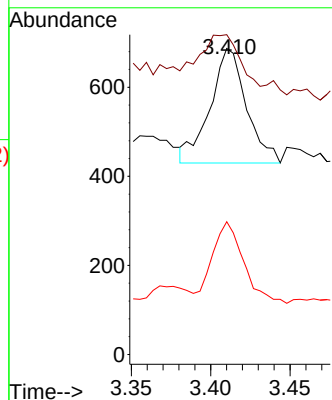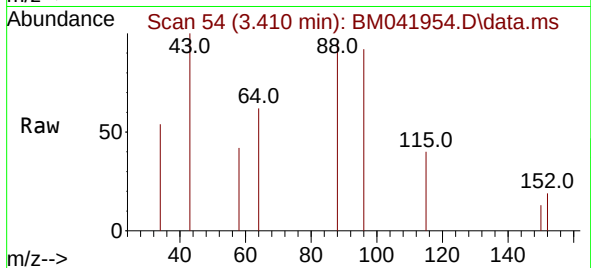

#19
Fluoranthene
Concen: 0.042 ng/ul
RT: 19.408 min Scan# 3587
Delta R.T. -0.014 min
Lab File: BM041954.D
Acq: 21 Sep 2023 13:15

Tgt Ion: 202 Resp: 1879
Ion Ratio Lower Upper
202 100
101 21.9 10.1 15.1#
100 17.0 7.5 11.3#

