

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041959.D
 Acq On : 21 Sep 2023 16:18
 Operator : MA/JU
 Sample : 04344-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHX3

Quant Time: Sep 21 16:47:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 16 03:49:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6497	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.774	136	16561	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.606	164	8613	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.358	188	15379	0.400	ng/ul	-0.01
17) Chrysene-d12	21.527	240	5935	0.400	ng/ul	#-0.01
23) Perylene-d12	23.936	264	6214	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	42204	5.543	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	8230	0.363	ng/ul	-0.01
18) Fluoranthene-d10	19.375	212	12828	0.586	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.410	88	22593	2.854	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041959.D
Acq On : 21 Sep 2023 16:18
Operator : MA/JU
Sample : 04344-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHX3


Quant Time: Sep 21 16:47:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 16 03:49:33 2023
Response via : Initial Calibration

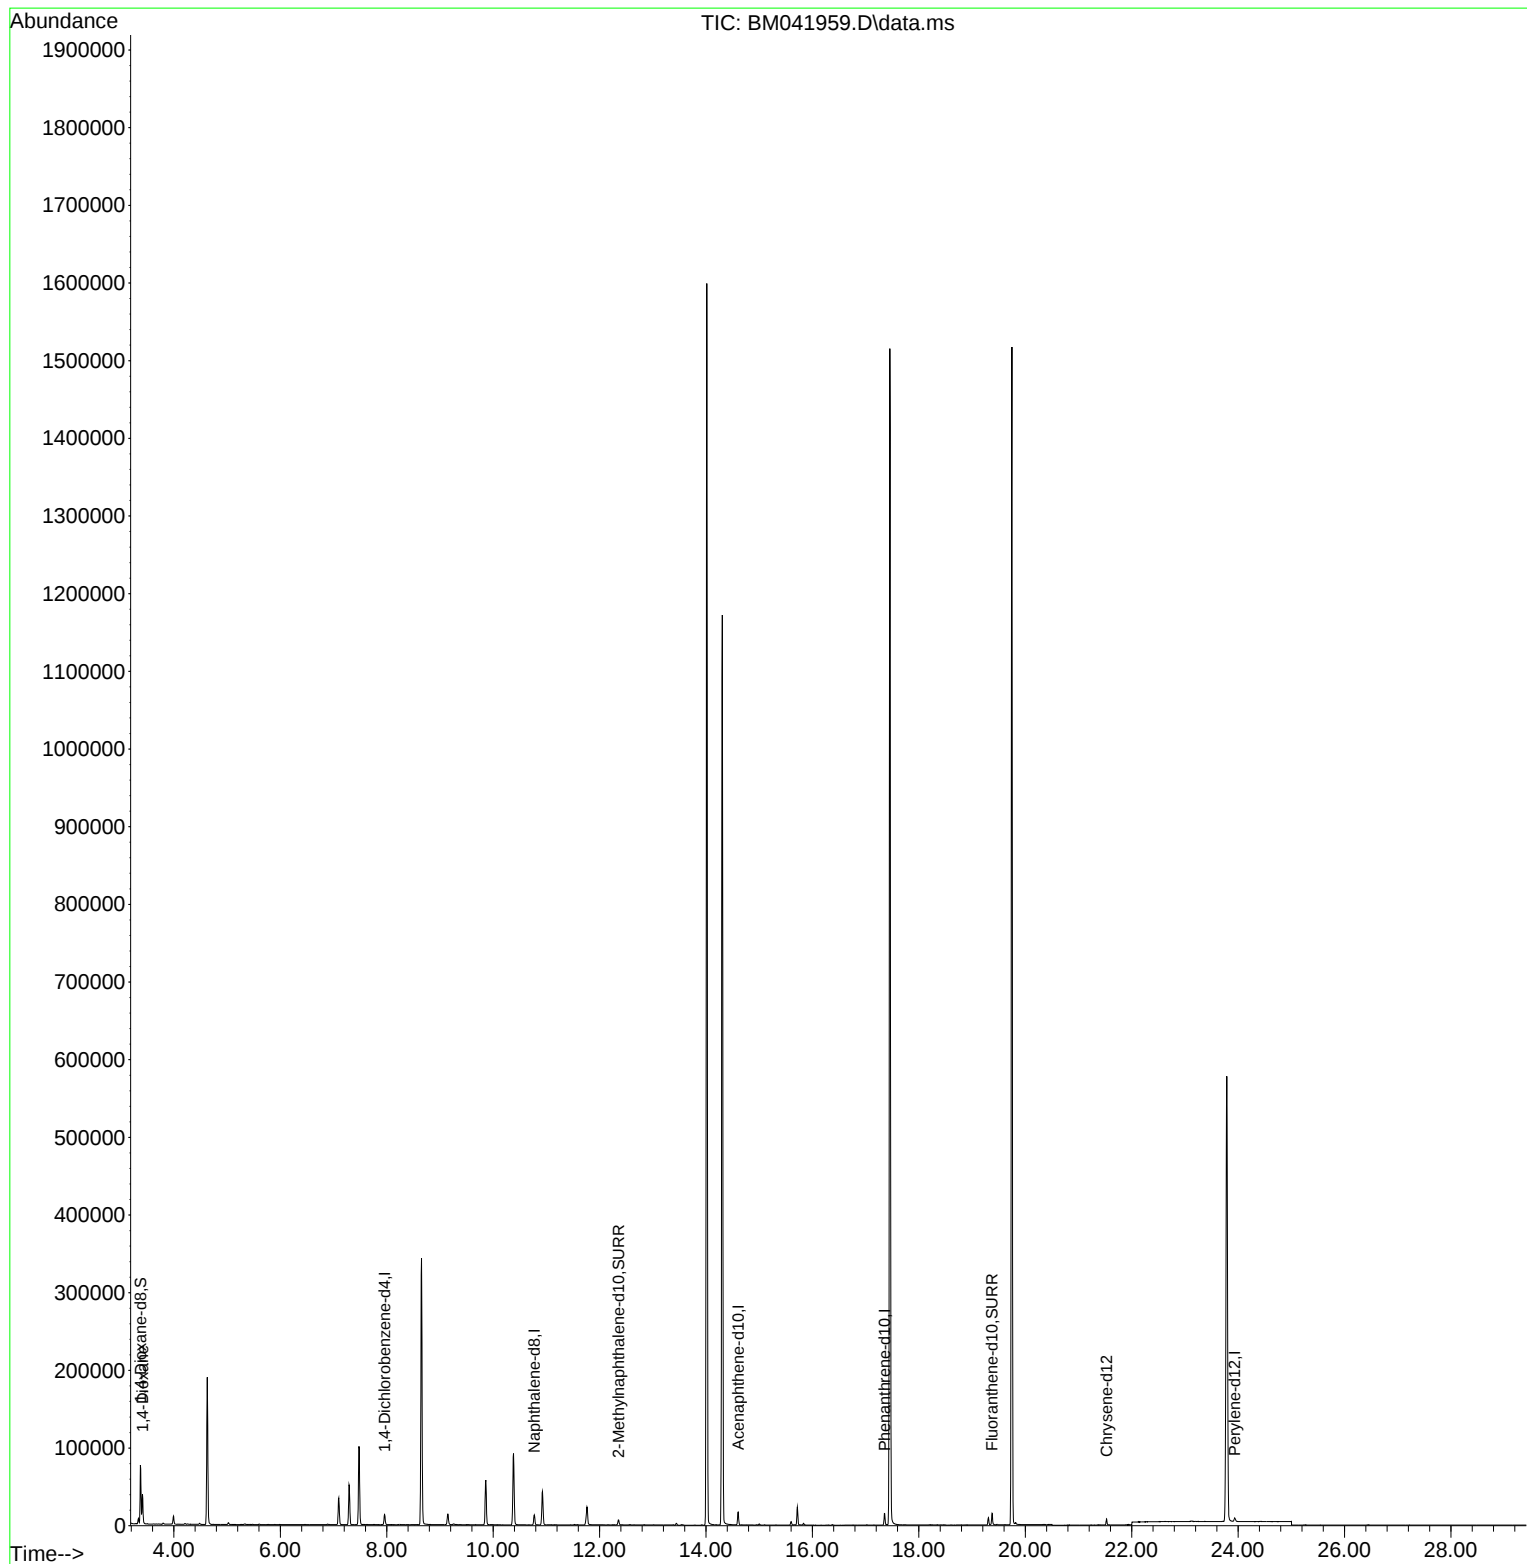

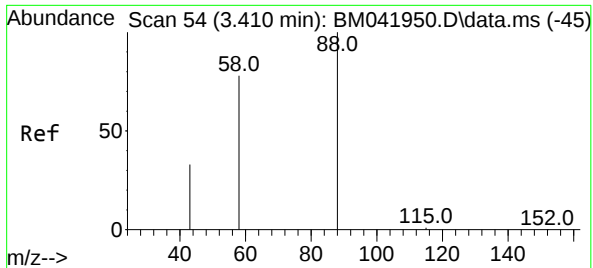

#2
 1,4-Dioxane
 Concen: 2.854 ng/ul
 RT: 3.410 min Scan# 54
 Delta R.T. -0.008 min
 Lab File: BM041959.D
 Acq: 21 Sep 2023 16:18

Instrument :
 BNA_M
 ClientSampleId :
 BBHX3

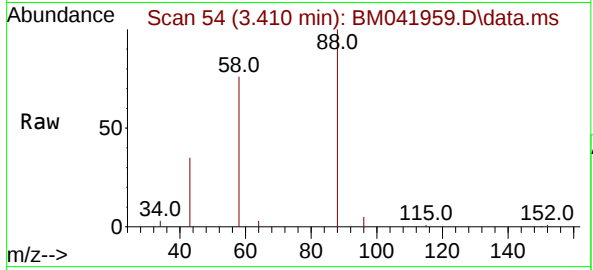

Tgt Ion:	88	Resp:	22593
Ion	Ratio	Lower	Upper
88	100		
43	35.4	51.0	76.4#
58	75.6	56.2	84.4

