

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041964.D
 Acq On : 21 Sep 2023 19:22
 Operator : MA/JU
 Sample : 04344-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBJH3

Quant Time: Sep 22 03:26:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6591	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	15642	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.606	164	7409	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	13516	0.400	ng/ul	0.00
17) Chrysene-d12	21.527	240	6113	0.400	ng/ul	# 0.00
23) Perylene-d12	23.939	264	7025	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.377	96	39497	5.114	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.357	152	6893	0.321	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	10994	0.487	ng/ul	0.00
Target Compounds						
16) Anthracene	17.489	178	3807	0.073	ng/ul#	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041964.D
Acq On : 21 Sep 2023 19:22
Operator : MA/JU
Sample : 04344-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBJH3


Quant Time: Sep 22 03:26:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:25:00 2023
Response via : Initial Calibration

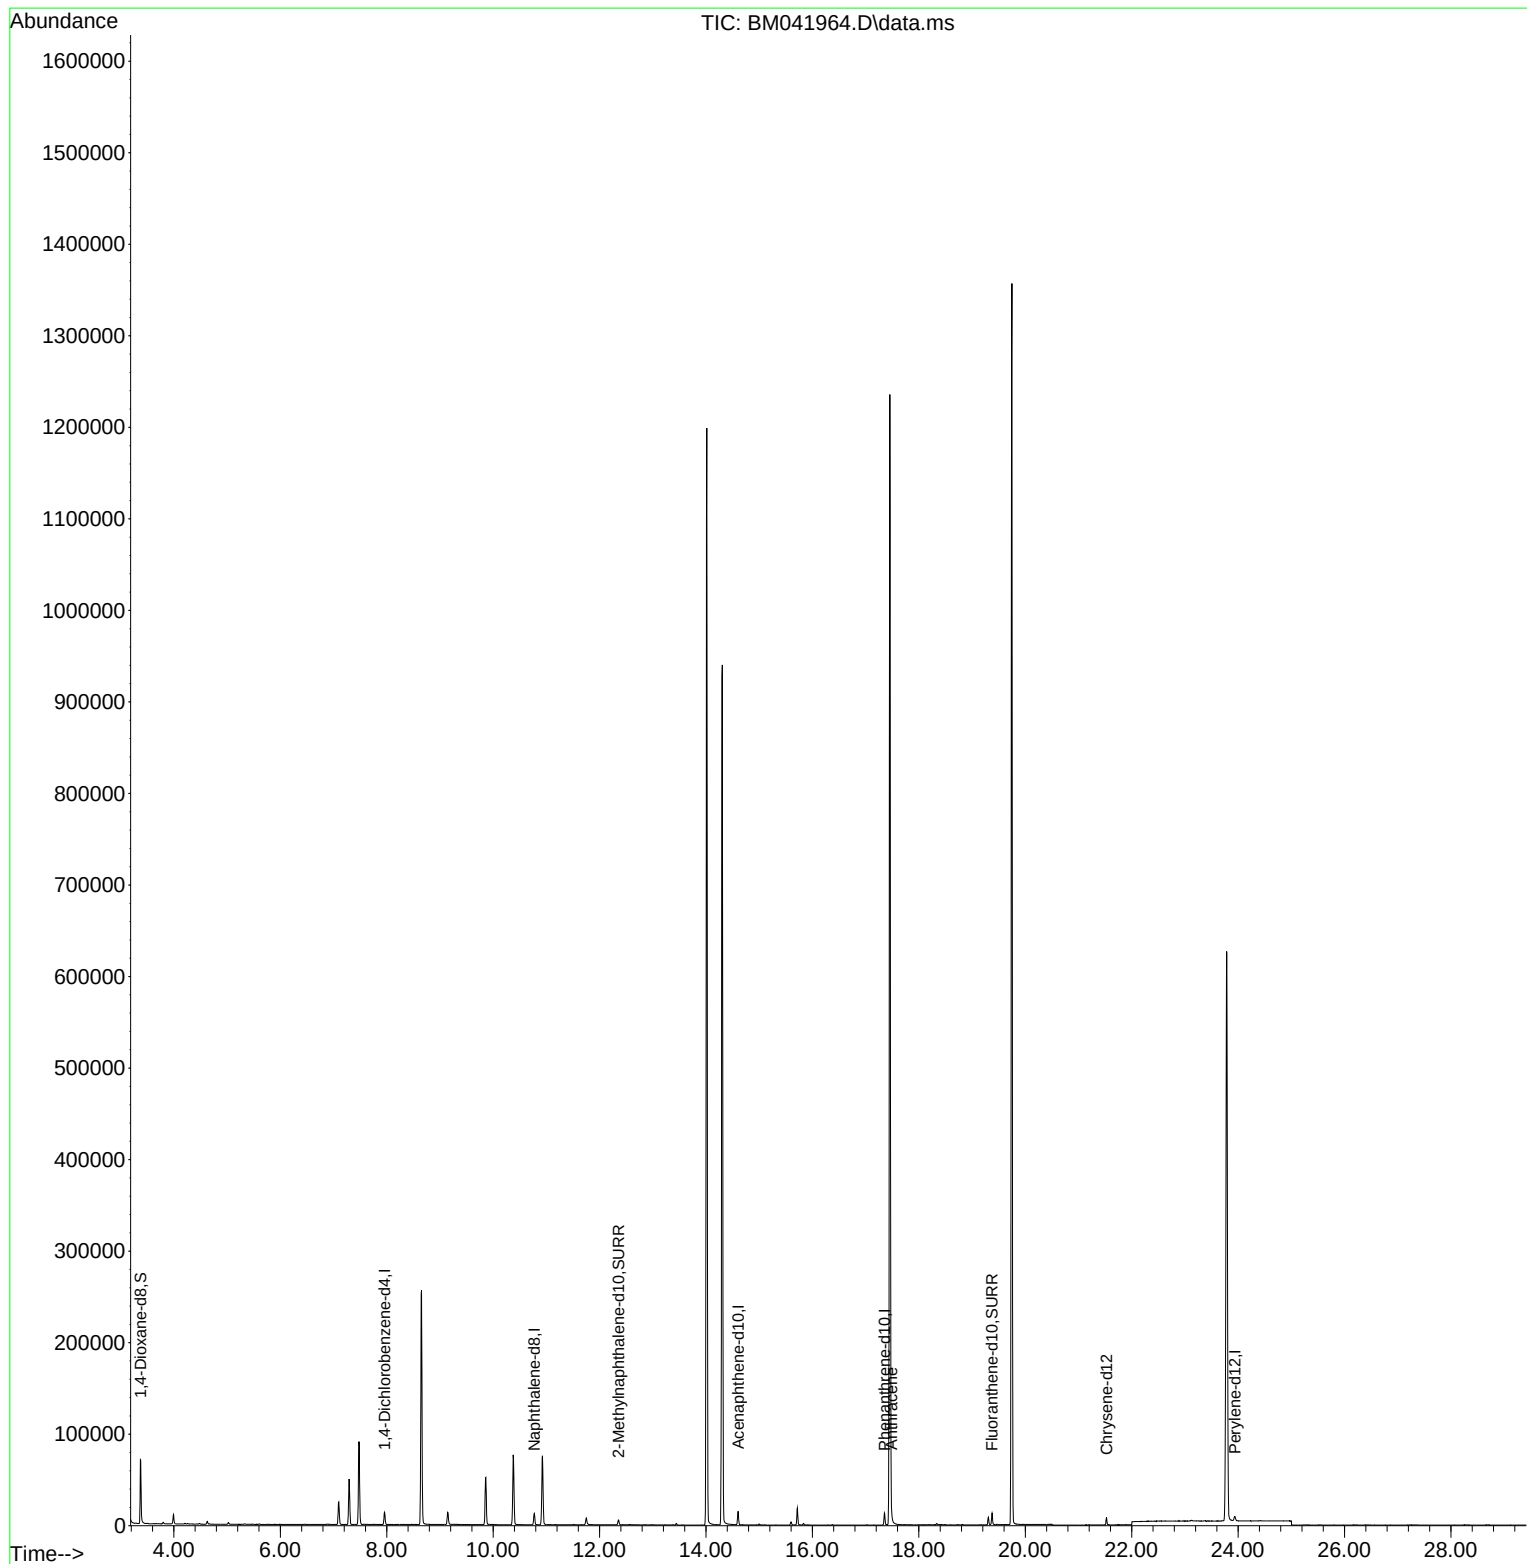

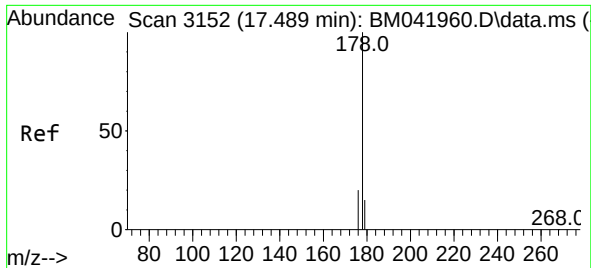

#16
 Anthracene
 Concen: 0.073 ng/ul
 RT: 17.489 min Scan# 3152
 Delta R.T. 0.000 min
 Lab File: BM041964.D
 Acq: 21 Sep 2023 19:22

Instrument :
 BNA_M
 ClientSampleId :
 BBJH3

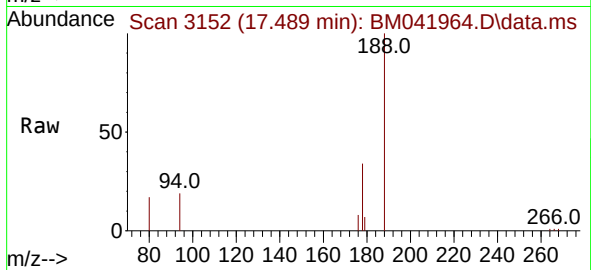

Tgt Ion	Ratio	Lower	Upper
178	100		
179	20.3	12.9	19.3#
176	22.5	16.3	24.5

