

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041968.D
 Acq On : 21 Sep 2023 21:48
 Operator : MA/JU
 Sample : 04344-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHL8

Quant Time: Sep 22 03:27:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	7173	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	17132	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	9174	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	14588	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.527	240	5646	0.400	ng/ul	# 0.00
23) Perylene-d12	23.939	264	5714	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	42424	5.047	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	7018	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	10816	0.519	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Anthracene	17.489	178	5844	0.104	ng/ul#	87
19) Fluoranthene	19.408	202	1842	0.043	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041968.D
Acq On : 21 Sep 2023 21:48
Operator : MA/JU
Sample : 04344-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHL8

Quant Time: Sep 22 03:27:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:25:00 2023
Response via : Initial Calibration




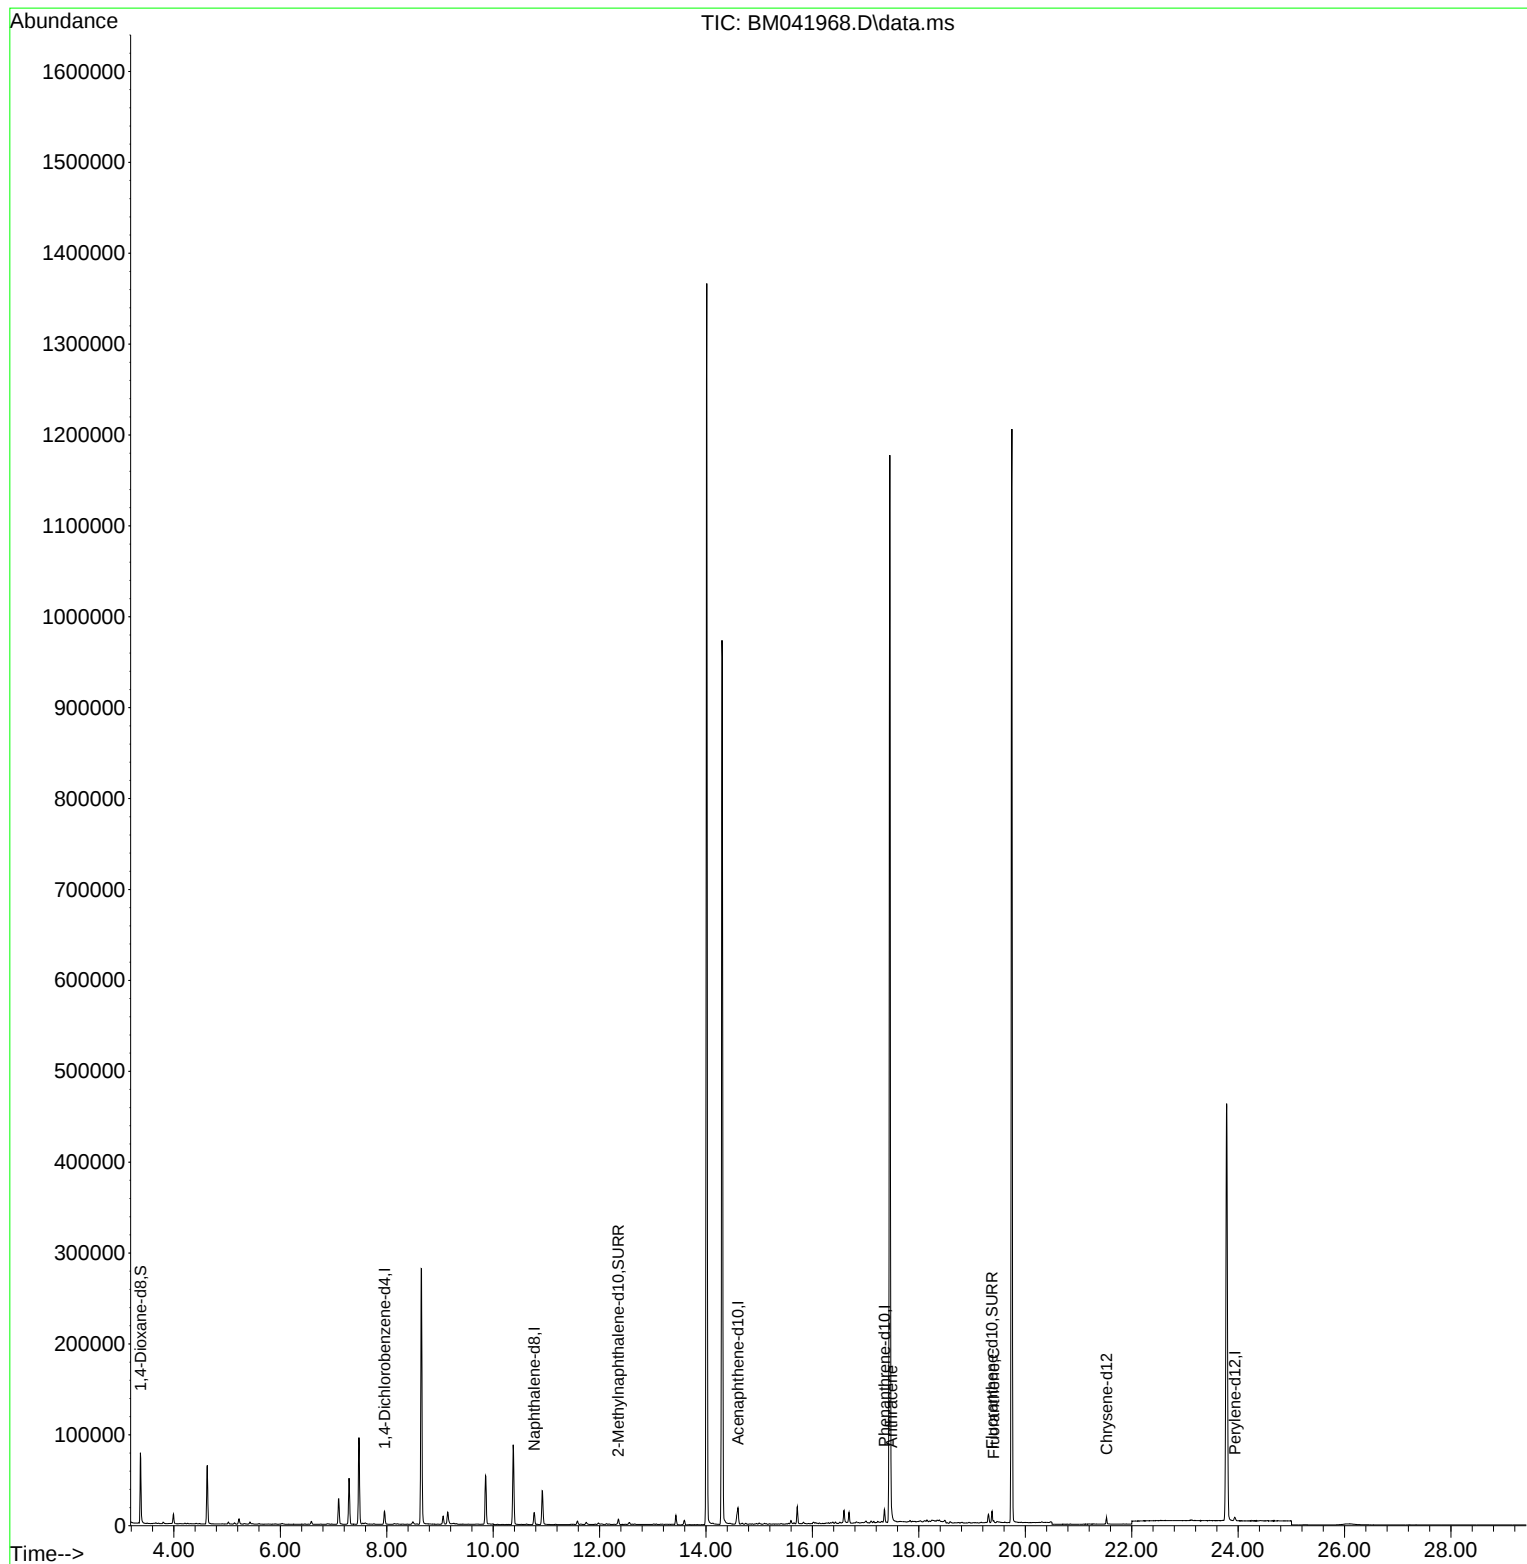


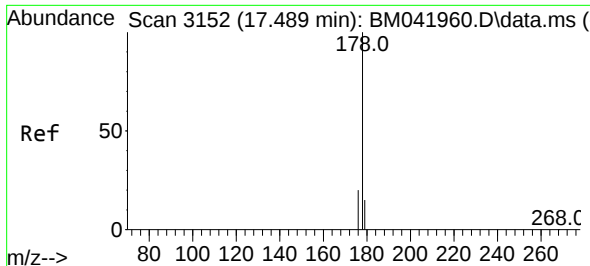

#16
 Anthracene
 Concen: 0.104 ng/ul
 RT: 17.489 min Scan# 3152
 Delta R.T. 0.000 min
 Lab File: BM041968.D
 Acq: 21 Sep 2023 21:48

Instrument :
 BNA_M
 ClientSampleId :
 BBHL8

Tgt Ion:178 Resp: 5844
 Ion Ratio Lower Upper
 178 100
 179 23.9 12.9 19.3#
 176 24.7 16.3 24.5#

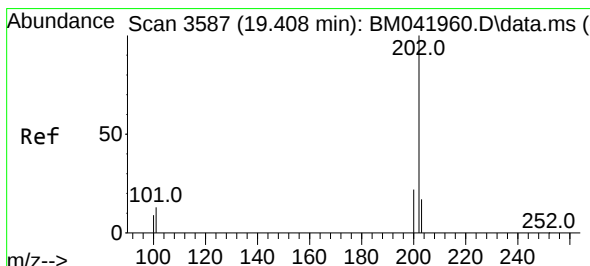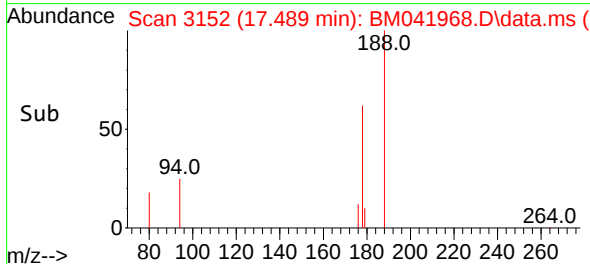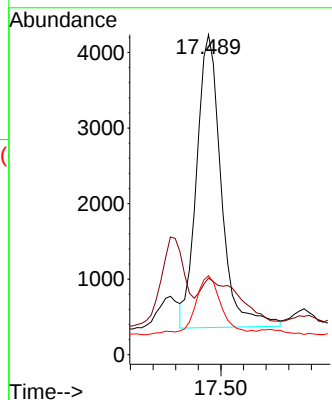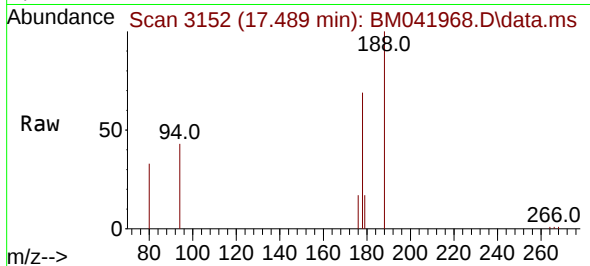

#19
 Fluoranthene
 Concen: 0.043 ng/ul
 RT: 19.408 min Scan# 3587
 Delta R.T. 0.000 min
 Lab File: BM041968.D
 Acq: 21 Sep 2023 21:48

Tgt Ion:202 Resp: 1842
 Ion Ratio Lower Upper
 202 100
 101 27.0 10.1 15.1#
 100 19.3 7.5 11.3#

