

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041969.D
 Acq On : 21 Sep 2023 22:25
 Operator : MA/JU
 Sample : 04344-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHAU9

Quant Time: Sep 22 03:27:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6956	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	16291	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	8263	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	13386	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.527	240	5718	0.400	ng/ul	# 0.00
23) Perylene-d12	23.936	264	5874	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	35277	4.328	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	6369	0.285	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	9676	0.458	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Anthracene	17.489	178	6053	0.117	ng/ul#	88
19) Fluoranthene	19.408	202	2445	0.057	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041969.D
Acq On : 21 Sep 2023 22:25
Operator : MA/JU
Sample : 04344-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHAU9

Quant Time: Sep 22 03:27:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:25:00 2023
Response via : Initial Calibration




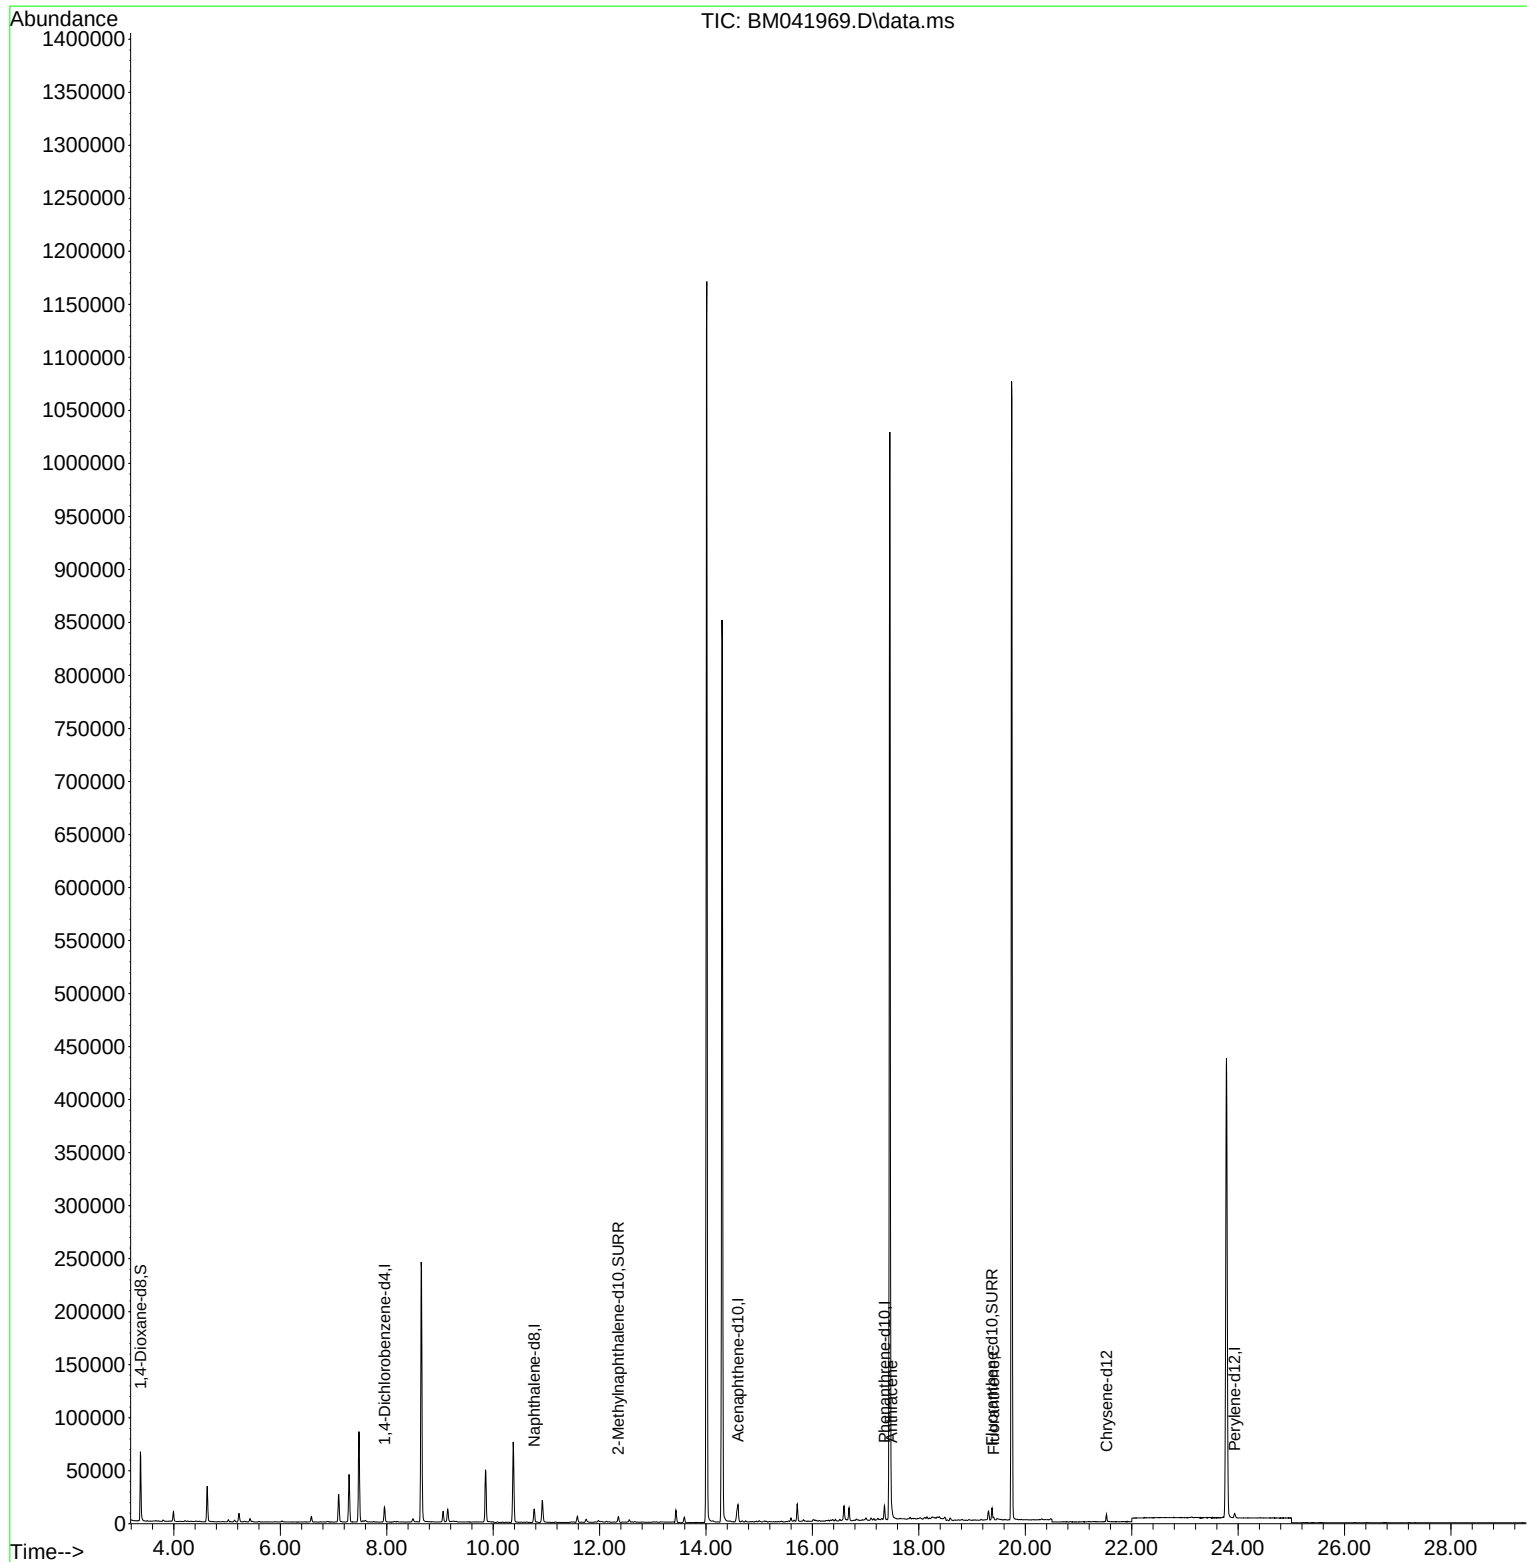


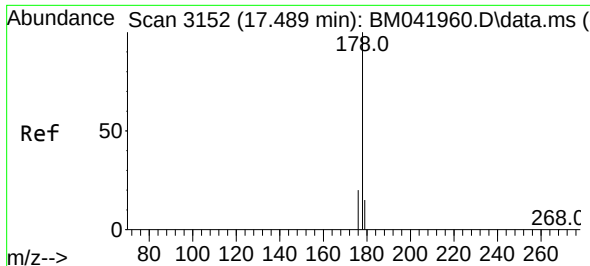

#16
 Anthracene
 Concen: 0.117 ng/ul
 RT: 17.489 min Scan# 3152
 Delta R.T. 0.000 min
 Lab File: BM041969.D
 Acq: 21 Sep 2023 22:25

Instrument :
 BNA_M
 ClientSampleId :
 BHAU9

Tgt Ion:178 Resp: 6053
 Ion Ratio Lower Upper
 178 100
 179 23.0 12.9 19.3#
 176 24.8 16.3 24.5#

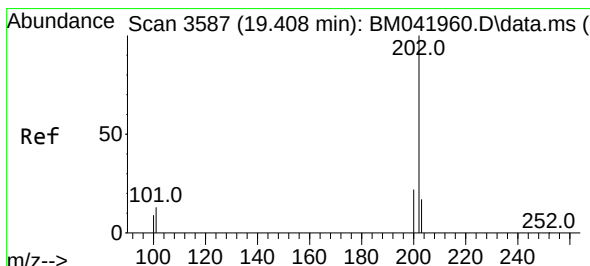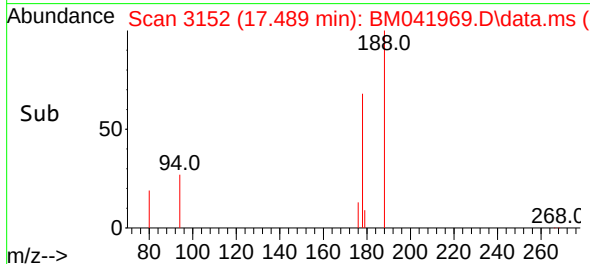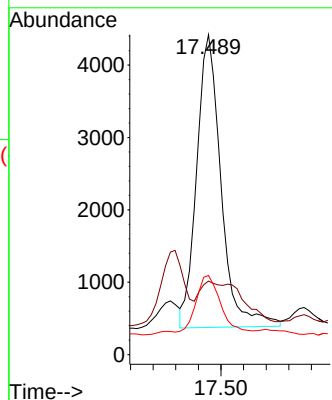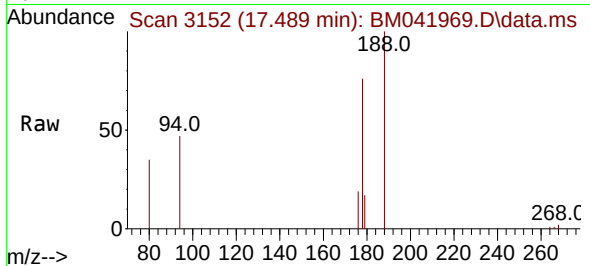

#19
 Fluoranthene
 Concen: 0.057 ng/ul
 RT: 19.408 min Scan# 3587
 Delta R.T. 0.000 min
 Lab File: BM041969.D
 Acq: 21 Sep 2023 22:25

Tgt Ion:202 Resp: 2445
 Ion Ratio Lower Upper
 202 100
 101 26.1 10.1 15.1#
 100 18.4 7.5 11.3#

