

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
 Data File : BM041970.D
 Acq On : 21 Sep 2023 23:01
 Operator : MA/JU
 Sample : 04344-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHR8

Quant Time: Sep 22 03:27:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 03:25:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.958	152	6696	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	16914	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	8782	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.354	188	16185	0.400	ng/ul	0.00
17) Chrysene-d12	21.524	240	5815	0.400	ng/ul	# 0.00
23) Perylene-d12	23.933	264	5808	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	37820	4.820	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	6956	0.300	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	11110	0.518	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.410	88	4758	0.583	ng/ul#	87
14) Pentachlorophenol	16.978	266	5126	0.533	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092123\
Data File : BM041970.D
Acq On : 21 Sep 2023 23:01
Operator : MA/JU
Sample : 04344-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHR8

Quant Time: Sep 22 03:27:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM091523.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 03:25:00 2023
Response via : Initial Calibration




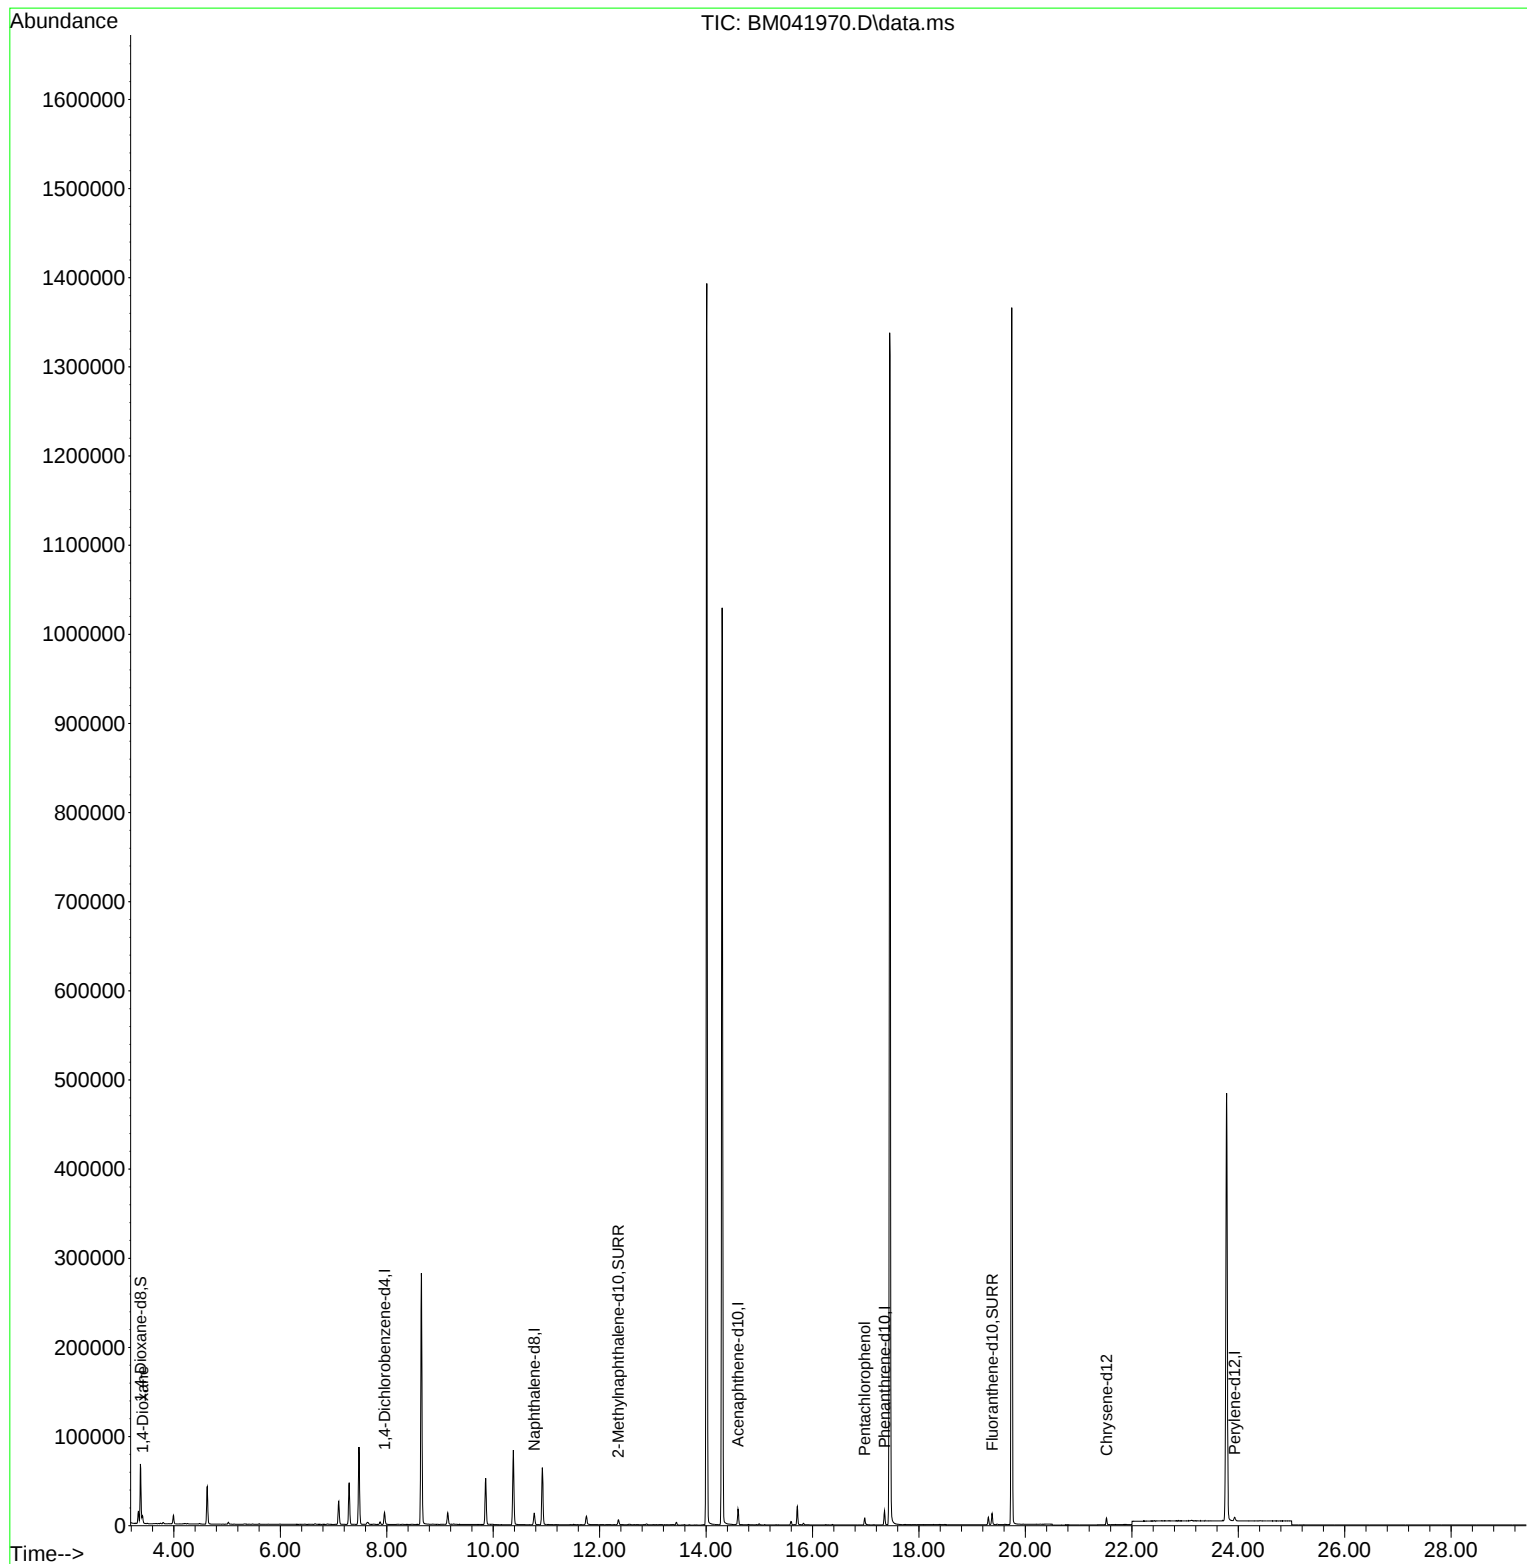


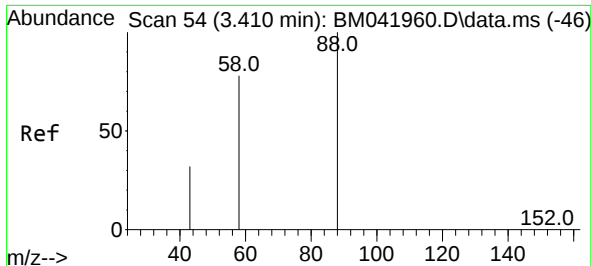

#2
 1,4-Dioxane
 Concen: 0.583 ng/ul
 RT: 3.410 min Scan# 54
 Delta R.T. 0.000 min
 Lab File: BM041970.D
 Acq: 21 Sep 2023 23:01

Instrument :
 BNA_M
 ClientSampleId :
 BBHR8

Tgt Ion: 88 Resp: 4758
 Ion Ratio Lower Upper
 88 100
 43 44.5 51.0 76.4#
 58 71.7 56.2 84.4

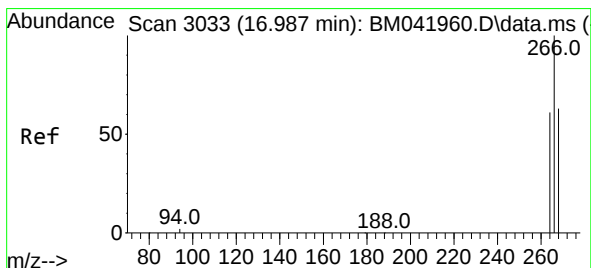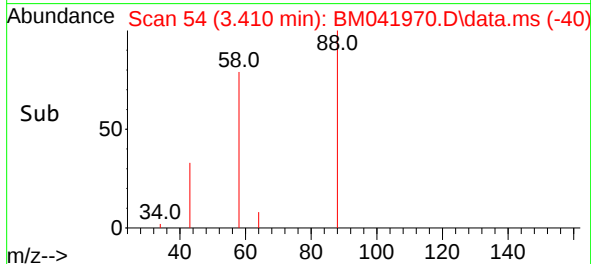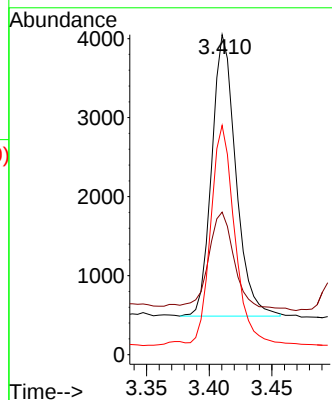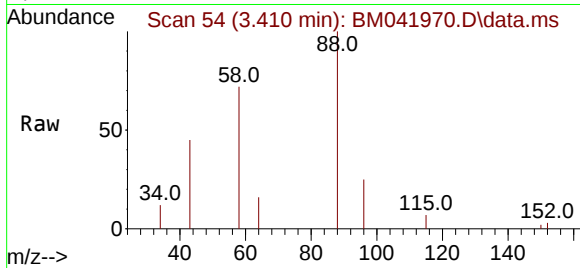

#14
 Pentachlorophenol
 Concen: 0.533 ng/ul
 RT: 16.978 min Scan# 3031
 Delta R.T. -0.008 min
 Lab File: BM041970.D
 Acq: 21 Sep 2023 23:01

Tgt Ion: 266 Resp: 5126
 Ion Ratio Lower Upper
 266 100
 264 62.5 49.8 74.8
 268 63.8 51.3 76.9

