

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM041999.D
 Acq On : 22 Sep 2023 22:29
 Operator : MA/JU
 Sample : 04386-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF0

Quant Time: Sep 23 02:40:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	5218	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	13004	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	6115	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	11520	0.400	ng/ul	0.00
17) Chrysene-d12	21.524	240	4519	0.400	ng/ul	0.00
23) Perylene-d12	23.933	264	4574	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	30946	4.352	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	3543	0.218	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	4600	0.247	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.775	252	2419	0.084	ng/ul#	Qvalue 35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
Data File : BM041999.D
Acq On : 22 Sep 2023 22:29
Operator : MA/JU
Sample : 04386-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF0

Quant Time: Sep 23 02:40:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

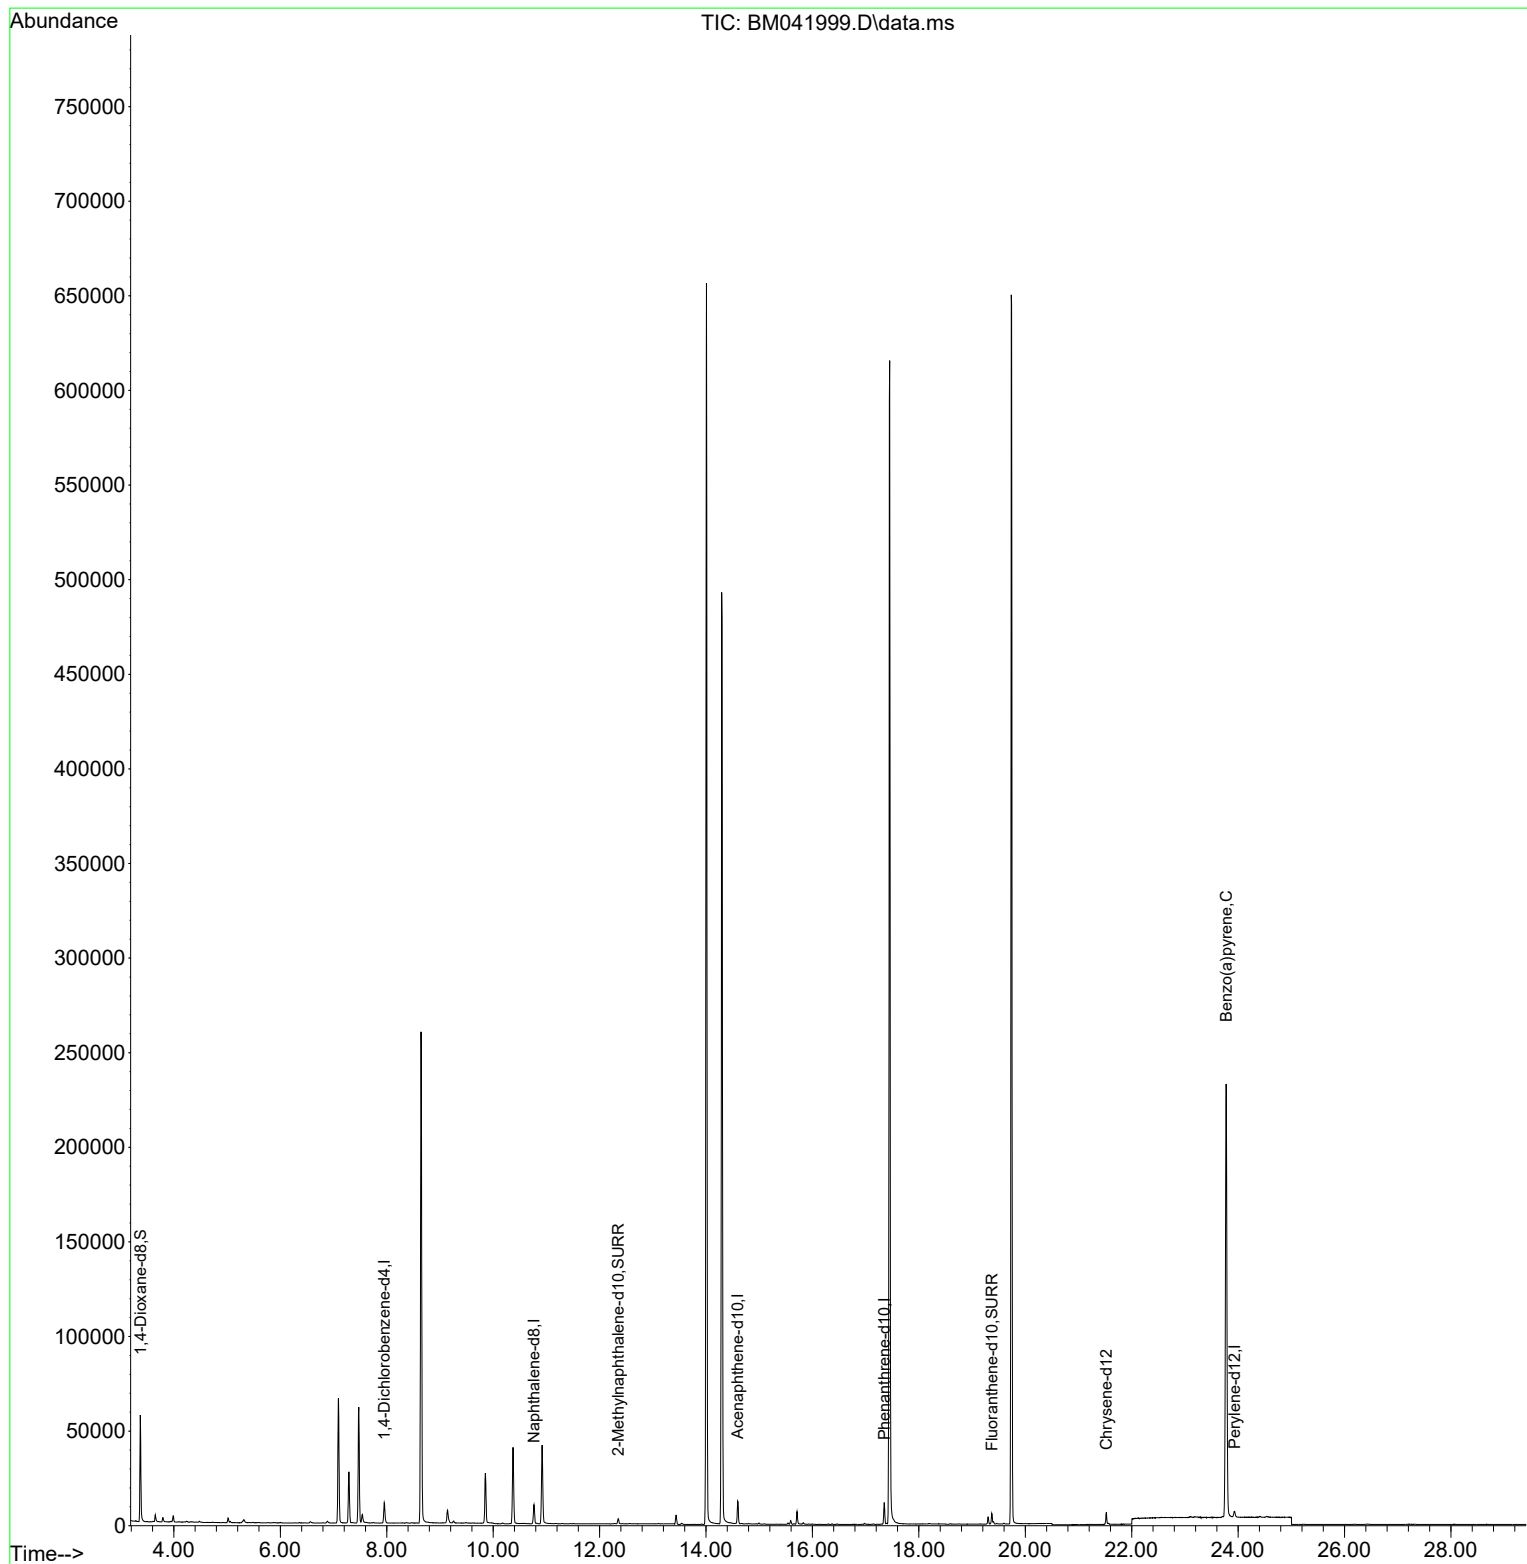

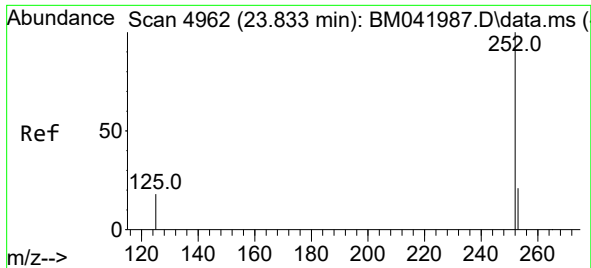

#26

Benzo(a)pyrene

Concen: 0.084 ng/ul

RT: 23.775 min Scan# 49

Delta R.T. -0.053 min

Lab File: BM041999.D


Acq: 22 Sep 2023 22:29

Instrument :

BNA_M

ClientSampleId :

C0AF0

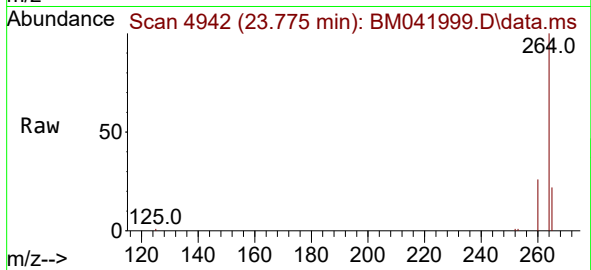

Tgt Ion:252 Resp: 2419

Ion Ratio Lower Upper

252 100

253 59.7 23.2 34.8#

125 66.9 22.5 33.7#

