

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM042013.D
 Acq On : 23 Sep 2023 07:37
 Operator : MA/JU
 Sample : 04386-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF7

Quant Time: Sep 25 01:03:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	5652	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	14432	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	6723	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	14525	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	5744	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	4874	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	33835	4.393	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5060	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	7702	0.326	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.393	88	427	0.053	ng/ul#	1
20) Pyrene	19.738	202	2702	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.769	252	2934	0.095	ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
Data File : BM042013.D
Acq On : 23 Sep 2023 07:37
Operator : MA/JU
Sample : 04386-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Time: Sep 25 01:03:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




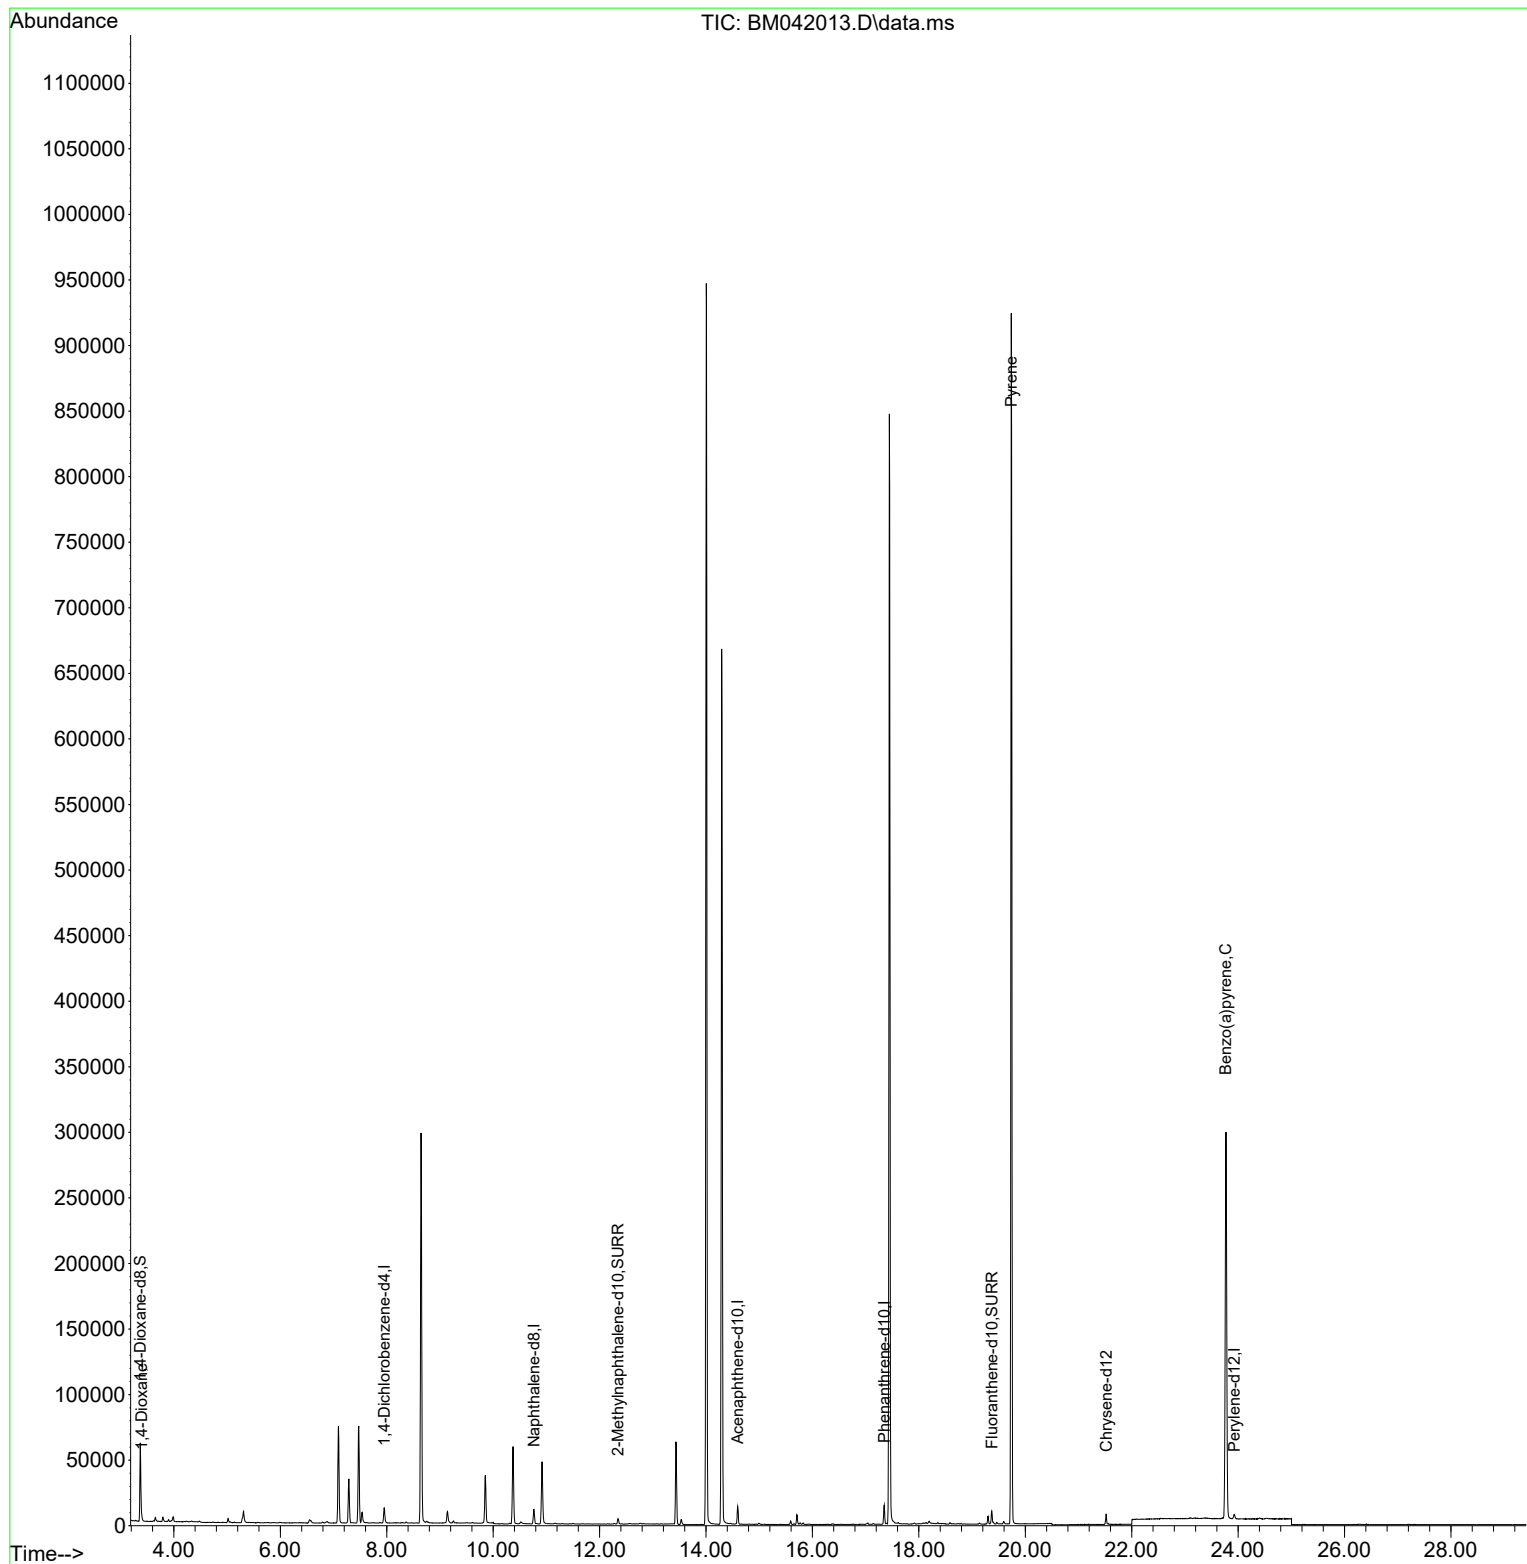


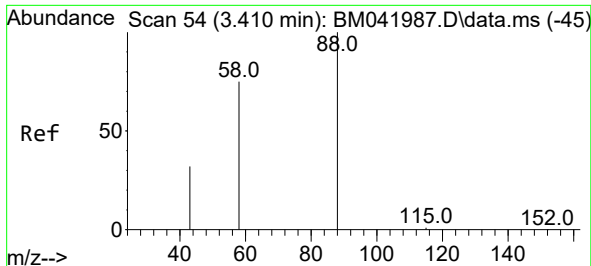

#2
1,4-Dioxane
Concen: 0.053 ng/ul
RT: 3.393 min Scan# 50
Delta R.T. -0.017 min
Lab File: BM042013.D
Acq: 23 Sep 2023 07:37




Instrument :
BNA_M
ClientSampleId :
C0AF7


Tgt Ion: 88 Resp: 427
Ion Ratio Lower Upper
88 100
43 445.1 42.9 64.3#
58 27.8 56.4 84.6#

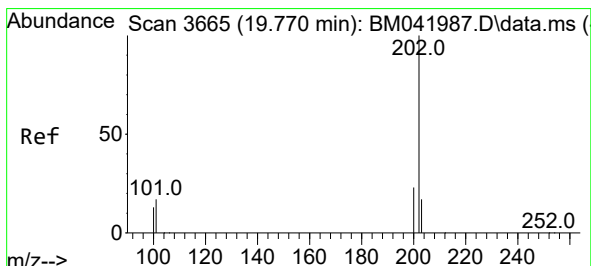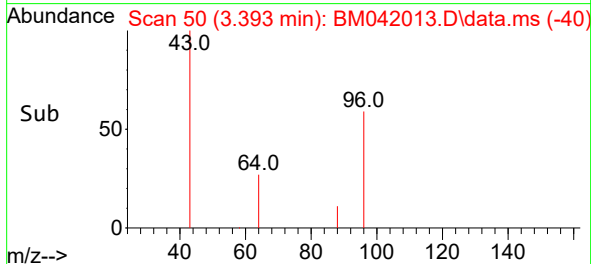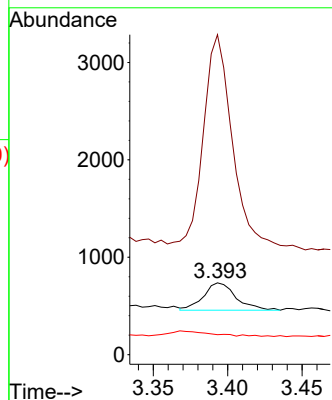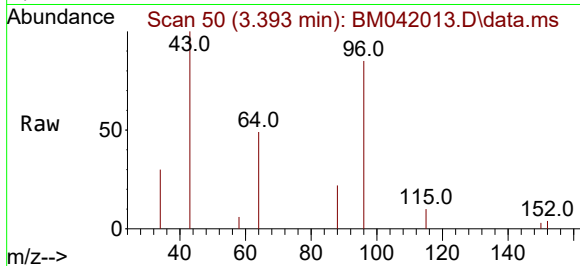

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.738 min Scan# 3658
Delta R.T. -0.033 min
Lab File: BM042013.D
Acq: 23 Sep 2023 07:37


Tgt Ion: 202 Resp: 2702
Ion Ratio Lower Upper
202 100
101 174.6 14.1 21.1#
100 1293.4 11.4 17.0#

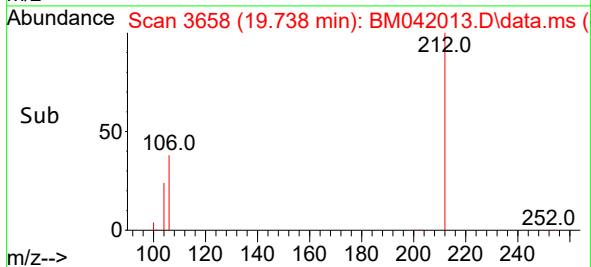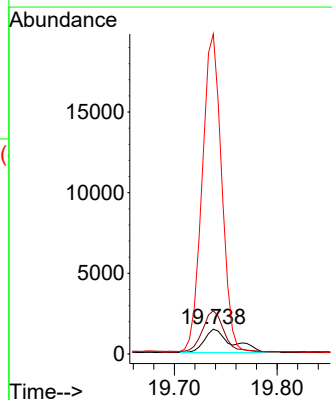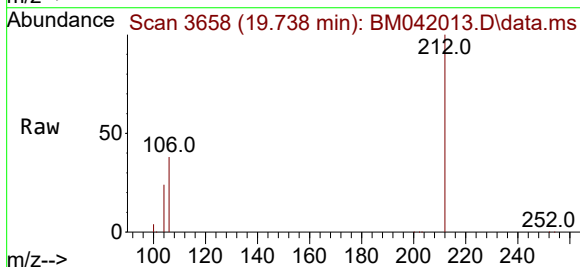

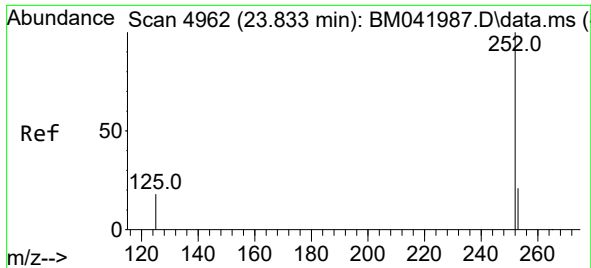

#26
Benzo(a)pyrene
Concen: 0.095 ng/ul
RT: 23.769 min Scan# 4940
Delta R.T. -0.059 min
Lab File: BM042013.D
Acq: 23 Sep 2023 07:37

Instrument :
BNA_M
ClientSampleId :
C0AF7

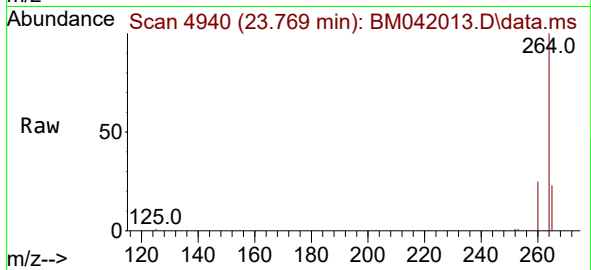

Tgt Ion:252 Resp: 2934
Ion Ratio Lower Upper
252 100
253 62.9 23.2 34.8#
125 69.4 22.5 33.7#

