

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM042017.D
 Acq On : 23 Sep 2023 10:01
 Operator : MA/JU
 Sample : 04386-14
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM9

Quant Time: Sep 25 01:04:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.950	152	5213	0.400	ng/ul	0.00
4) Naphthalene-d8	10.763	136	12916	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	5887	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	11985	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	4430	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	4122	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	33873	4.768	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	5493	0.340	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	7432	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.738	202	2555	0.052	ng/ul#	1
26) Benzo(a)pyrene	23.772	252	3011	0.115	ng/ul#	30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
Data File : BM042017.D
Acq On : 23 Sep 2023 10:01
Operator : MA/JU
Sample : 04386-14
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM9

Quant Time: Sep 25 01:04:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




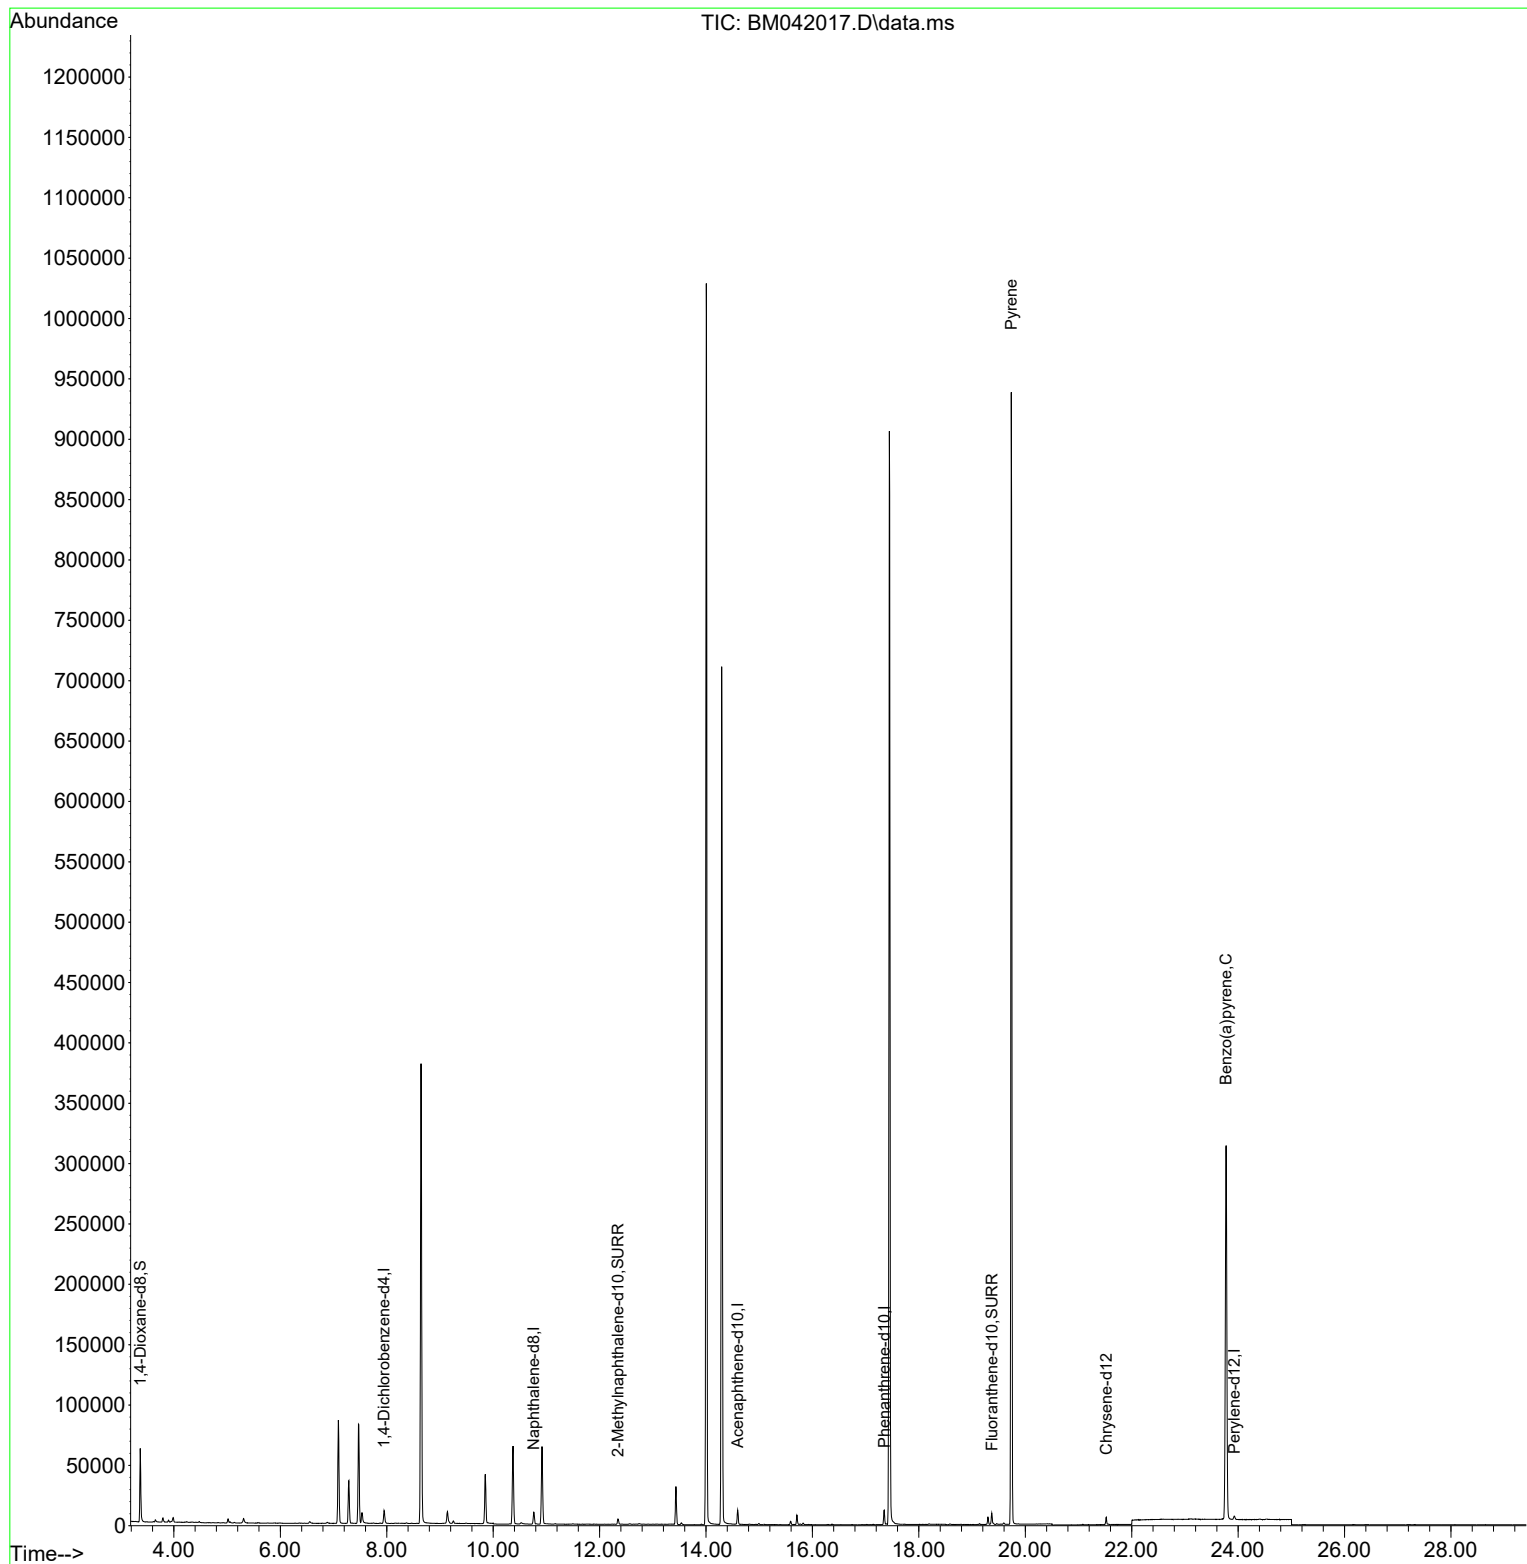


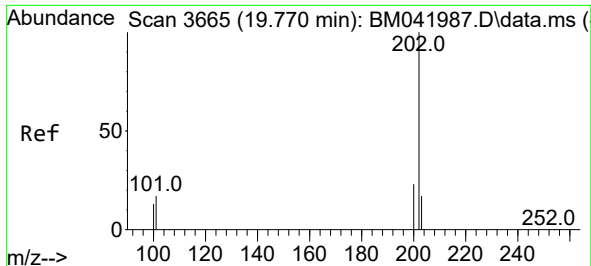

#20
Pyrene
Concen: 0.052 ng/ul
RT: 19.738 min Scan# 301
Delta R.T. -0.033 min
Lab File: BM042017.D
Acq: 23 Sep 2023 10:01

Instrument :
BNA_M
ClientSampleId :
C0AM9

Tgt Ion:202 Resp: 2555
Ion Ratio Lower Upper
202 100
101 181.9 14.1 21.1#
100 1339.3 11.4 17.0#

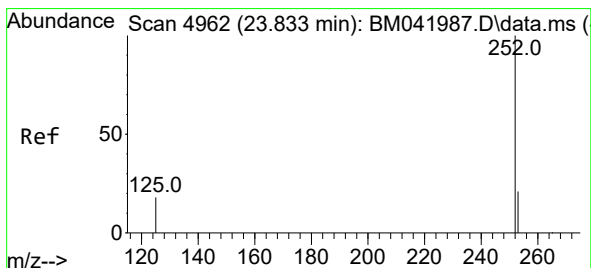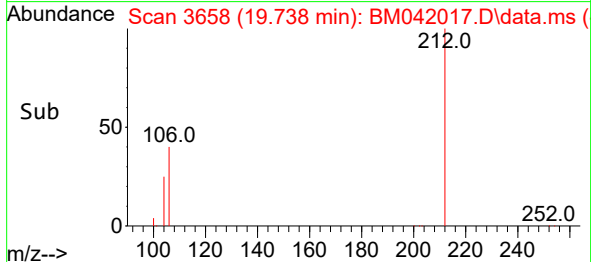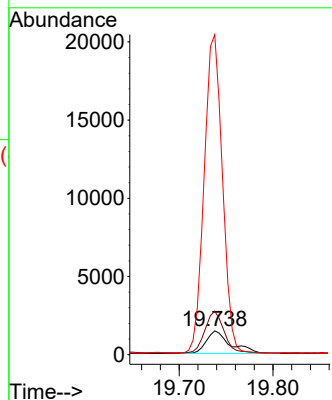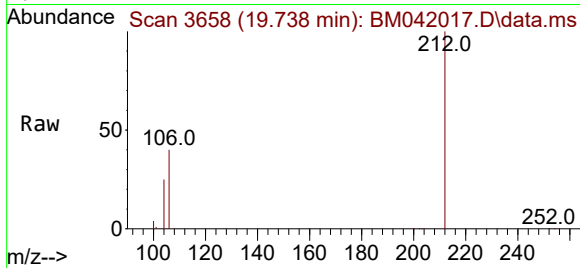

#26
Benzo(a)pyrene
Concen: 0.115 ng/ul
RT: 23.772 min Scan# 4941
Delta R.T. -0.056 min
Lab File: BM042017.D
Acq: 23 Sep 2023 10:01

Tgt Ion:252 Resp: 3011
Ion Ratio Lower Upper
252 100
253 60.1 23.2 34.8#
125 71.4 22.5 33.7#

