

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM041991.D
 Acq On : 22 Sep 2023 17:37
 Operator : MA/JU
 Sample : 04378-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHL2

Quant Time: Sep 22 18:23:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	7753	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	18921	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	8868	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	16310	0.400	ng/ul	0.00
17) Chrysene-d12	21.524	240	6650	0.400	ng/ul	0.00
23) Perylene-d12	23.933	264	6733	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	49146	4.652	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	7337	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	11326	0.414	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	75047	6.752	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
Data File : BM041991.D
Acq On : 22 Sep 2023 17:37
Operator : MA/JU
Sample : 04378-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHL2

Quant Time: Sep 22 18:23:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

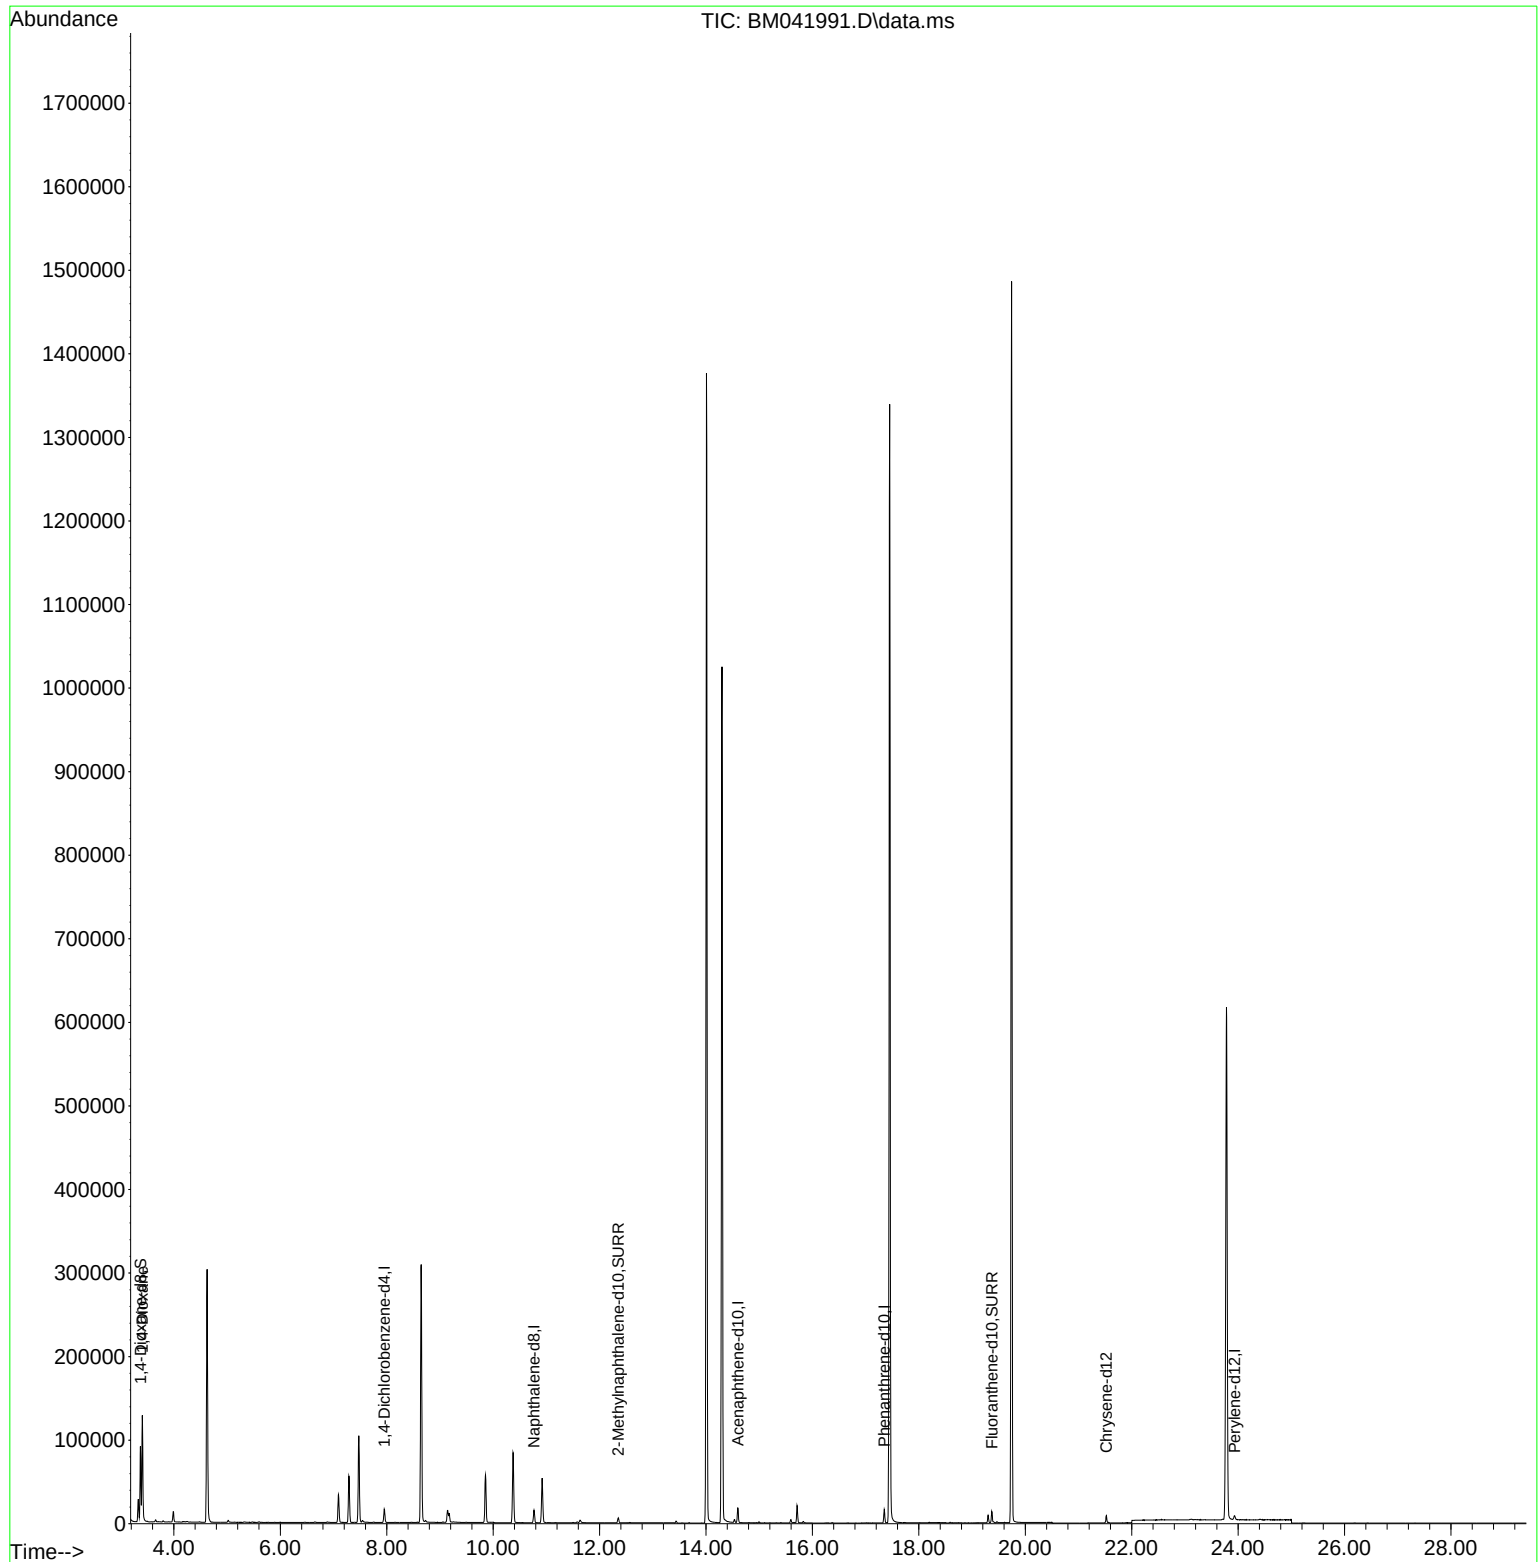

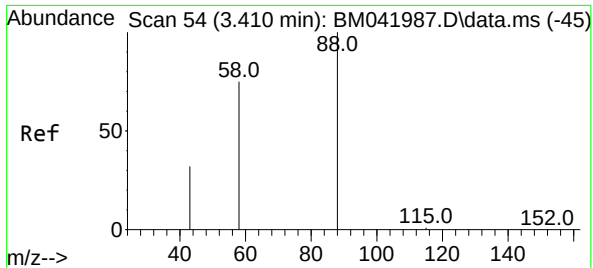

#2
 1,4-Dioxane
 Concen: 6.752 ng/ul
 RT: 3.406 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM041991.D
 Acq: 22 Sep 2023 17:37

Instrument :
 BNA_M
 ClientSampleId :
 BBHL2

Tgt Ion: 88 Resp: 75047

Ion	Ratio	Lower	Upper
88	100		
43	35.5	42.9	64.3#
58	79.9	56.4	84.6

