

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM042002.D
 Acq On : 23 Sep 2023 00:20
 Operator : MA/JU
 Sample : 04386-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF8

Quant Time: Sep 23 02:40:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	5155	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	13020	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	6276	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	11738	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	4712	0.400	ng/ul	0.00
23) Perylene-d12	23.930	264	4570	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	34682	4.937	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.352	152	4238	0.260	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	5559	0.287	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.403	202	1588	0.030	ng/ul#	87
24) Benzo(b)fluoranthene	23.190	252	902	0.026	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
Data File : BM042002.D
Acq On : 23 Sep 2023 00:20
Operator : MA/JU
Sample : 04386-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF8

Quant Time: Sep 23 02:40:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration




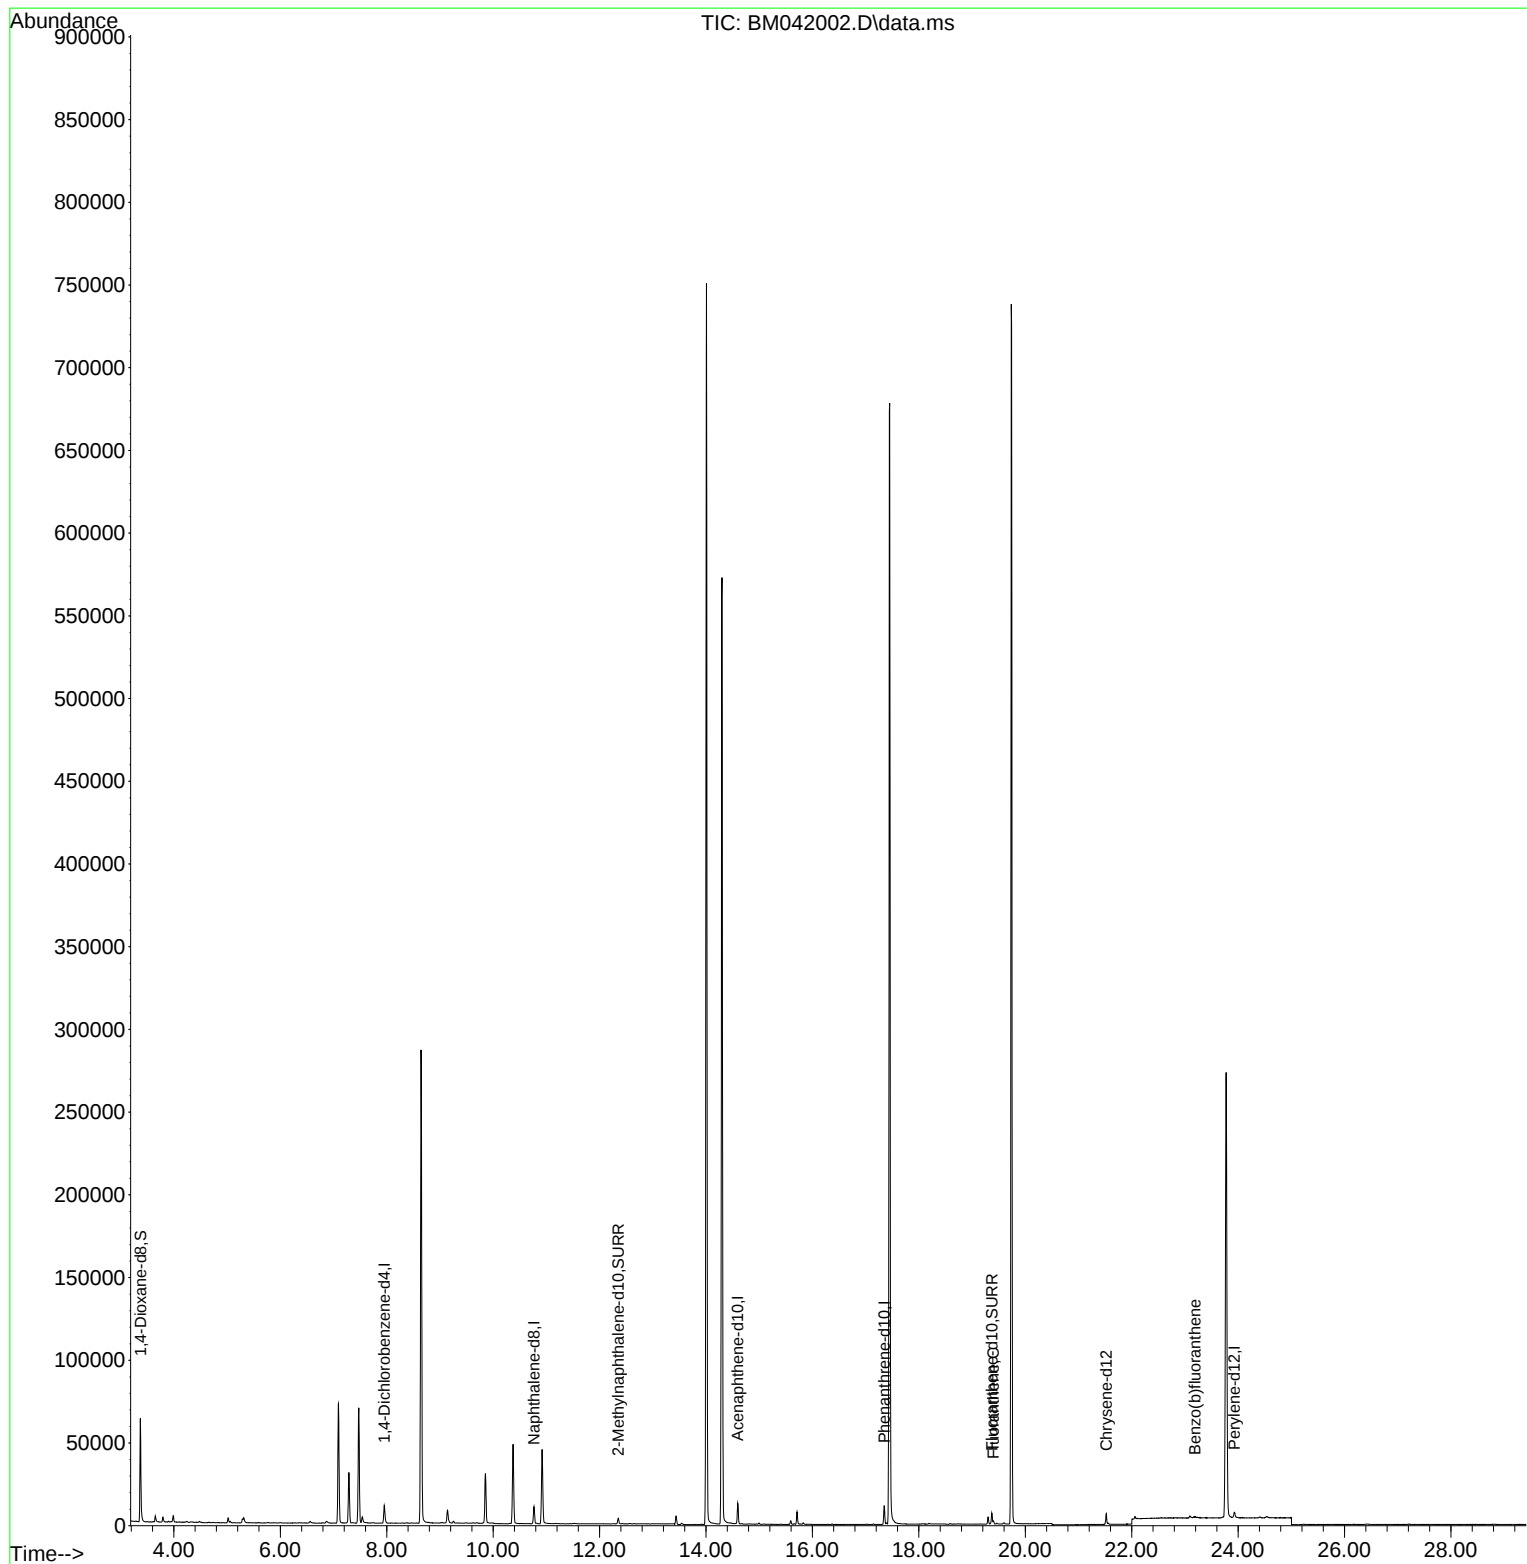


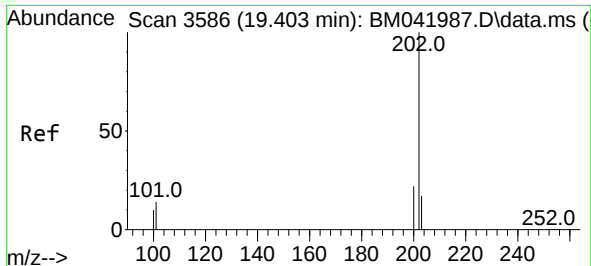

#19
Fluoranthene
Concen: 0.030 ng/ul
RT: 19.403 min Scan# 31
Delta R.T. 0.000 min
Lab File: BM042002.D
Acq: 23 Sep 2023 00:20

Instrument :
BNA_M
ClientSampleId :
C0AF8

Tgt Ion:202 Resp: 1588
Ion Ratio Lower Upper
202 100
101 20.6 11.8 17.6#
100 15.9 9.1 13.7#

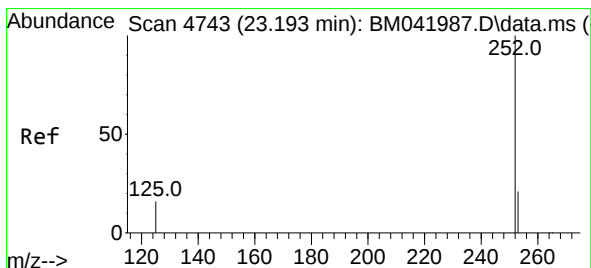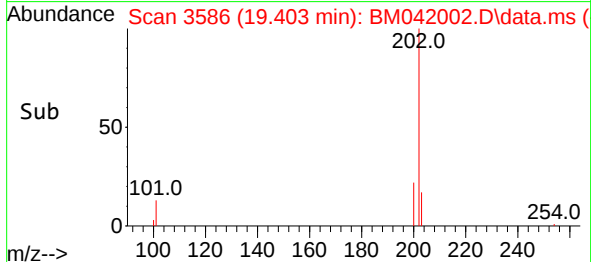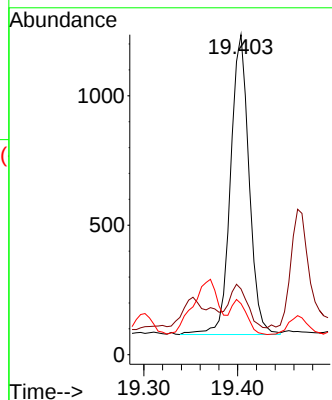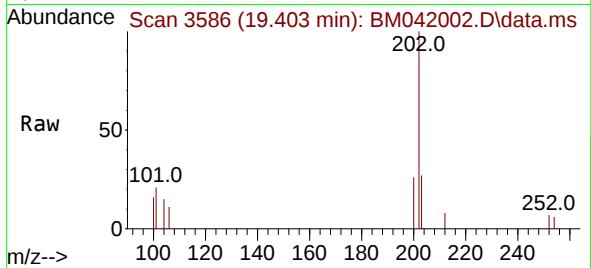

#24
Benzo(b)fluoranthene
Concen: 0.026 ng/ul
RT: 23.190 min Scan# 4742
Delta R.T. 0.000 min
Lab File: BM042002.D
Acq: 23 Sep 2023 00:20

Tgt Ion:252 Resp: 902
Ion Ratio Lower Upper
252 100
253 84.3 0.0 54.4#
125 119.3 0.0 46.2#

