

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM042011.D
 Acq On : 23 Sep 2023 06:25
 Operator : MA/JU
 Sample : 04344-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBHX3

Quant Time: Sep 25 01:03:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	6854	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	17799	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	8476	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	17992	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	7298	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	6579	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.368	96	35782	3.831	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	7400	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	13071	0.435	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	21213	2.159	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
Data File : BM042011.D
Acq On : 23 Sep 2023 06:25
Operator : MA/JU
Sample : 04344-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BBHX3


Quant Time: Sep 25 01:03:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration

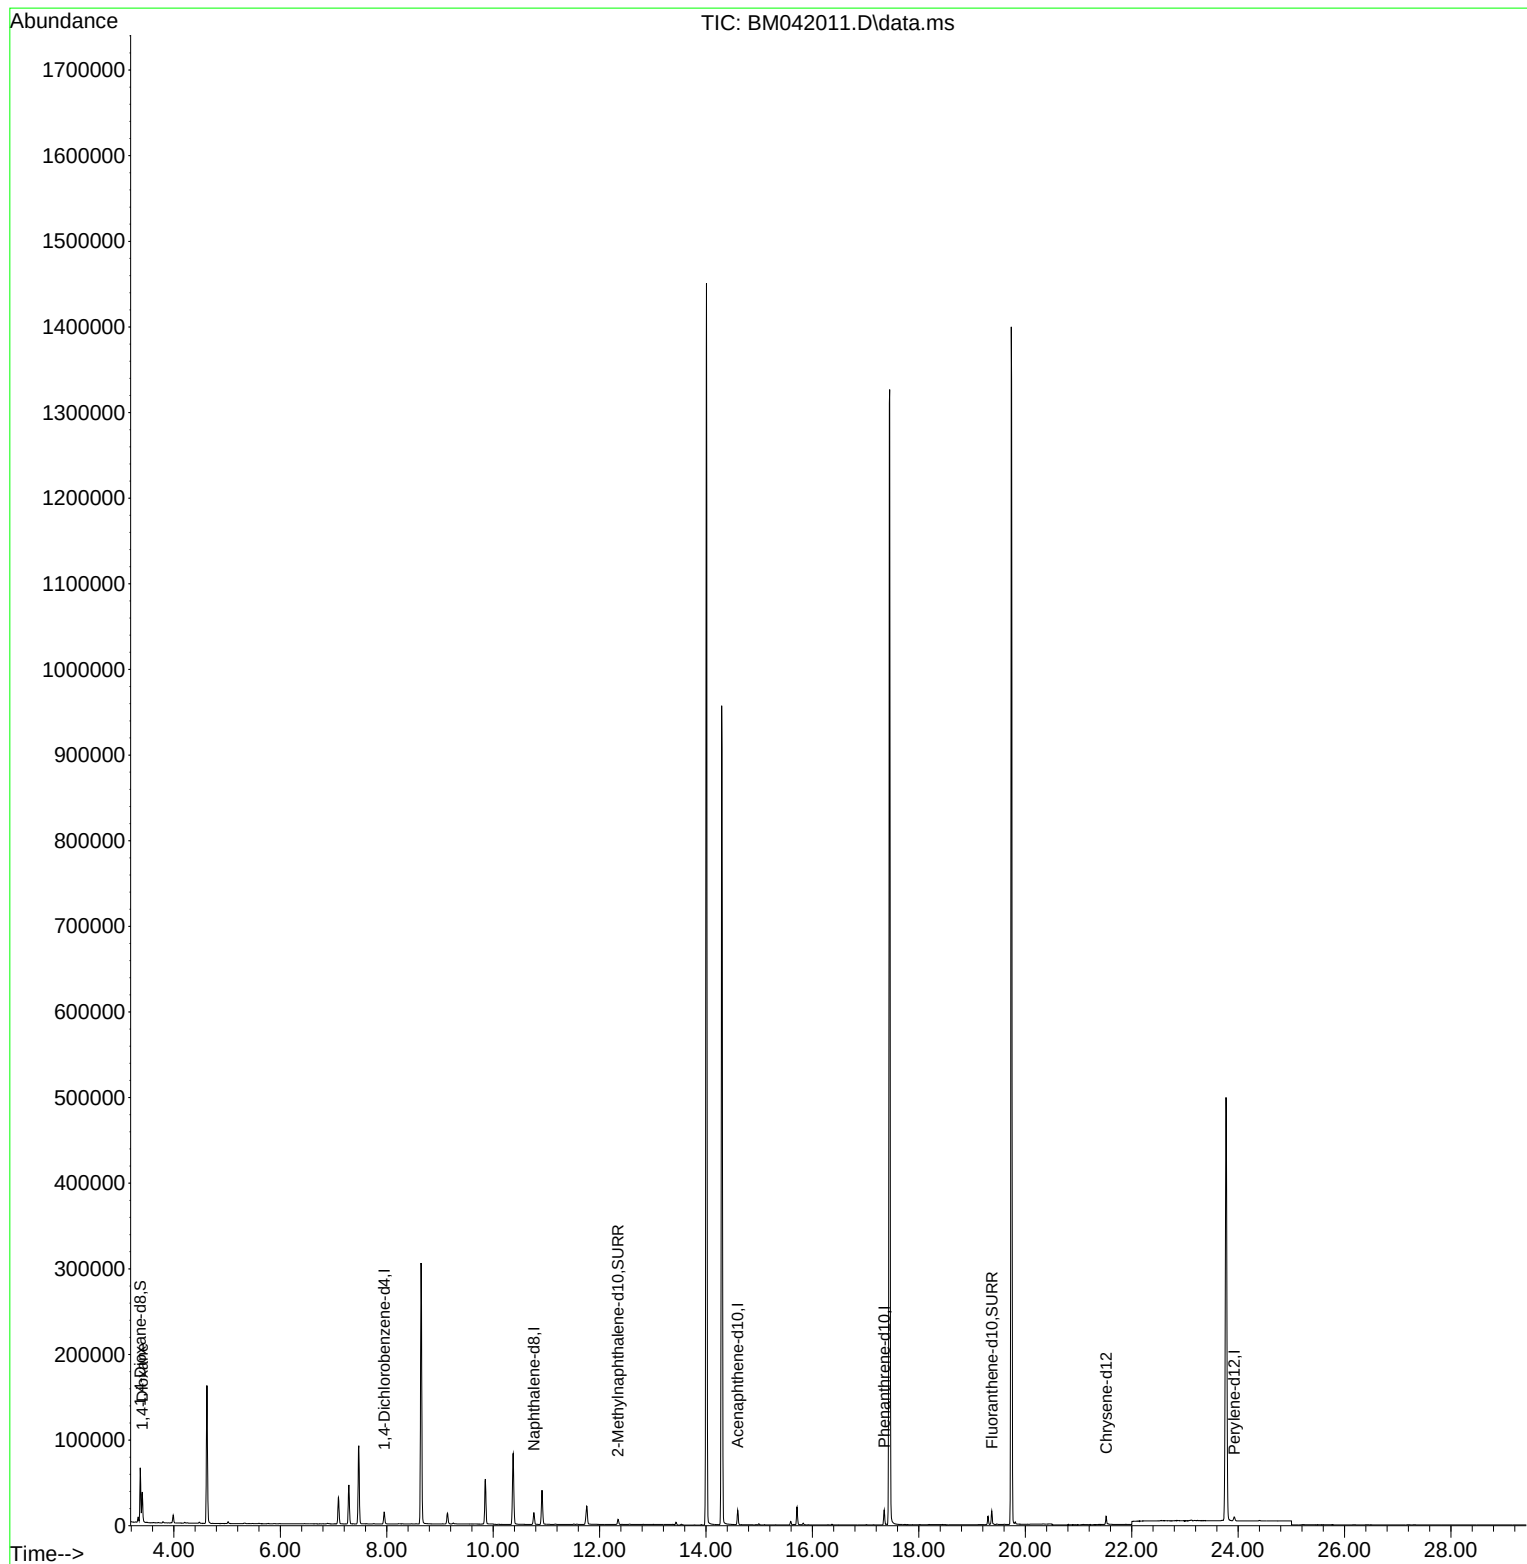

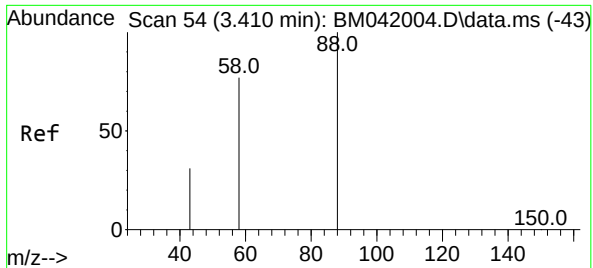

#2
 1,4-Dioxane
 Concen: 2.159 ng/ul
 RT: 3.406 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM042011.D
 Acq: 23 Sep 2023 06:25

Instrument :
 BNA_M
 ClientSampleId :
 BBHX3

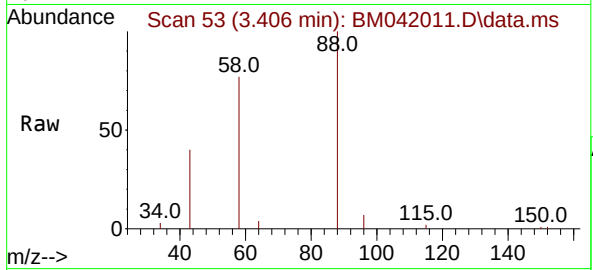

Tgt Ion: 88 Resp: 21213

Ion	Ratio	Lower	Upper
88	100		
43	40.1	42.9	64.3#
58	76.6	56.4	84.6

