

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092223\
 Data File : BM042012.D
 Acq On : 23 Sep 2023 07:01
 Operator : MA/JU
 Sample : 04378-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BBKA9

Quant Time: Sep 25 01:03:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 22 13:50:58 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.954	152	5290	0.400	ng/ul	0.00
4) Naphthalene-d8	10.768	136	14734	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.597	164	6683	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	13826	0.400	ng/ul	0.00
17) Chrysene-d12	21.521	240	5196	0.400	ng/ul	0.00
23) Perylene-d12	23.927	264	4862	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	28526	3.957	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.346	152	6610	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	11128	0.520	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.406	88	1091	0.144	ng/ul#	32
5) Naphthalene	10.818	128	1924	0.039	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 25 01:03:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM092223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 22 13:50:58 2023
Response via : Initial Calibration







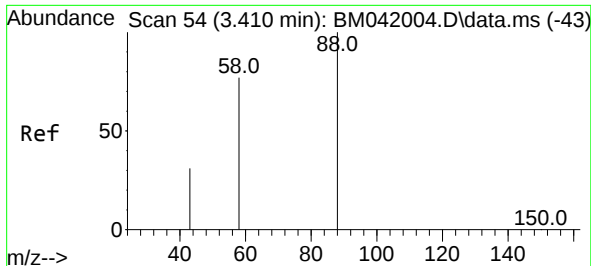

#2
1,4-Dioxane
Concen: 0.144 ng/ul
RT: 3.406 min Scan# 51
Delta R.T. -0.004 min
Lab File: BM042012.D
Acq: 23 Sep 2023 07:01

Instrument :
BNA_M
ClientSampleId :
BBKA9

Tgt Ion: 88 Resp: 1091
Ion Ratio Lower Upper
88 100
43 156.9 42.9 64.3#
58 63.3 56.4 84.6

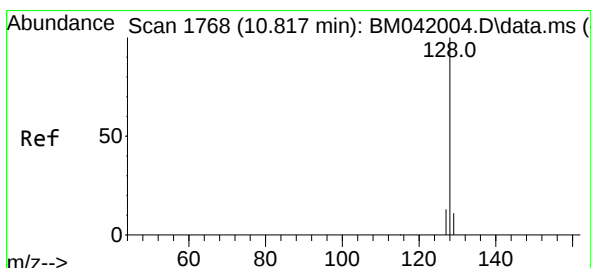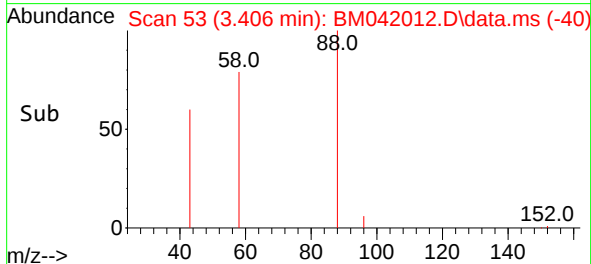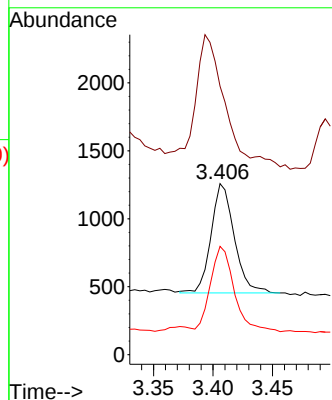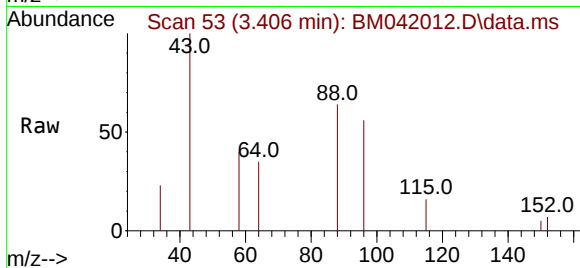

#5
Naphthalene
Concen: 0.039 ng/ul
RT: 10.818 min Scan# 1768
Delta R.T. 0.000 min
Lab File: BM042012.D
Acq: 23 Sep 2023 07:01

Tgt Ion: 128 Resp: 1924
Ion Ratio Lower Upper
128 100
129 19.8 9.2 13.8#
127 18.0 10.8 16.2#

