

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092324\
 Data File : BM047600.D
 Acq On : 23 Sep 2024 11:04
 Operator : RC/JU
 Sample : PB163344BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB163344BL

Quant Time: Sep 23 18:57:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 21 02:22:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.845	152	304832	20.000	ng	0.00
21) Naphthalene-d8	10.634	136	1161519	20.000	ng	0.00
39) Acenaphthene-d10	14.469	164	523773	20.000	ng	0.00
64) Phenanthrene-d10	17.204	188	914542	20.000	ng	0.00
76) Chrysene-d12	21.427	240	616013	20.000	ng	-0.01
86) Perylene-d12	24.450	264	584879	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.416	112	1920175	96.531	ng	0.00
7) Phenol-d6	7.004	99	2440958	93.130	ng	0.00
23) Nitrobenzene-d5	8.992	82	2245447	96.235	ng	0.00
42) 2,4,6-Tribromophenol	15.951	330	338589	69.812	ng	0.00
45) 2-Fluorobiphenyl	13.098	172	4038464	109.099	ng	0.00
79) Terphenyl-d14	19.821	244	4365635	127.158	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092324\
Data File : BM047600.D
Acq On : 23 Sep 2024 11:04
Operator : RC/JU
Sample : PB163344BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB163344BL


Quant Time: Sep 23 18:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:22:39 2024
Response via : Initial Calibration

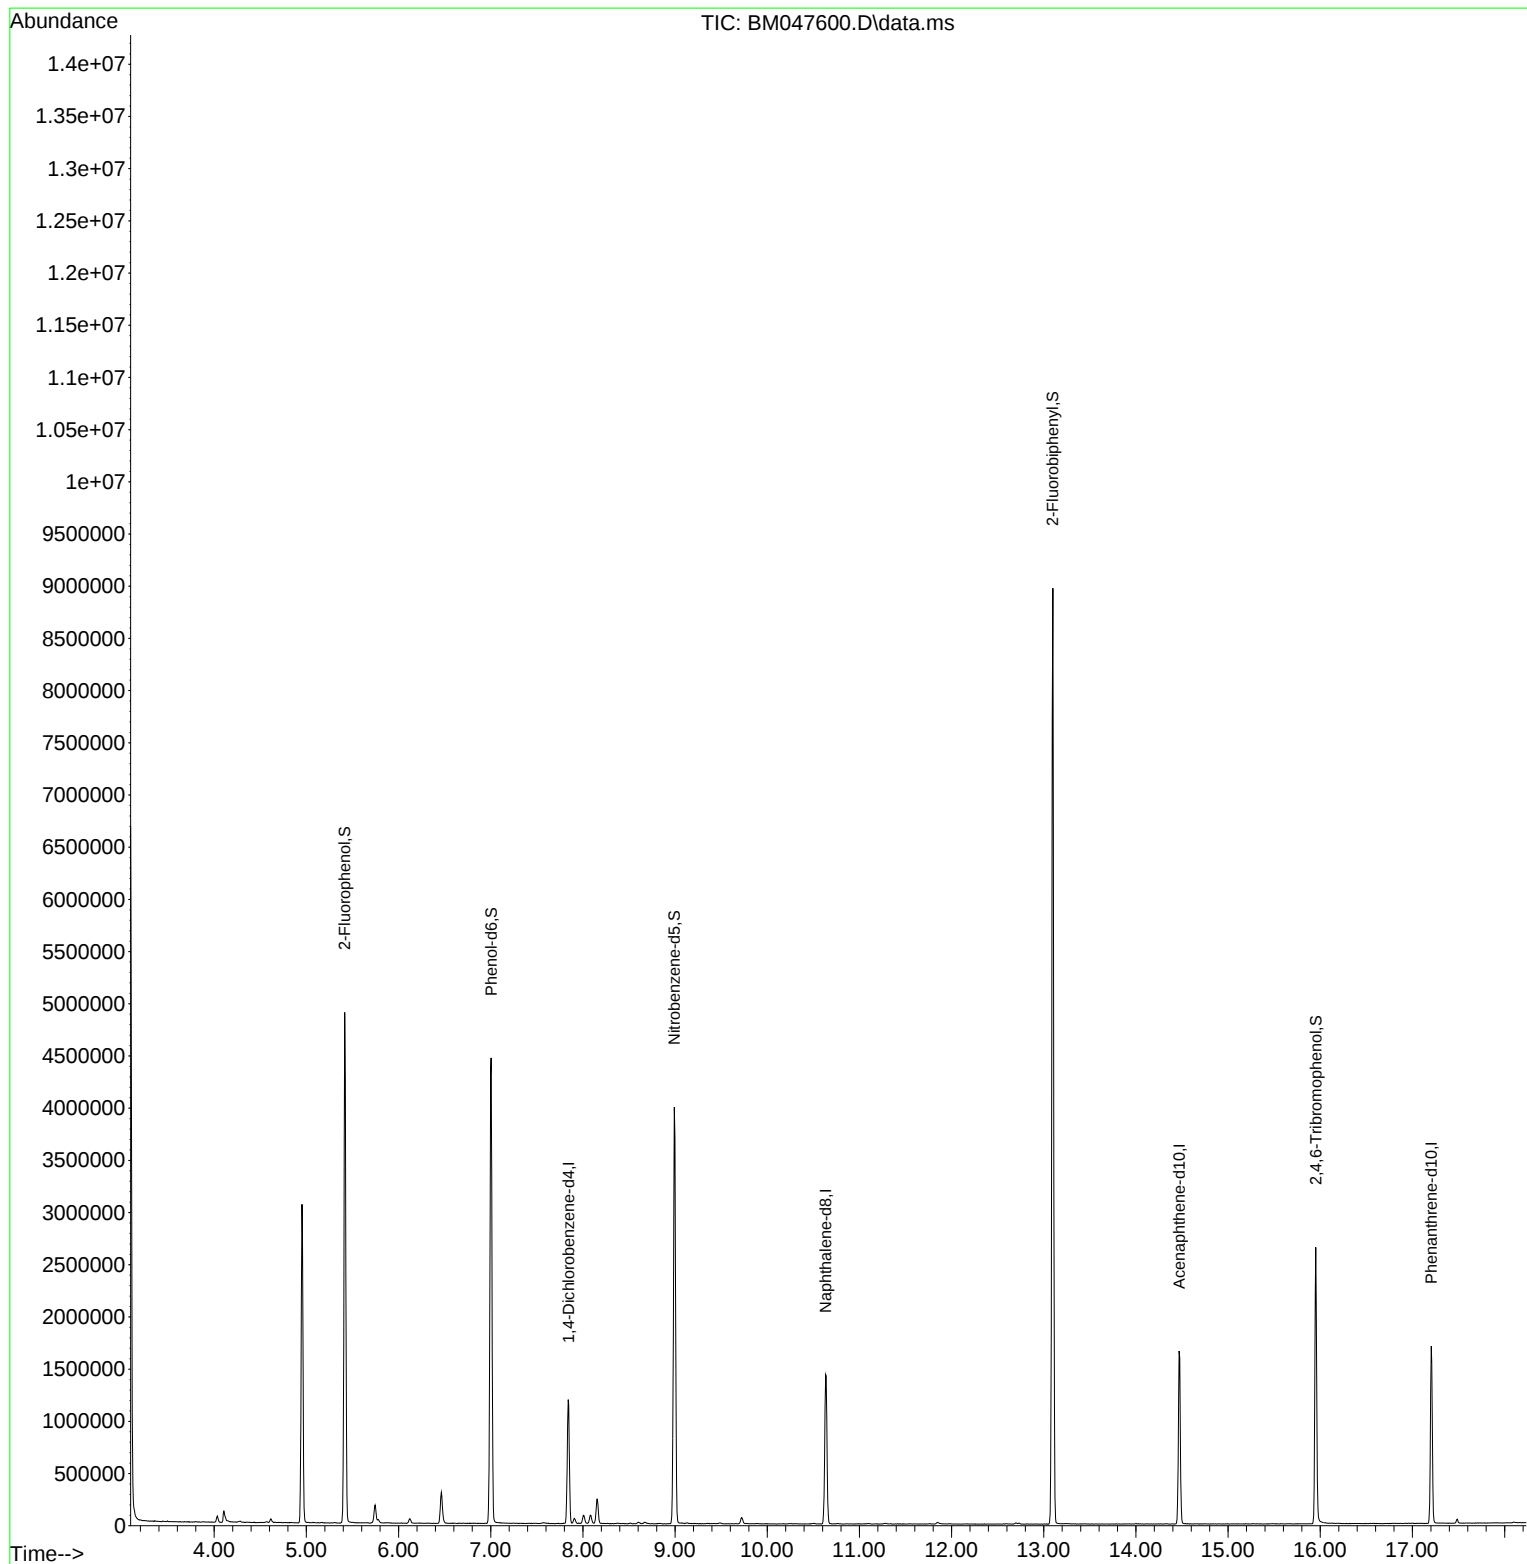


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092324\
Data File : BM047600.D
Acq On : 23 Sep 2024 11:04
Operator : RC/JU
Sample : PB163344BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB163344BL

Quant Time: Sep 23 18:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 21 02:22:39 2024
Response via : Initial Calibration




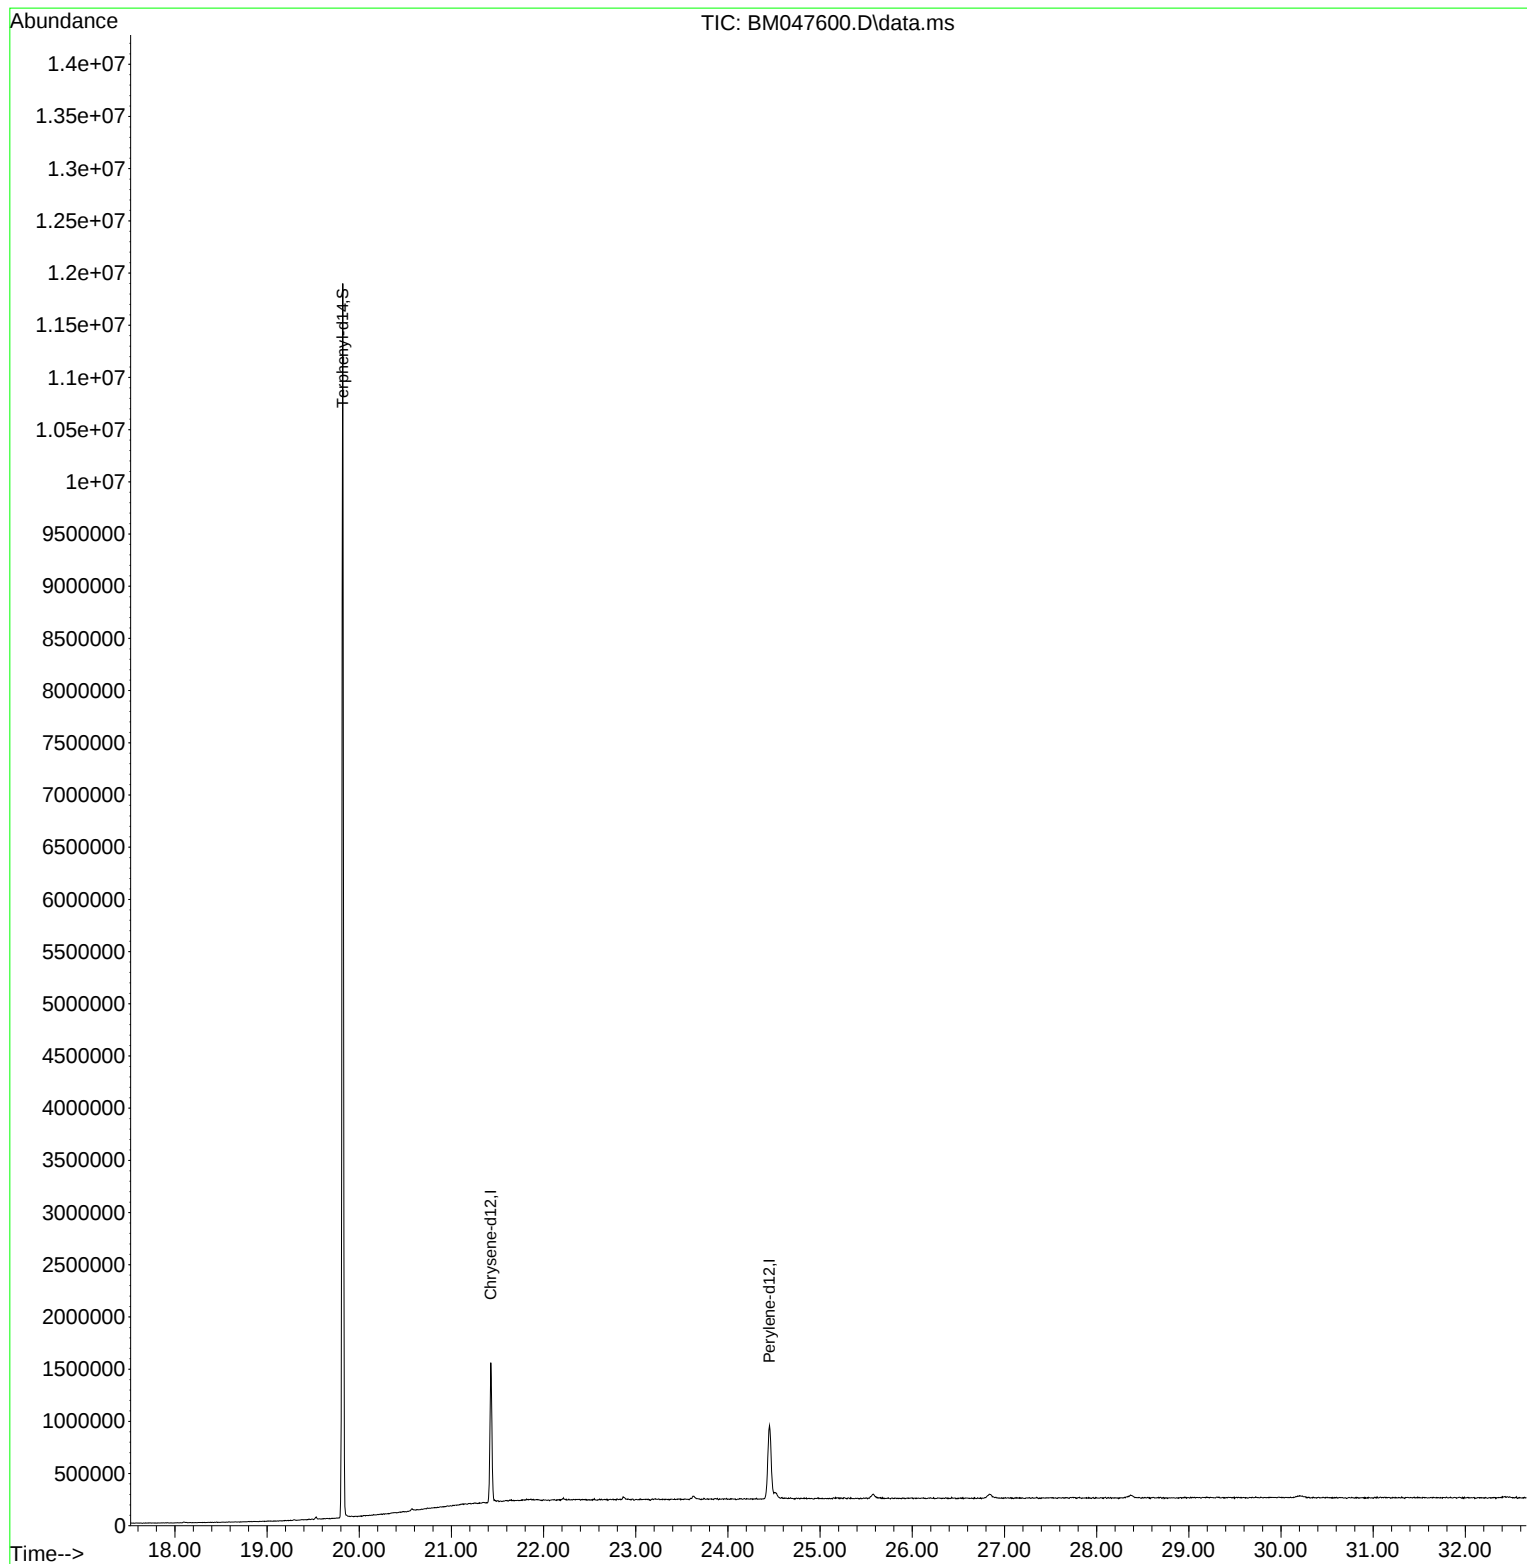


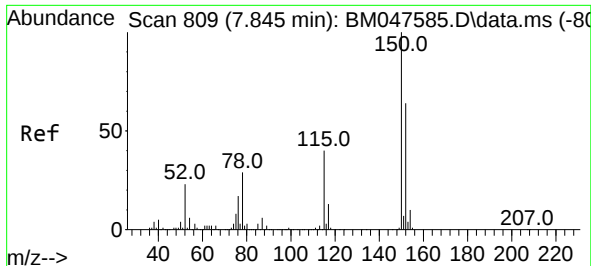

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.845 min Scan# 809
Delta R.T. 0.000 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04




Instrument :
BNA_M
ClientSampleId :
PB163344BL


Tgt Ion:152 Resp: 304832
Ion Ratio Lower Upper
152 100
150 155.6 124.5 186.7
115 60.6 49.9 74.9

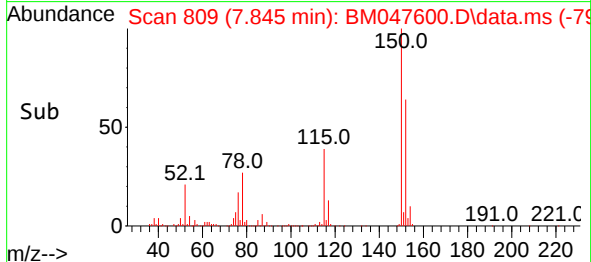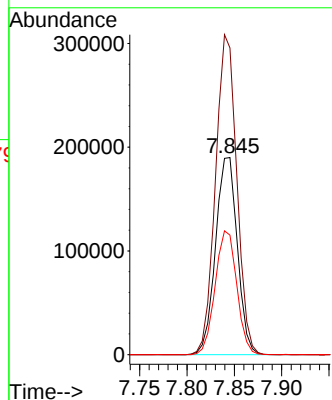

#5
2-Fluorophenol
Concen: 96.531 ng
RT: 5.416 min Scan# 396
Delta R.T. -0.006 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04

Tgt Ion:112 Resp: 1920175
Ion Ratio Lower Upper
112 100
64 58.3 46.8 70.2
63 31.8 25.2 37.8

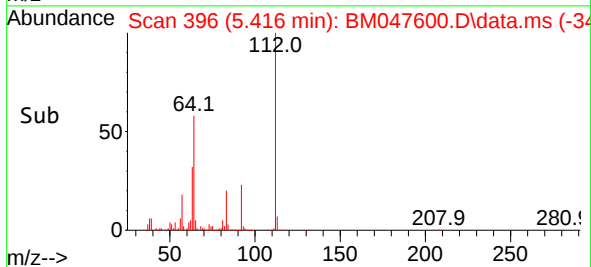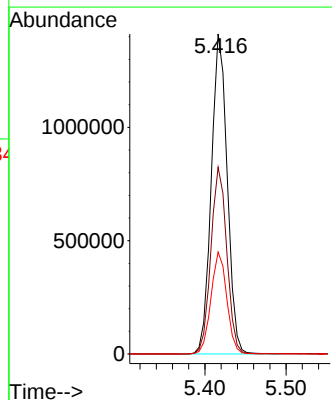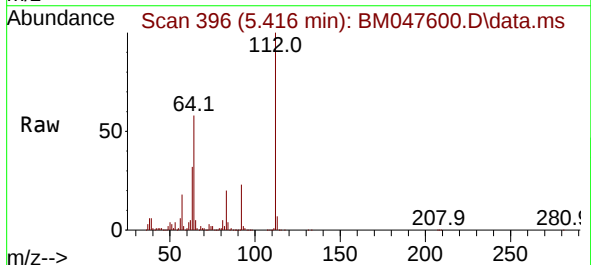




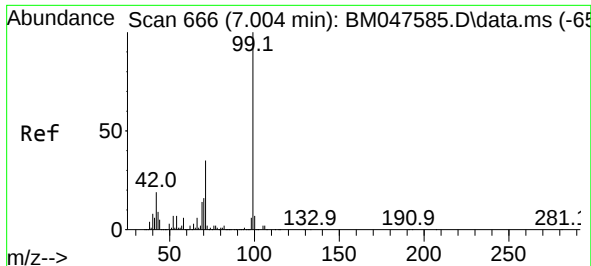


#7
Phenol-d6
Concen: 93.130 ng
RT: 7.004 min Scan# 666
Delta R.T. 0.000 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04

Instrument :
BNA_M
ClientSampleId :
PB163344BL

Tgt Ion: 99 Resp: 2440958




Ion	Ratio	Lower	Upper
99	100		
42	17.8	15.3	22.9
71	33.8	27.8	41.6

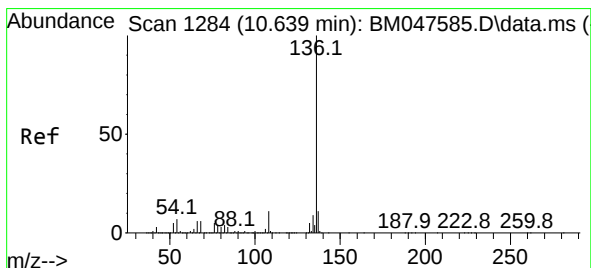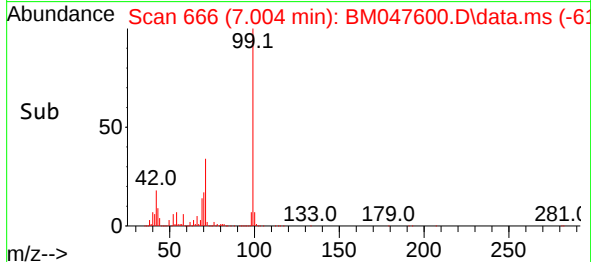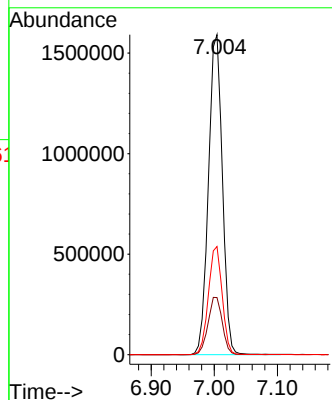


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.634 min Scan# 1283
Delta R.T. -0.006 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04

Tgt Ion: 136 Resp: 1161519

Ion	Ratio	Lower	Upper
136	100		
137	11.1	9.0	13.4
54	7.5	6.0	9.0
68	6.4	4.6	7.0


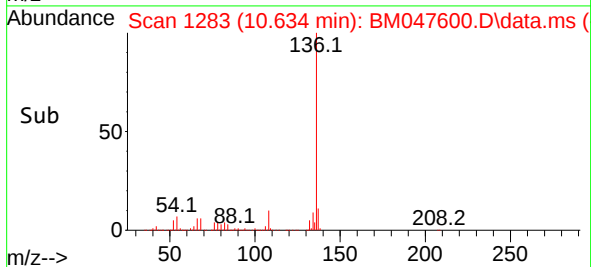
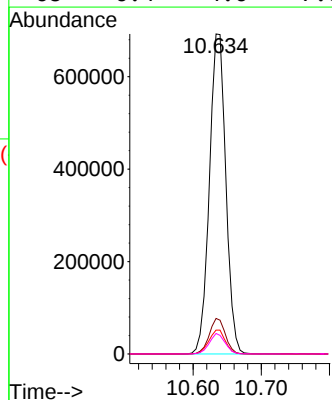
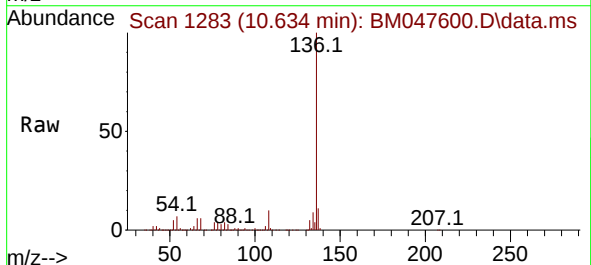


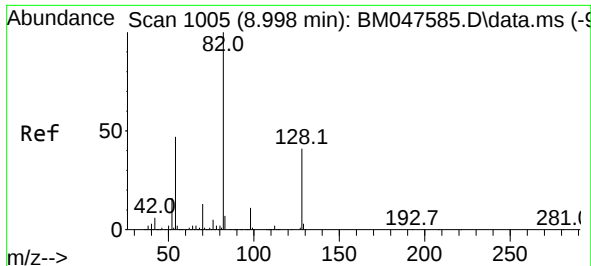

#23
Nitrobenzene-d5
Concen: 96.235 ng
RT: 8.992 min Scan# 1004
Delta R.T. -0.006 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04




Instrument :
BNA_M
ClientSampleId :
PB163344BL


Tgt Ion: 82 Resp: 2245447
Ion Ratio Lower Upper
82 100
128 41.0 32.5 48.7
54 46.4 37.5 56.3

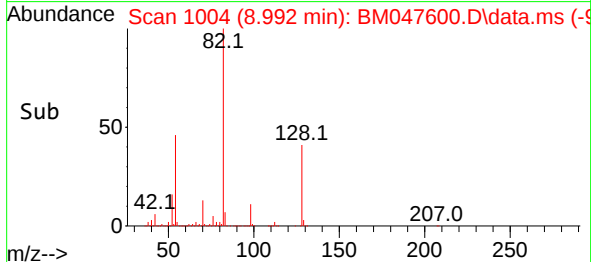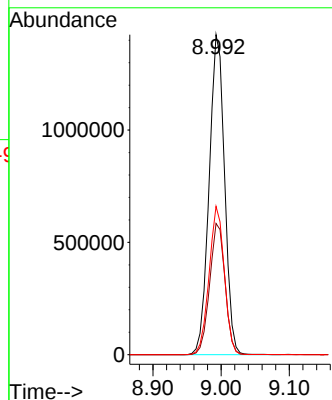

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.469 min Scan# 1935
Delta R.T. -0.005 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04

Tgt Ion:164 Resp: 523773
Ion Ratio Lower Upper
164 100
162 104.2 82.6 123.8
160 49.6 37.8 56.6


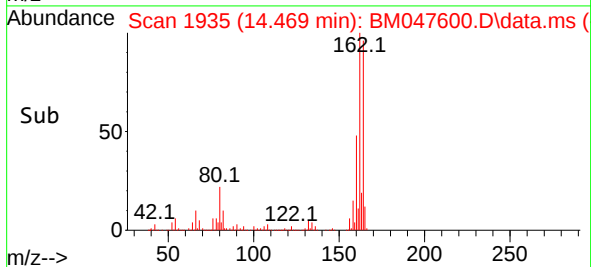
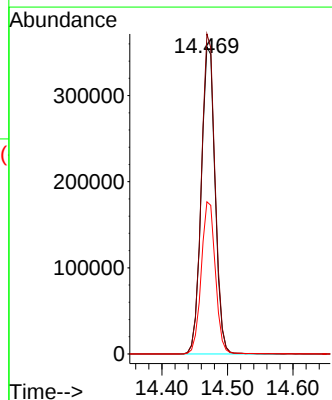
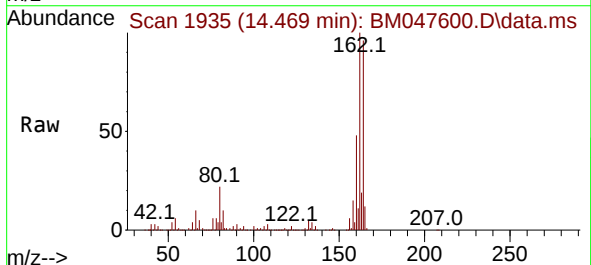


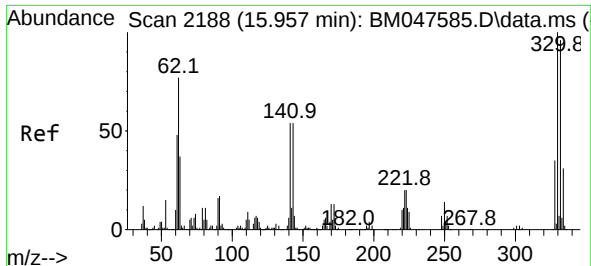

#42
2,4,6-Tribromophenol
Concen: 69.812 ng
RT: 15.951 min Scan# 2187
Delta R.T. -0.006 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04




Instrument :
BNA_M
ClientSampleId :
PB163344BL


Tgt Ion:330 Resp: 338589
Ion Ratio Lower Upper
330 100
332 95.6 77.0 115.4
141 59.6 45.9 68.9

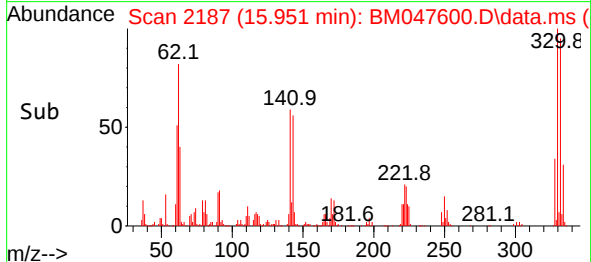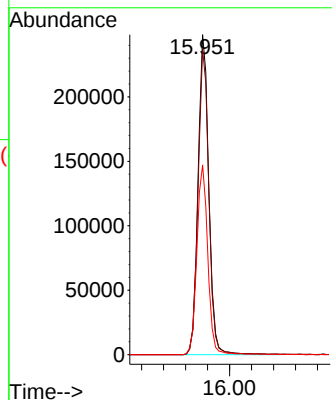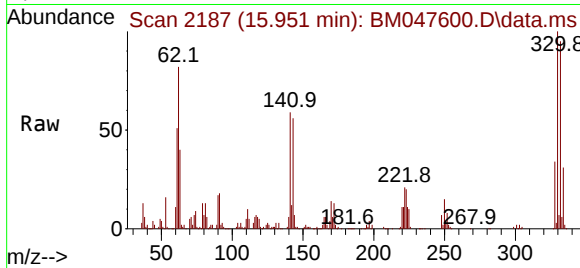

#45
2-Fluorobiphenyl
Concen: 109.099 ng
RT: 13.098 min Scan# 1702
Delta R.T. -0.006 min
Lab File: BM047600.D
Acq: 23 Sep 2024 11:04

Tgt Ion:172 Resp: 4038464
Ion Ratio Lower Upper
172 100
171 35.4 28.1 42.1
170 24.3 19.0 28.6

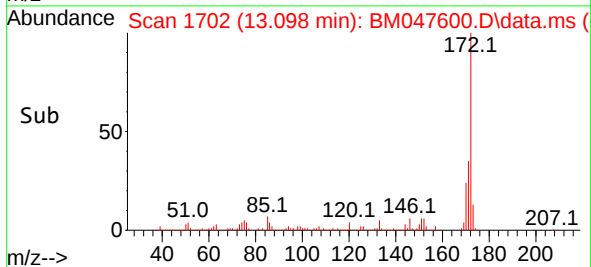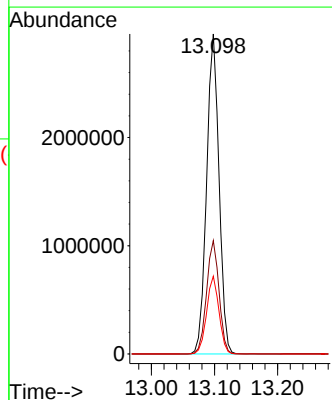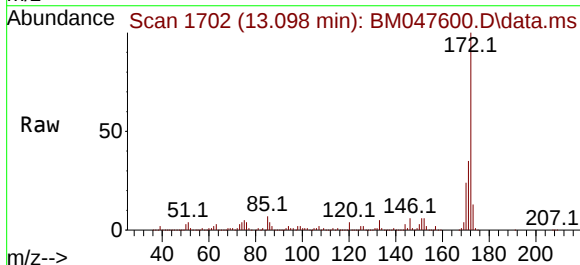



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.204 min Scan# 2401

Delta R.T. -0.005 min

Lab File: BM047600.D

Acq: 23 Sep 2024 11:04

Instrument :

BNA_M

ClientSampleId :

PB163344BL





Tgt Ion:188 Resp: 914542

Ion Ratio Lower Upper

188 100

94 10.9 8.6 13.0

80 12.4 9.9 14.9

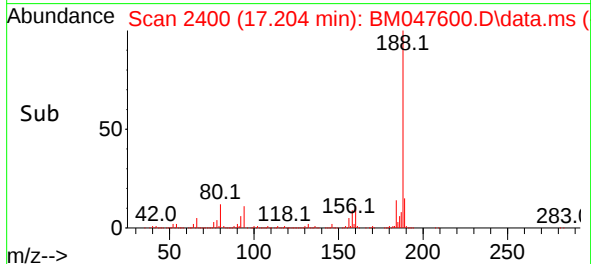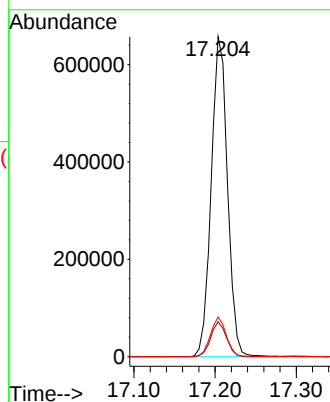

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.427 min Scan# 3118

Delta R.T. -0.012 min

Lab File: BM047600.D

Acq: 23 Sep 2024 11:04




Tgt Ion:240 Resp: 616013


Ion Ratio Lower Upper

240 100

120 14.3 10.8 16.2

236 26.3 20.8 31.2

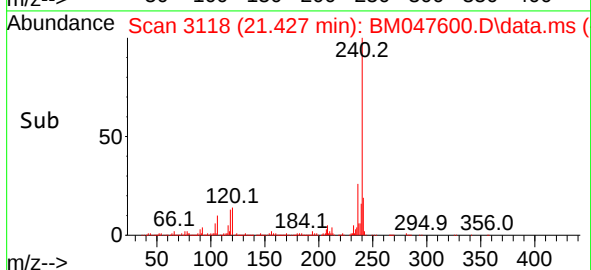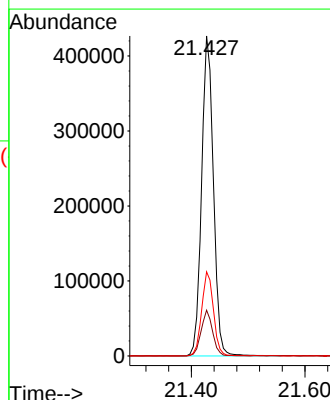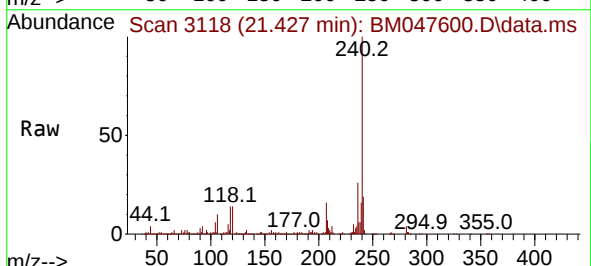



#79

Terphenyl-d14

Concen: 127.158 ng

RT: 19.821 min Scan# 21

Delta R.T. -0.006 min

Lab File: BM047600.D

Acq: 23 Sep 2024 11:04

Instrument :

BNA_M

ClientSampleId :

PB163344BL





Tgt Ion:244 Resp: 4365635

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0

122 13.1 10.0 15.0

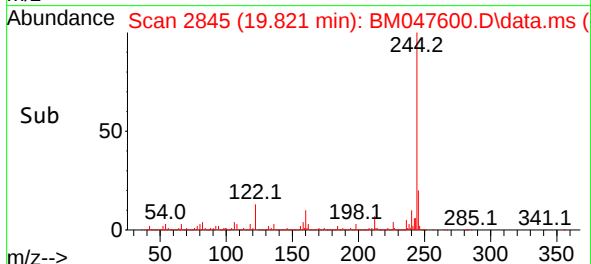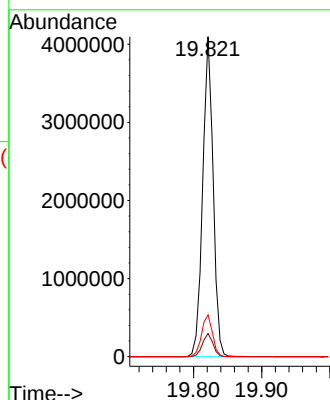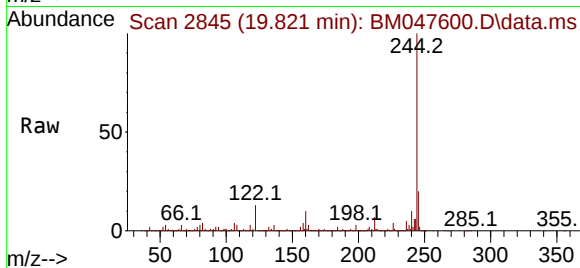

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.450 min Scan# 3632

Delta R.T. -0.012 min

Lab File: BM047600.D

Acq: 23 Sep 2024 11:04

Tgt Ion:264 Resp: 584879

Ion Ratio Lower Upper

264 100

260 23.2 18.9 28.3

265 21.5 17.0 25.6

