
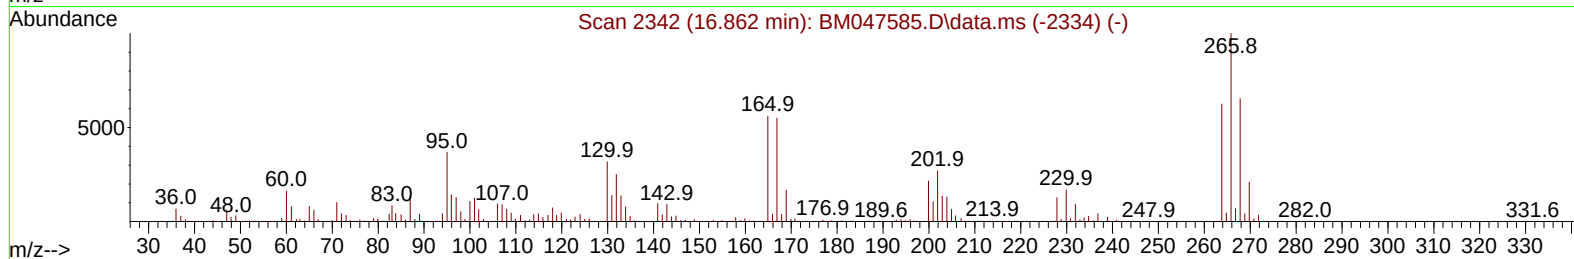
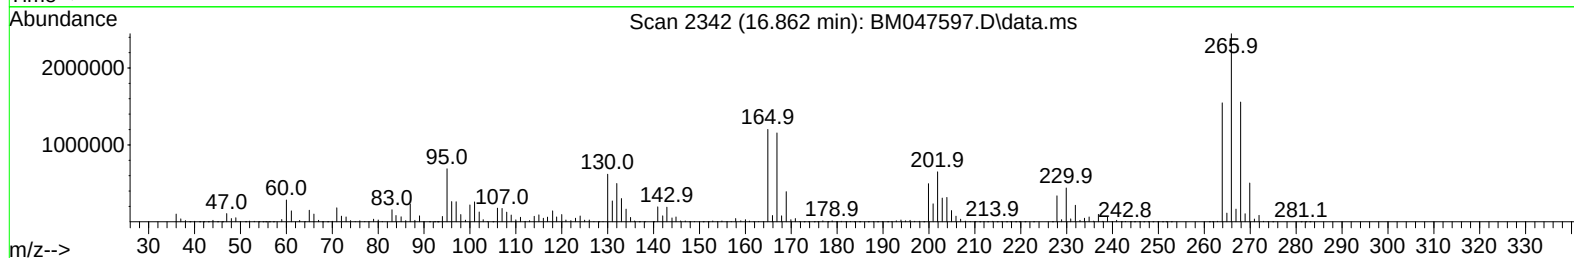


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM092324\  
Data File : BM047597.D  
Acq On : 23 Sep 2024 08:47  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 11:22:52 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM092024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Sep 21 02:22:39 2024  
Response via : Initial Calibration

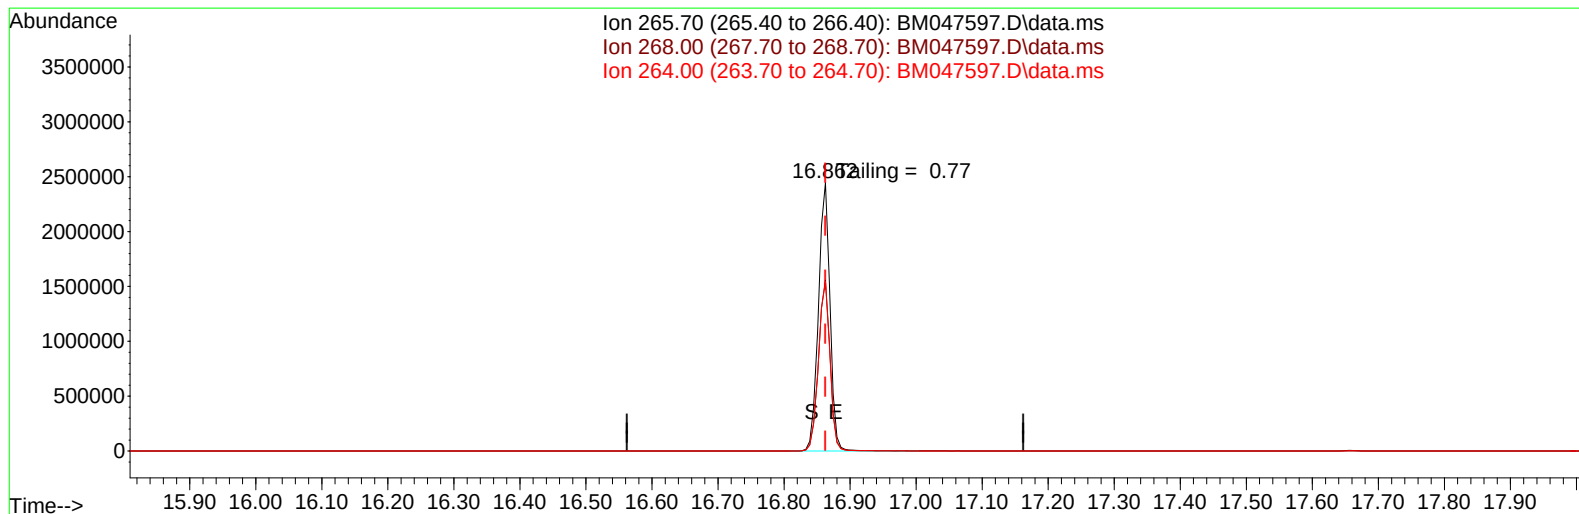

TIC: BM047597.D\data.ms

**(70) Pentachlorophenol (C)**




16.862min (+ 0.000) 0.00 ng

response 2968340

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.30  | 63.68  |
| 264.00 | 62.50  | 63.20  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM092324\  
Data File : BM047597.D  
Acq On : 23 Sep 2024 08:47  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 11:22:52 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM092024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Sep 21 02:22:39 2024  
Response via : Initial Calibration

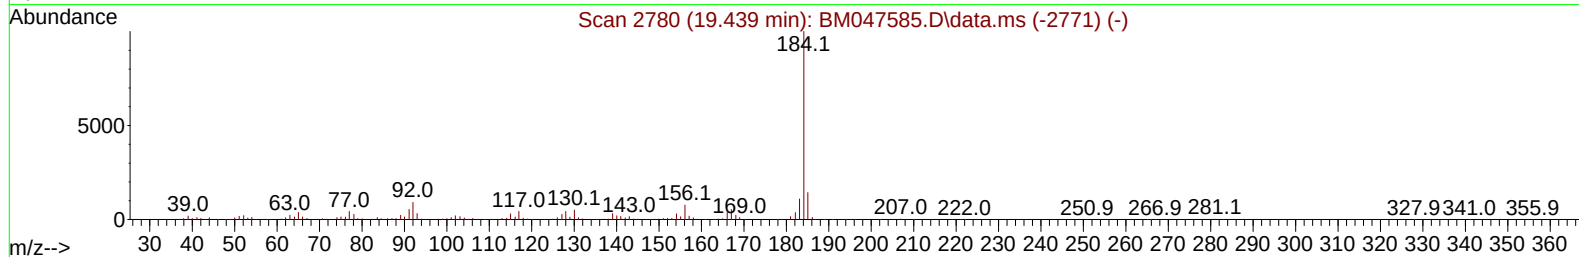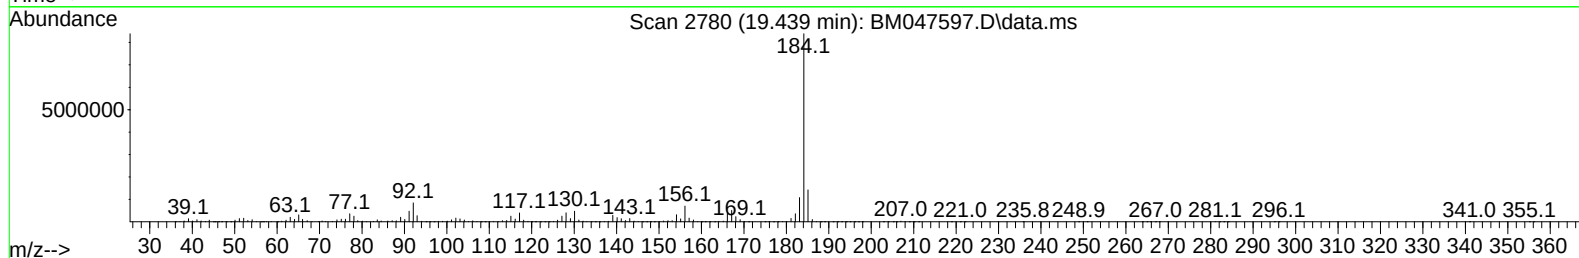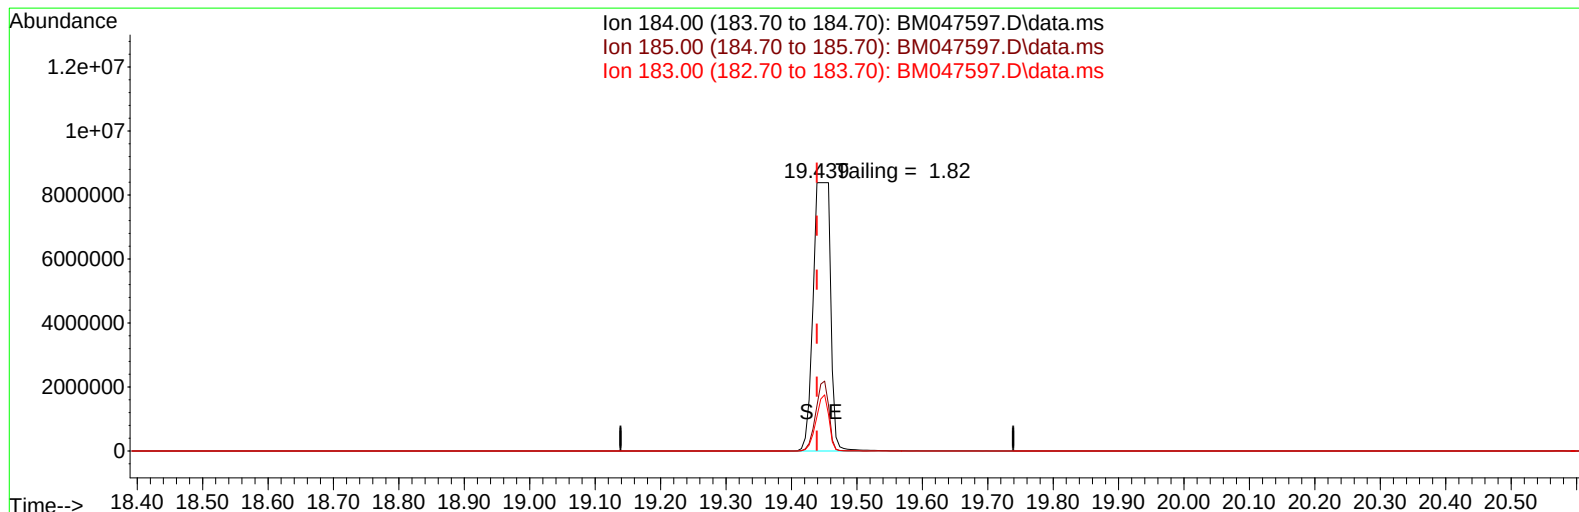

TIC: BM047597.D\data.ms

**(77) Benzidine****19.439min (-0.000) 2994134.77 ng****response 15453930**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.40  | 16.91  |
| 183.00 | 10.90  | 12.85  |
| 0.00   | 0.00   | 0.00   |