


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092419\
 Data File : BM022749.D
 Acq On : 24 Sep 2019 14:35
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM092019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 20 16:34:01 2019

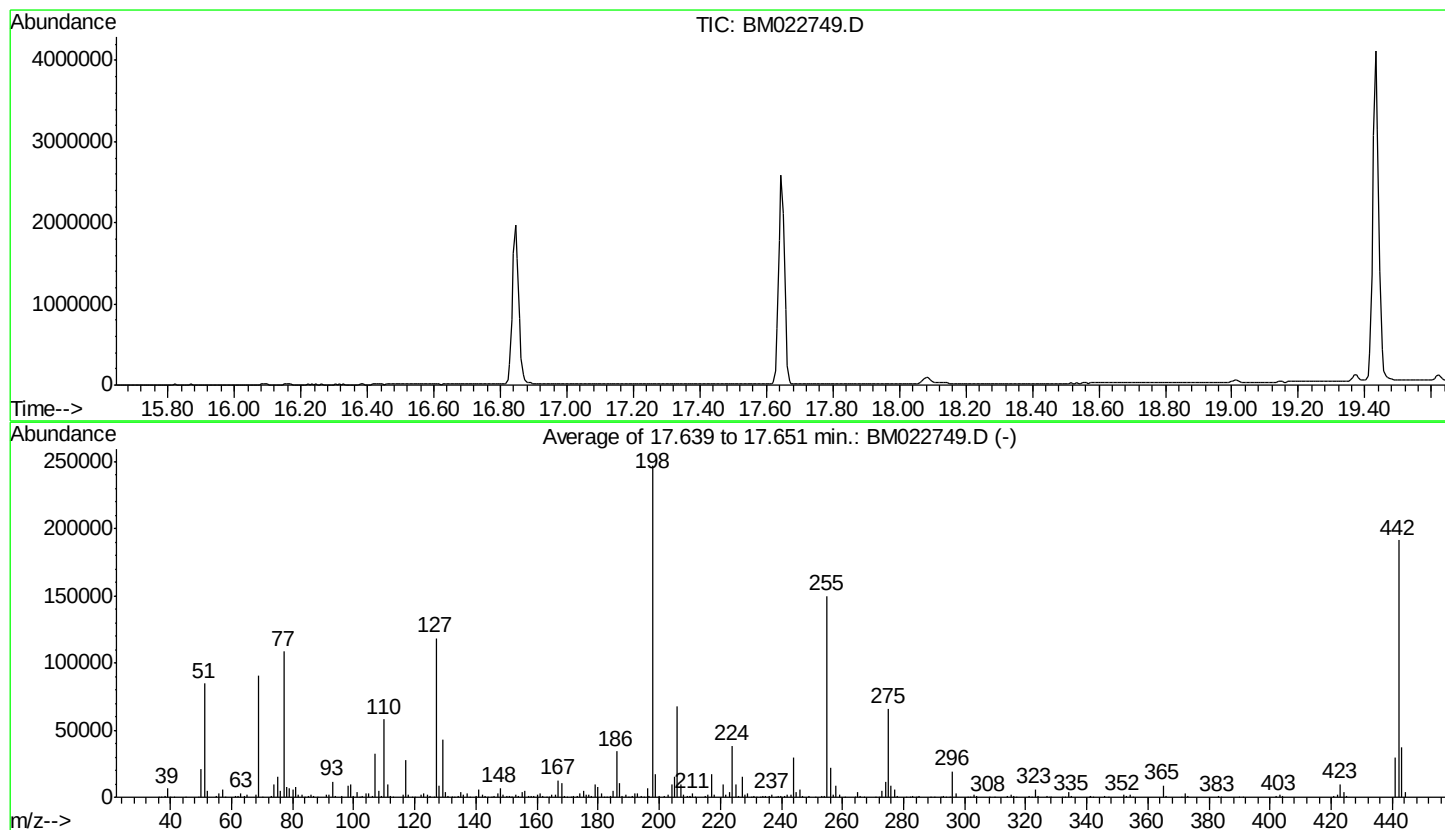

AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	84394	PASS
68	69	0.00	2	1.8	1606	PASS
69	198	0.00	100	36.8	90909	PASS
70	69	0.00	2	0.5	498	PASS
127	198	10	80	48.0	118466	PASS
197	198	0.00	2	0.3	666	PASS
198	198	100	100	100.0	246784	PASS
199	198	5	9	6.8	16893	PASS
275	198	10	60	26.8	66064	PASS
365	198	1	100	3.7	9073	PASS
441	198	0.01	100	11.8	29208	PASS
442	198	50	100	77.4	191120	PASS
443	442	15	24	19.4	36989	PASS