

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092519\
 Data File : BM022774.D
 Acq On : 25 Sep 2019 16:40
 Operator : JU
 Sample : PB123298BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB123298BL

Quant Time: Sep 26 06:01:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM092019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 20 16:34:01 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	214338	20.00	ng	-0.01
21) Naphthalene-d8	10.61	136	798867	20.00	ng	-0.01
39) Acenaphthene-d10	14.45	164	458269	20.00	ng	-0.01
64) Phenanthrene-d10	17.19	188	889022	20.00	ng	0.00
76) Chrysene-d12	21.37	240	812099	20.00	ng	-0.01
87) Perylene-d12	23.64	264	890880	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	1353840	100.18	ng	0.00
7) Phenol-d6	6.99	99	1830323	105.45	ng	0.00
23) Nitrobenzene-d5	8.97	82	1038640	72.17	ng	-0.01
42) 2,4,6-Tribromophenol	15.94	330	692705	121.09	ng	0.00
45) 2-Fluorobiphenyl	13.07	172	2579278	77.50	ng	-0.01
79) Terphenyl-d14	19.82	244	3787329	90.31	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.90	163	127623	3.854	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092519\
Data File : BM022774.D
Acq On : 25 Sep 2019 16:40
Operator : JU
Sample : PB123298BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB123298BL

Quant Time: Sep 26 06:01:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM092019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:34:01 2019
Response via : Initial Calibration

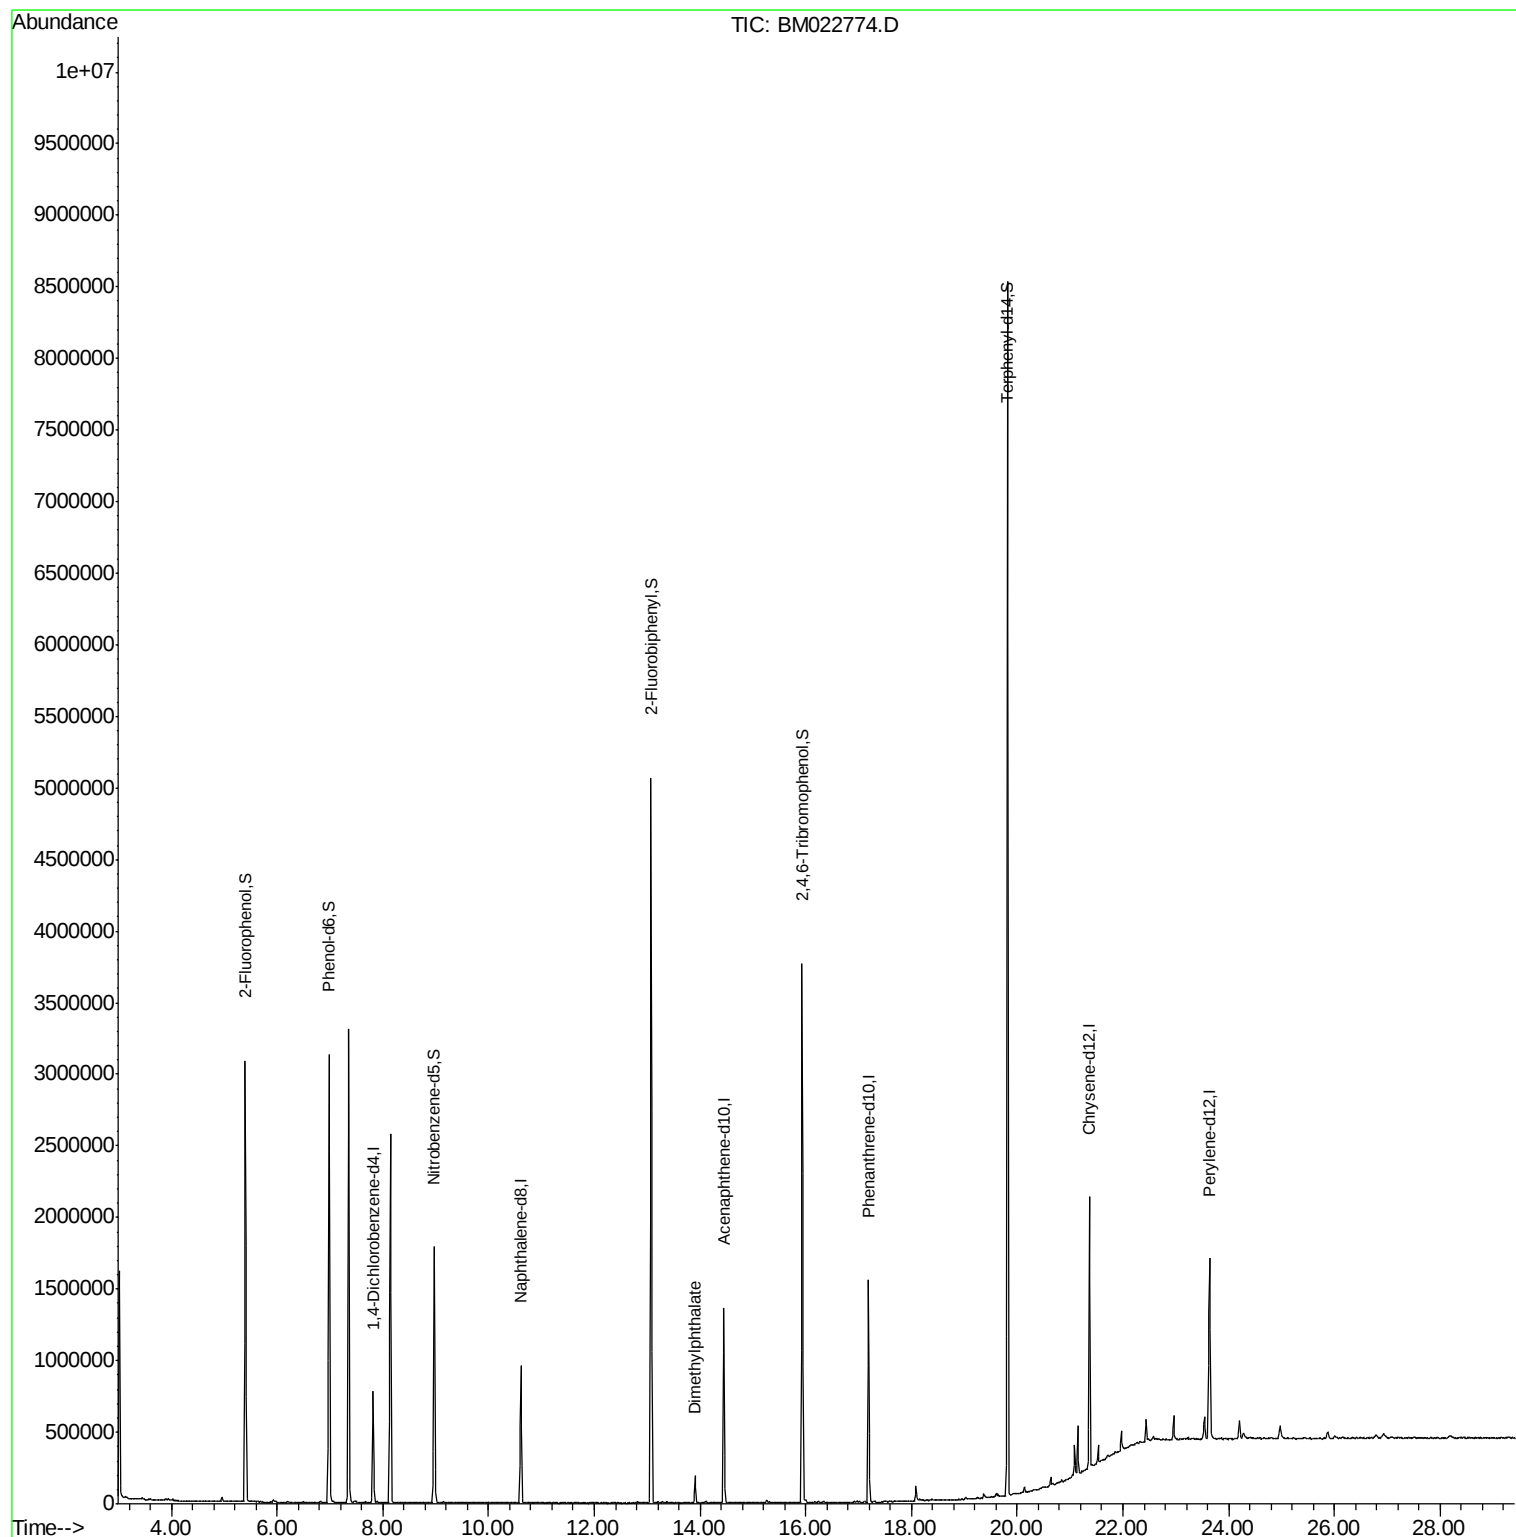

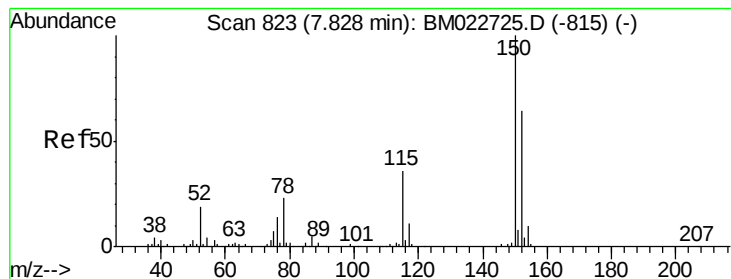


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.82 min Scan# 821
Delta R.T. -0.01 min
Lab File: BM022774.D
Acq: 25 Sep 2019 16:40

Instrument :
BNA_M
ClientSampleId :
PB123298BL

Tot Ion	152	Resp	214338
Ion	Ratio	Lower	Upper
152	100		
150	156.3	124.5	186.7
115	56.7	45.0	67.4



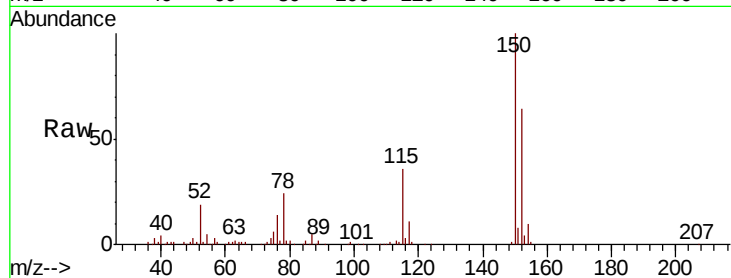


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

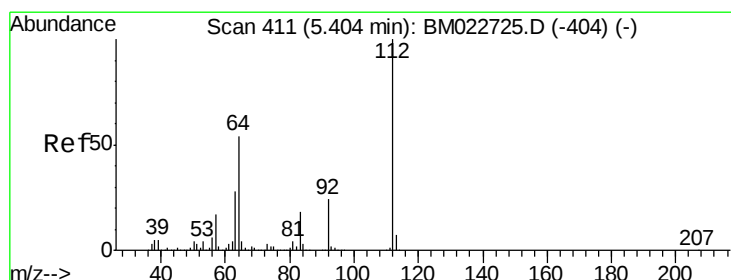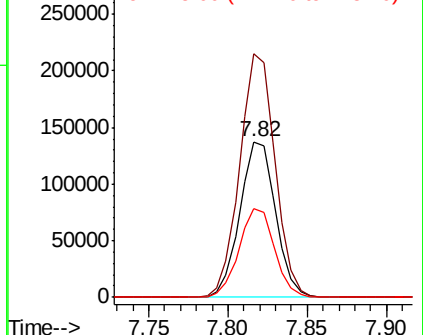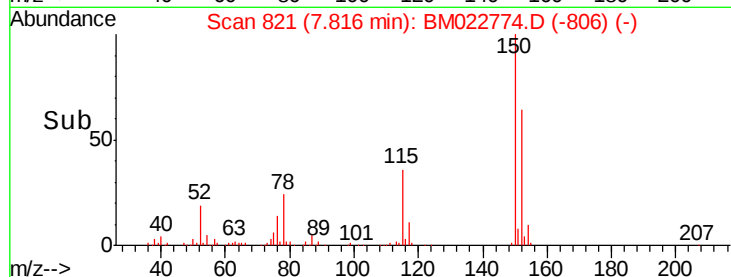

#5

2-Fluorophenol
Concen: 100.176 ng
RT: 5.40 min Scan# 410
Delta R.T. -0.01 min
Lab File: BM022774.D
Acq: 25 Sep 2019 16:40

Tgt Ion	112	Resp	1353840
Ion	Ratio	Lower	Upper
112	100		
64	55.2	43.4	65.2
63	28.2	22.1	33.1


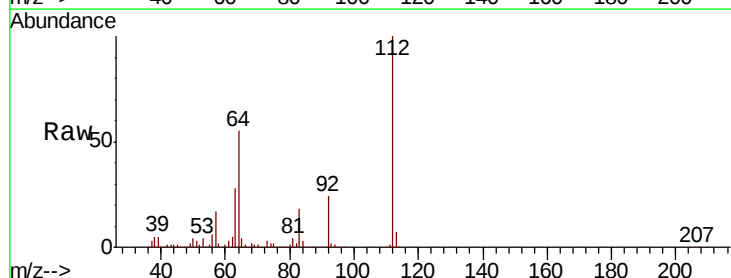



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

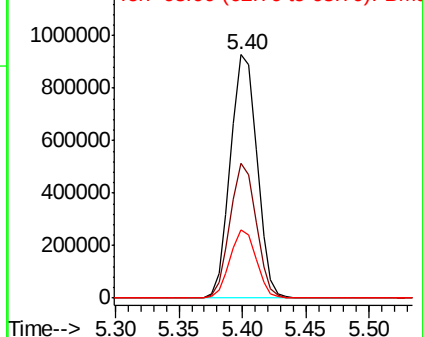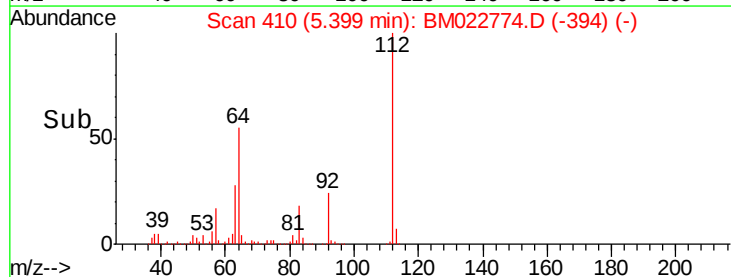

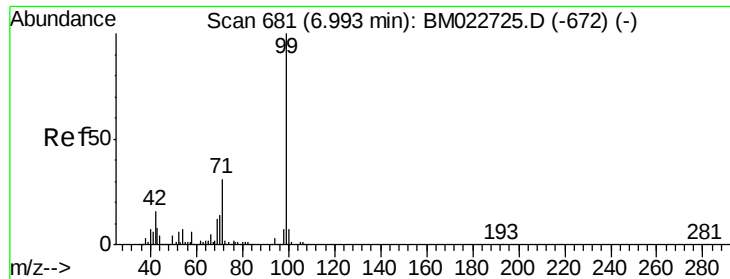

#7

Phenol-d6

Concen: 105.445 ng

RT: 6.99 min Scan# 680

Delta R.T. -0.01 min

Lab File: BM022774.D

Acq: 25 Sep 2019 16:40

Instrument :

BNA_M

ClientSampleId :

PB123298BL


Tot Ion: 99 Resp: 1830323

Ion Ratio Lower Upper

99 100

42 16.2 13.0 19.4

71 31.3 24.7 37.1

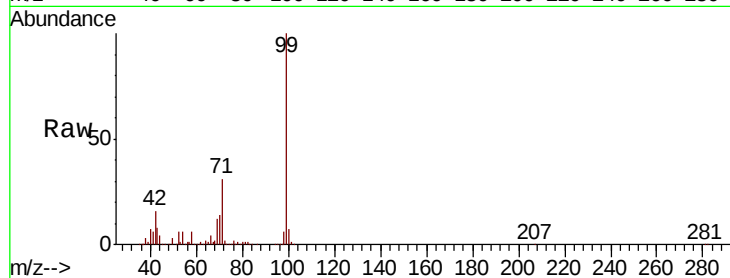


Abundance Ion 99.00 (98.70 to 99.70): BM022774.D (-664) (-)


Ion 42.00 (41.70 to 42.70): BM022774.D (-664) (-)

Ion 71.00 (70.70 to 71.70): BM022774.D (-664) (-)

Time-->

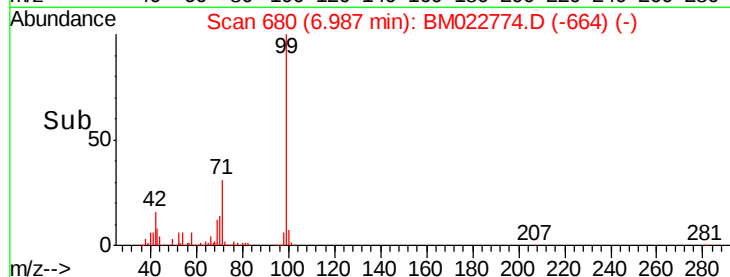

Time-->

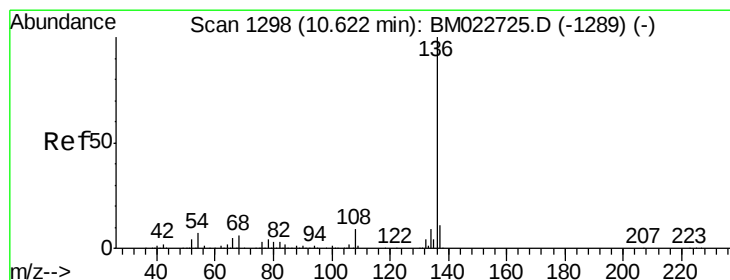

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.61 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BM022774.D

Acq: 25 Sep 2019 16:40

Tgt Ion: 136 Resp: 798867


Ion Ratio Lower Upper

136 100

137 11.0 8.6 13.0

54 7.4 6.0 9.0

68 6.0 4.9 7.3

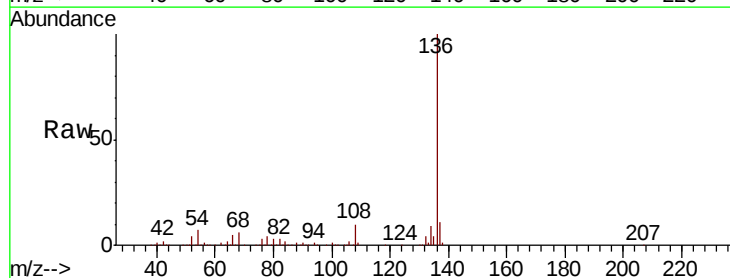


Abundance Ion 136.00 (135.70 to 136.70): BM022774.D (-1281) (-)

Ion 137.00 (136.70 to 137.70): BM022774.D (-1281) (-)


Ion 54.00 (53.70 to 54.70): BM022774.D (-1281) (-)

Ion 68.00 (67.70 to 68.70): BM022774.D (-1281) (-)

Time-->

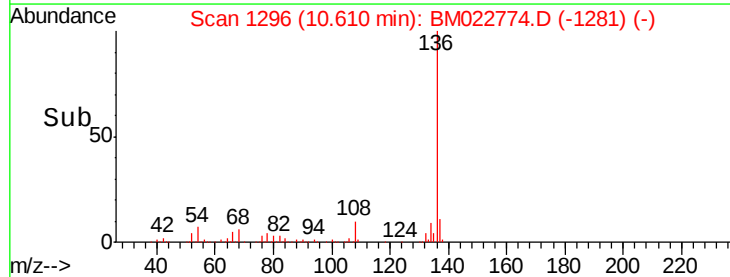





Time-->

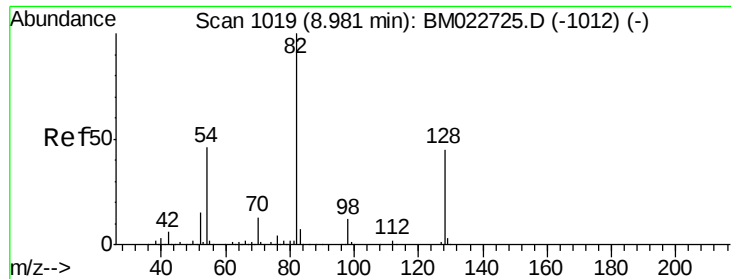

#23
 Nitrobenzene-d5
 Concen: 72.171 ng
 RT: 8.97 min Scan# 1017
 Delta R.T. -0.01 min
 Lab File: BM022774.D
 Acq: 25 Sep 2019 16:40




Instrument :
 BNA_M
 ClientSampleId :
 PB123298BL


Tot Ion: 82 Resp: 1038640
 Ion Ratio Lower Upper
 82 100
 128 44.3 36.0 54.0
 54 46.9 37.1 55.7

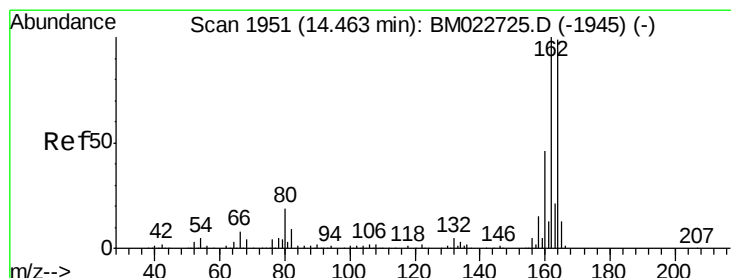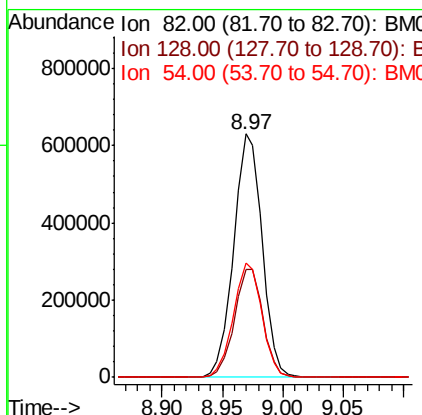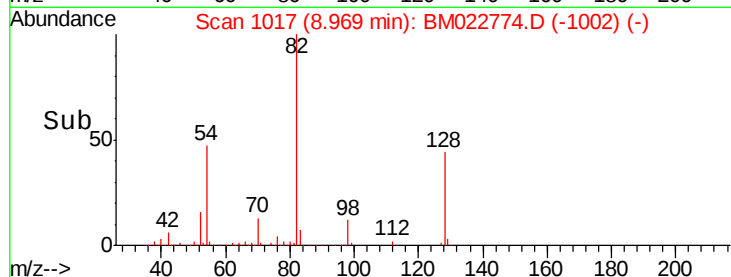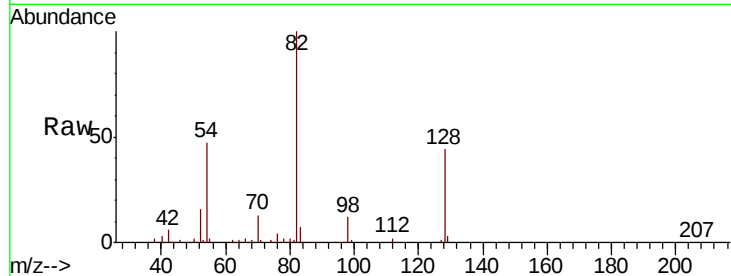

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.45 min Scan# 1949
 Delta R.T. -0.01 min
 Lab File: BM022774.D
 Acq: 25 Sep 2019 16:40

Tgt Ion: 164 Resp: 458269
 Ion Ratio Lower Upper
 164 100
 162 101.3 81.1 121.7
 160 46.4 36.9 55.3

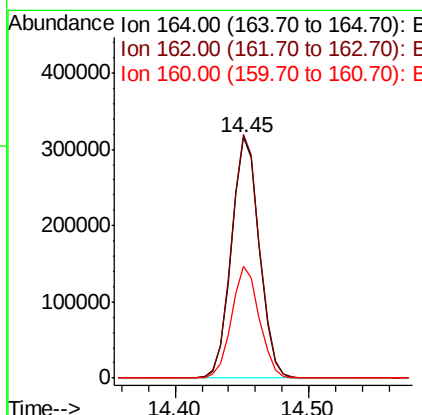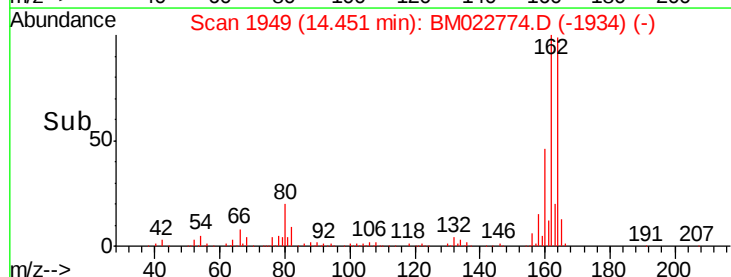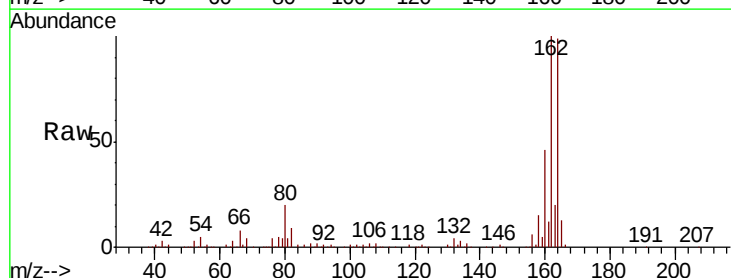

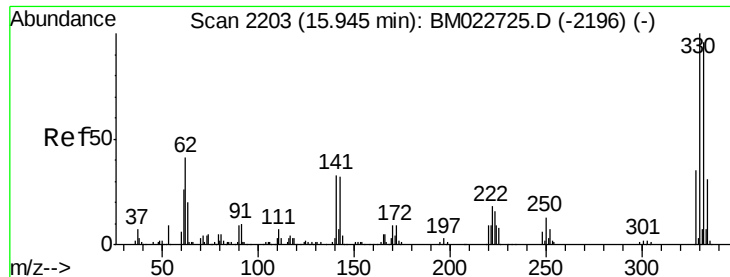

#42

2,4,6-Tribromophenol

Concen: 121.086 ng

RT: 15.94 min Scan# 2202

Delta R.T. -0.01 min

Lab File: BM022774.D

Acq: 25 Sep 2019 16:40

Instrument :

BNA_M

ClientSampleId :

PB123298BL


Tot Ion:330 Resp: 692705

Ion Ratio Lower Upper




330 100

332 96.1 76.9 115.3

141 34.6 28.6 42.8

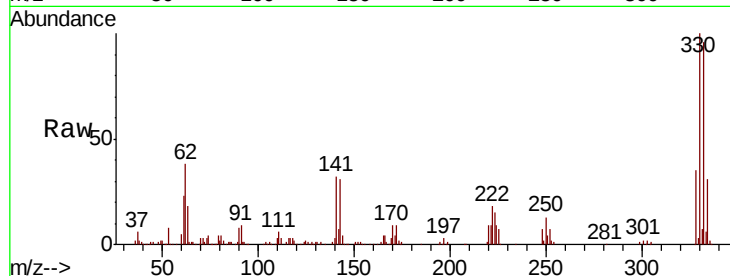

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

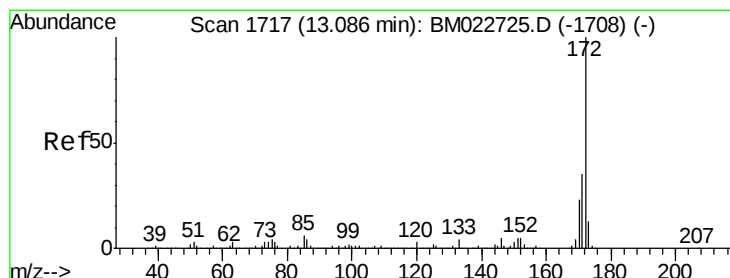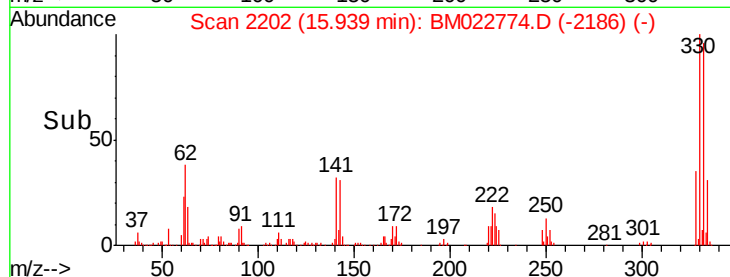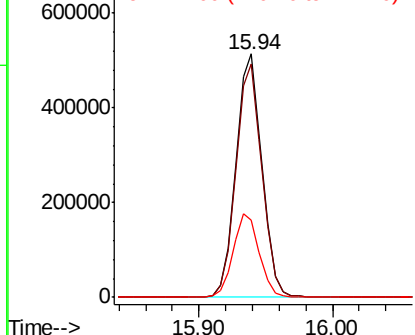

#45

2-Fluorobiphenyl

Concen: 77.504 ng

RT: 13.07 min Scan# 1715

Delta R.T. -0.01 min

Lab File: BM022774.D

Acq: 25 Sep 2019 16:40


Tgt Ion:172 Resp: 2579278

Ion Ratio Lower Upper



172 100


171 35.3 27.8 41.8

170 23.3 18.7 28.1

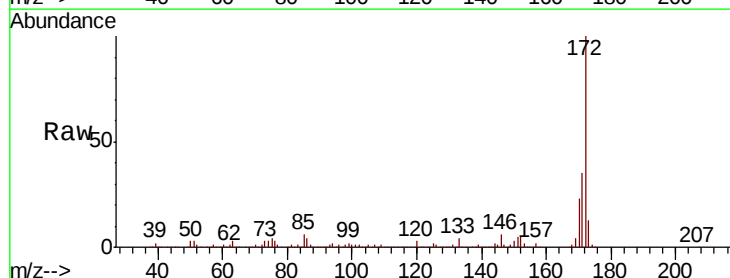

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

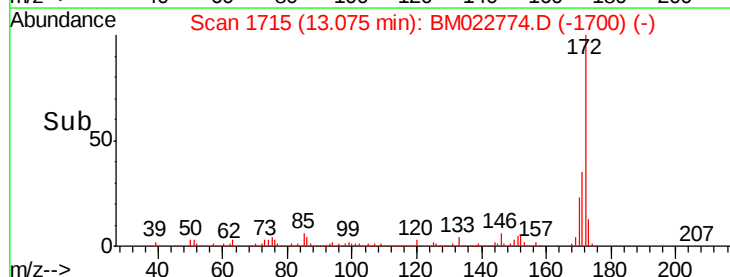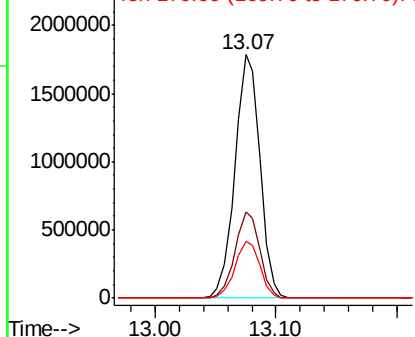

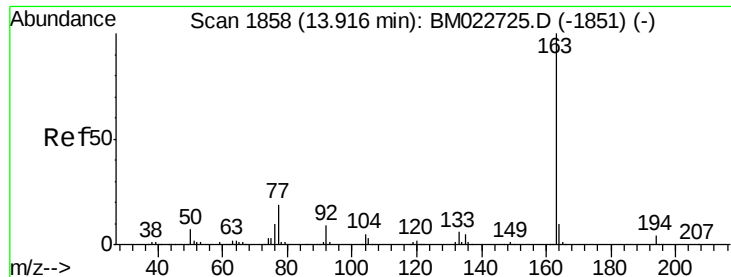

#50

Dimethylphthalate

Concen: 3.854 ng

RT: 13.90 min Scan# 1856

Delta R.T. -0.01 min

Lab File: BM022774.D

Acq: 25 Sep 2019 16:40

Instrument :

BNA_M

ClientSampleId :

PB123298BL


Tot Ion:163 Resp: 127623

Ion Ratio Lower Upper

163 100

194 4.0 3.3 4.9




164 10.7 8.2 12.2

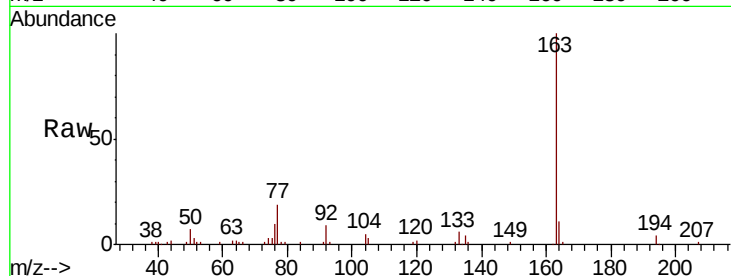

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

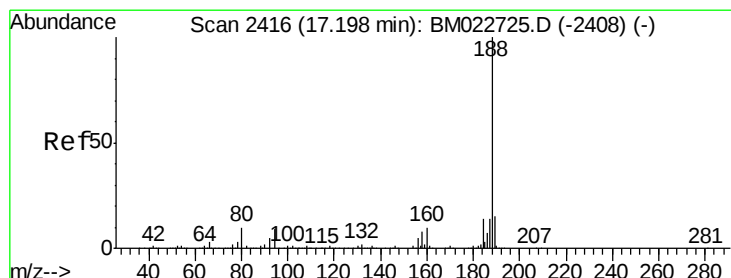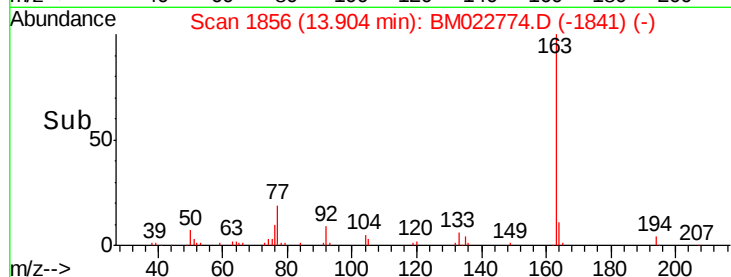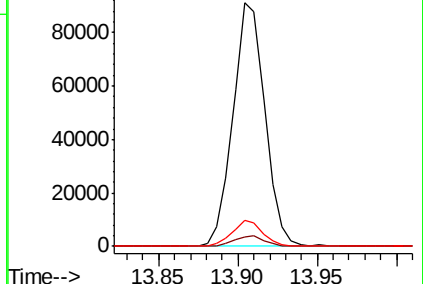

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.19 min Scan# 2415

Delta R.T. -0.01 min

Lab File: BM022774.D

Acq: 25 Sep 2019 16:40


Tgt Ion:188 Resp: 889022

Ion Ratio Lower Upper

188 100

94 8.8 7.3 10.9



80 9.8 7.8 11.8

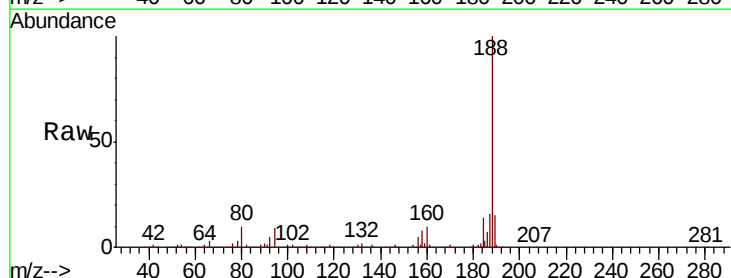


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM



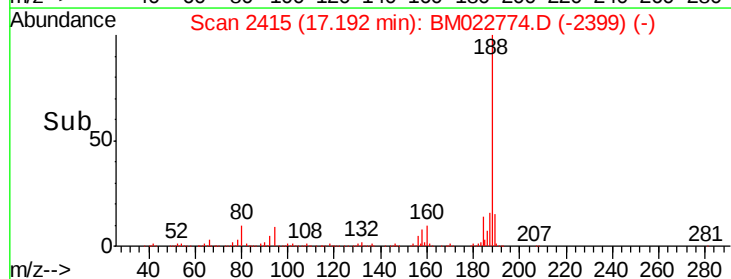
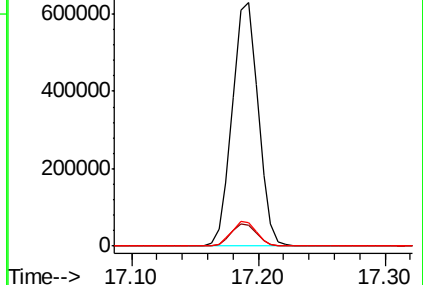


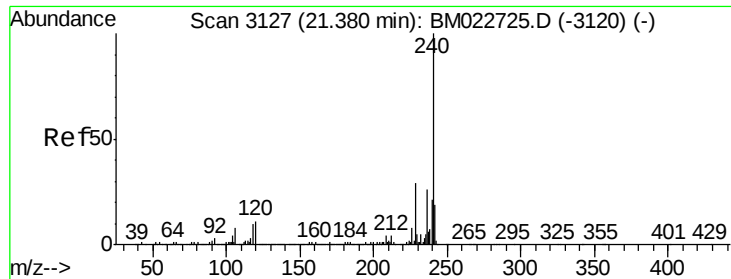

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.37 min Scan# 3125
 Delta R.T. -0.01 min
 Lab File: BM022774.D
 Acq: 25 Sep 2019 16:40




Instrument :
 BNA_M
 ClientSampleId :
 PB123298BL


Tot Ion	Ratio	Lower	Upper
240	100		
120	10.9	8.8	13.2
236	26.5	20.8	31.2

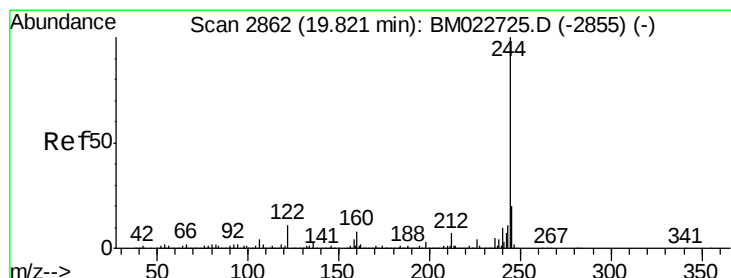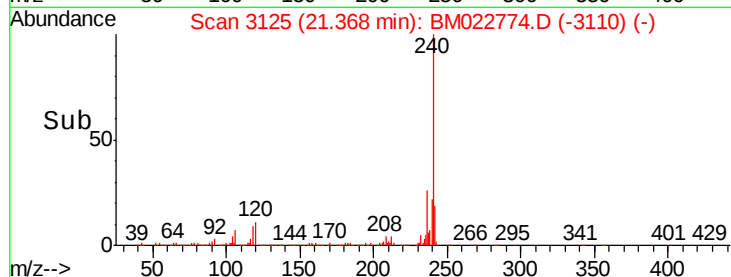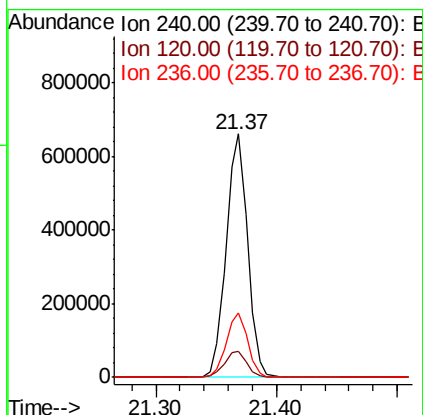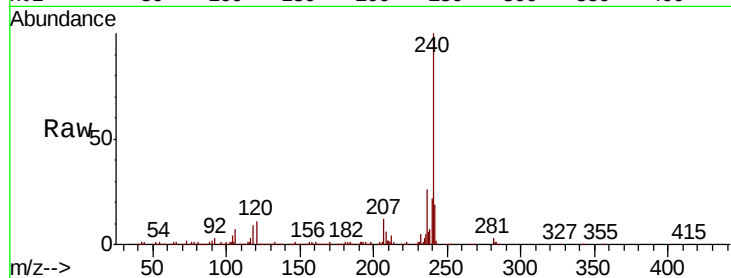

#79
 Terphenyl-d14
 Concen: 90.305 ng
 RT: 19.82 min Scan# 2861
 Delta R.T. -0.01 min
 Lab File: BM022774.D
 Acq: 25 Sep 2019 16:40

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.5	5.9	8.9
122	10.8	9.0	13.4

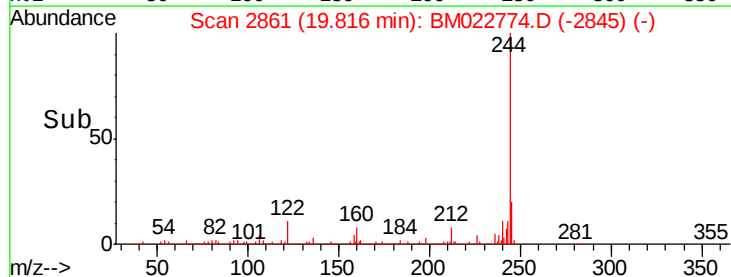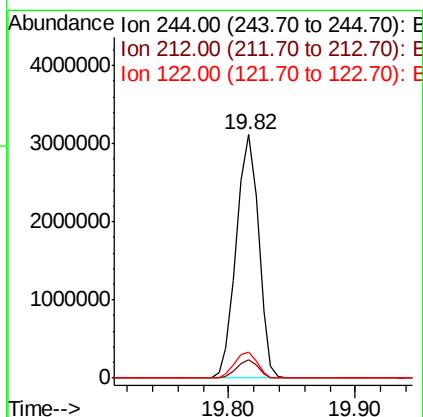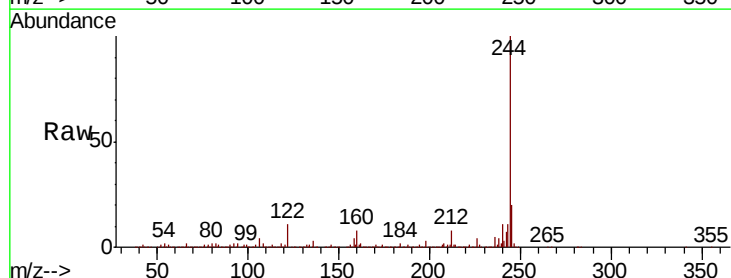

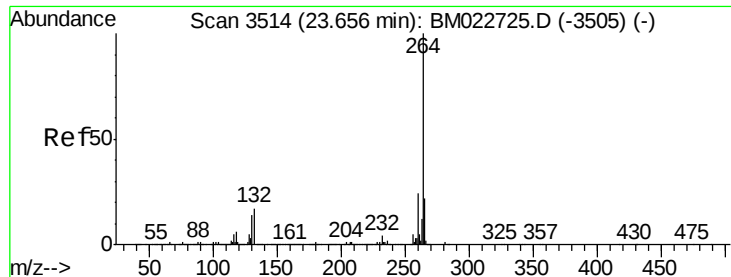

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.64 min Scan# 3511
 Delta R.T. -0.02 min
 Lab File: BM022774.D
 Acq: 25 Sep 2019 16:40

Instrument :
 BNA_M
 ClientSampleId :
 PB123298BL

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.1	28.7
265	22.0	17.9	26.9

